

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040422\
 Data File : FF010247.D
 Signal(s) : FID2B.ch
 Acq On : 04 Apr 2022 11:14
 Operator : AJ\MA
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/05/2022
 Supervised By :mohammad ahmed 04/06/2022

Integration File: autoint1.e
 Quant Time: Apr 05 01:11:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.624	5766328	48.242 ug/mlm
Target Compounds			
2) N-DECANE	4.364	6606336	49.691 ug/ml
3) N-DODECANE	6.382	6610628	49.649 ug/ml
4) N-TETRADECANE	8.175	6602042	49.794 ug/ml
5) N-HEXADECANE	9.776	6598765	49.705 ug/ml
6) N-OCTADECANE	11.218	6779068	49.306 ug/ml
7) N-EICOSANE	12.528	6578214	48.962 ug/ml
8) N-DOCOSANE	13.727	6519339	48.724 ug/ml
10) N-TETRACOSANE	14.830	6520404	48.694 ug/ml
11) N-HEXACOSANE	15.851	6439870	48.552 ug/ml
12) N-OCTACOSANE	16.800	6413642	48.390 ug/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040422\
Data File : FF010247.D
Signal(s) : FID2B.ch
Acq On : 04 Apr 2022 11:14
Operator : AJ\MA
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2022
Supervised By :mohammad ahmed 04/06/2022

Integration File: autoint1.e
Quant Time: Apr 05 01:11:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

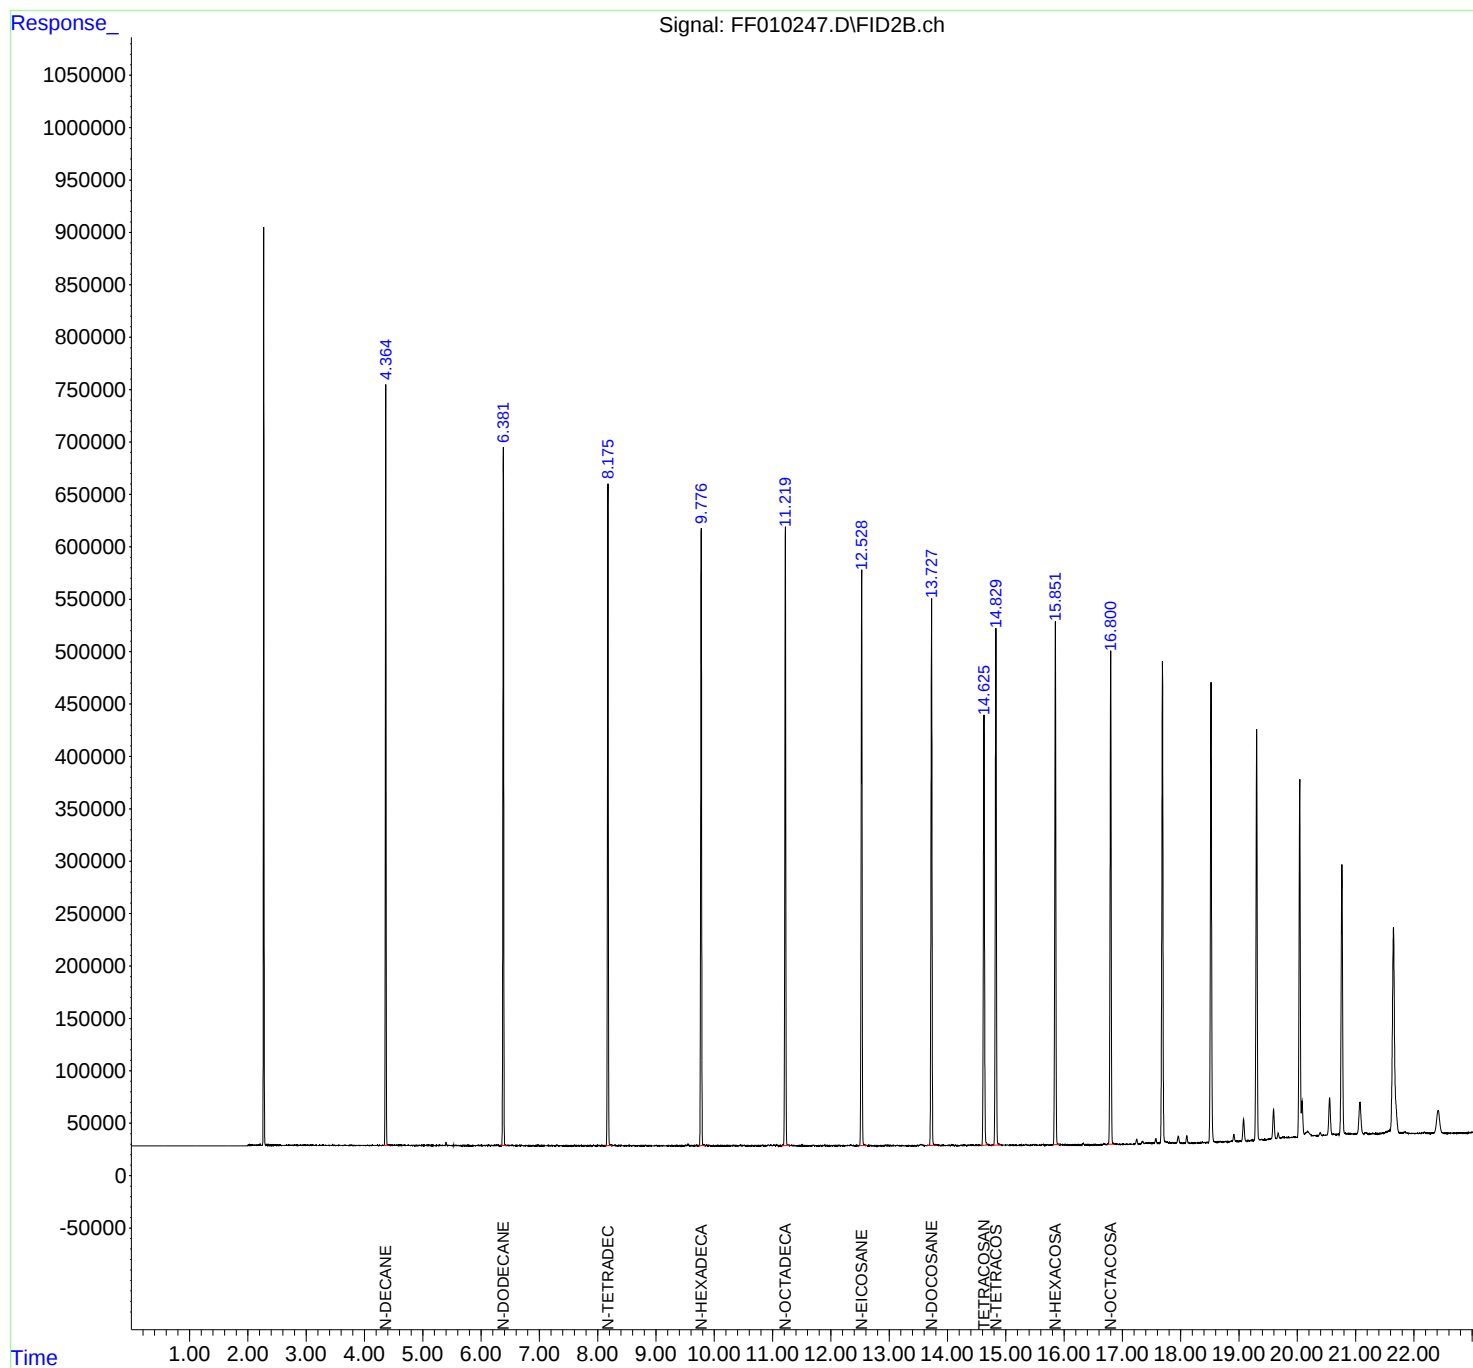

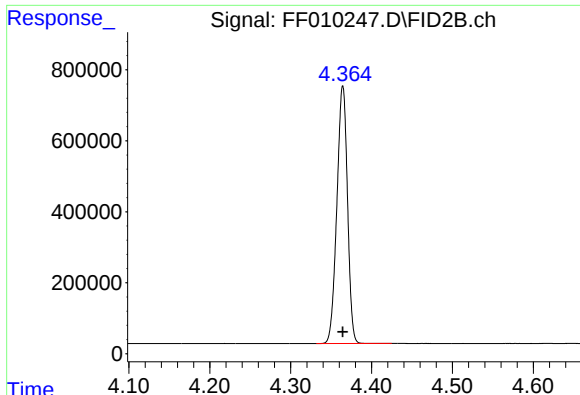


#2 N-DECANE

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 6606336
Conc: 49.69 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2022
Supervised By :mohammad ahmed 04/06/2022

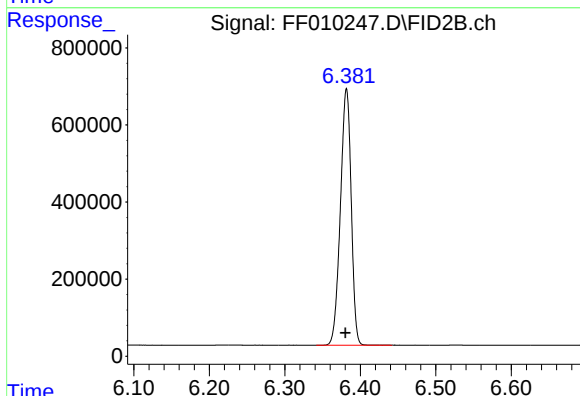


#3 N-DODECANE

R.T.: 6.382 min
Delta R.T.: 0.001 min
Response: 6610628
Conc: 49.65 ug/ml

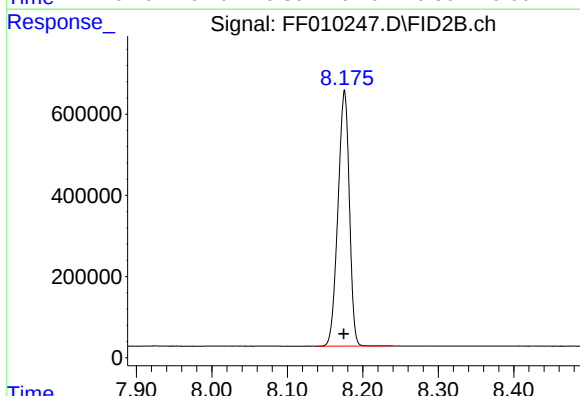


#4 N-TETRADECANE

R.T.: 8.175 min
Delta R.T.: 0.000 min
Response: 6602042
Conc: 49.79 ug/ml

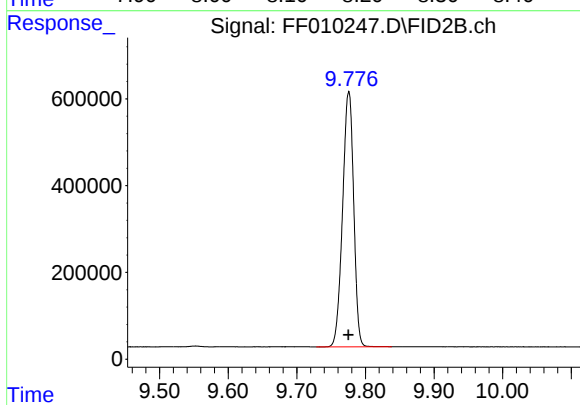

#5 N-HEXADECANE

R.T.: 9.776 min
Delta R.T.: 0.000 min
Response: 6598765
Conc: 49.70 ug/ml

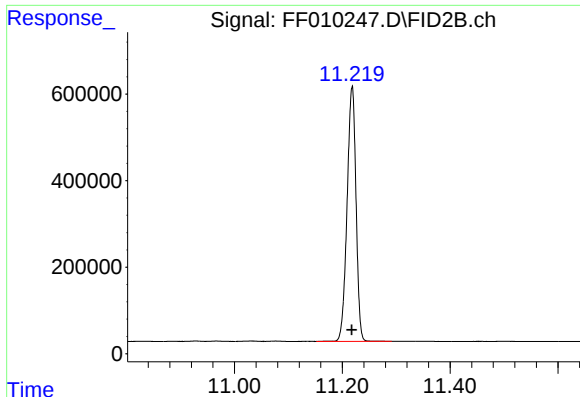


#6 N-OCTADECANE

R.T.: 11.218 min
Delta R.T.: 0.000 min
Response: 6779068
Conc: 49.31 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2022
Supervised By :mohammad ahmed 04/06/2022

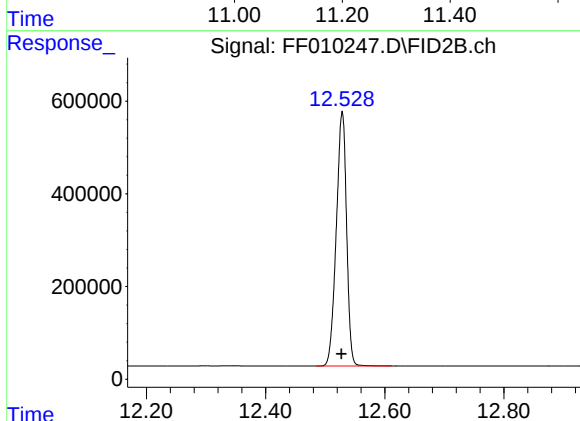


#7 N-EICOSANE

R.T.: 12.528 min
Delta R.T.: 0.001 min
Response: 6578214
Conc: 48.96 ug/ml

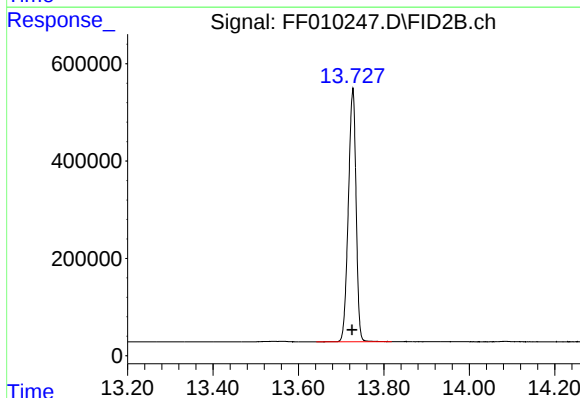


#8 N-DOCOSANE

R.T.: 13.727 min
Delta R.T.: 0.001 min
Response: 6519339
Conc: 48.72 ug/ml

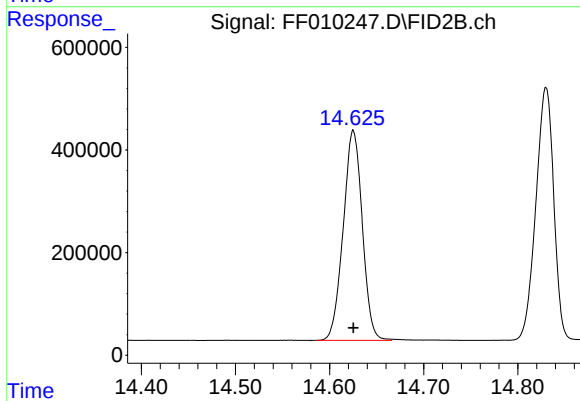

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.624 min
Delta R.T.: 0.000 min
Response: 5766328
Conc: 48.24 ug/ml m

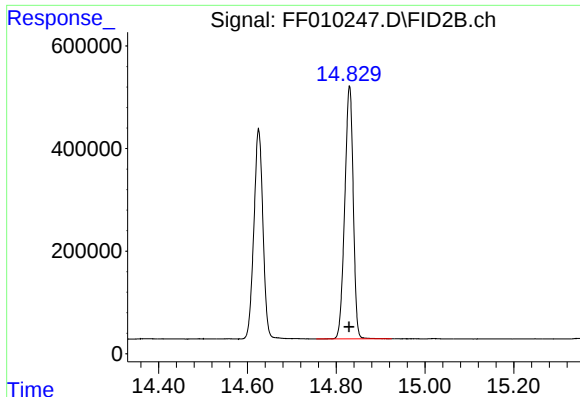


#10 N-TETRACOSANE

R.T.: 14.830 min
Delta R.T.: 0.001 min
Response: 6520404
Conc: 48.69 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2022
Supervised By :mohammad ahmed 04/06/2022

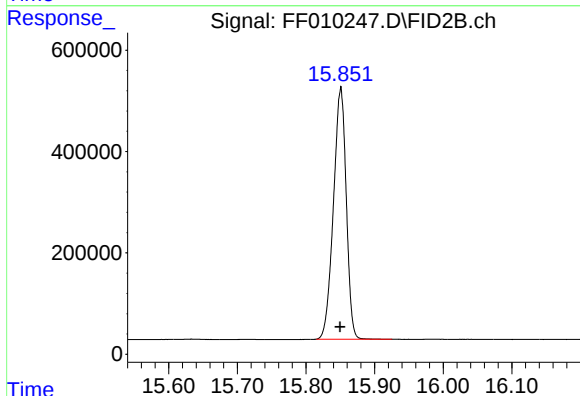

#11 N-HEXACOSANE

R.T.: 15.851 min
Delta R.T.: 0.000 min
Response: 6439870
Conc: 48.55 ug/ml

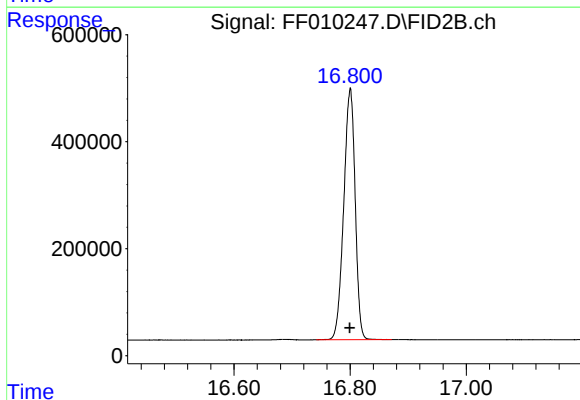

#12 N-OCTACOSANE

R.T.: 16.800 min
Delta R.T.: 0.000 min
Response: 6413642
Conc: 48.39 ug/ml