

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040422\
Data File : FF010255.D
Signal(s) : FID2B.ch
Acq On : 04 Apr 2022 15:46
Operator : AJ\MA
Sample : PB143835BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB143835BL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2022
Supervised By :mohammad ahmed 04/06/2022

Integration File: autoint1.e
Quant Time: Apr 05 01:13:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.623	2128390	17.807 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040422\
Data File : FF010255.D
Signal(s) : FID2B.ch
Acq On : 04 Apr 2022 15:46
Operator : AJ\MA
Sample : PB143835BL
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
PB143835BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2022
Supervised By :mohammad ahmed 04/06/2022

Integration File: autoint1.e
Quant Time: Apr 05 01:13:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

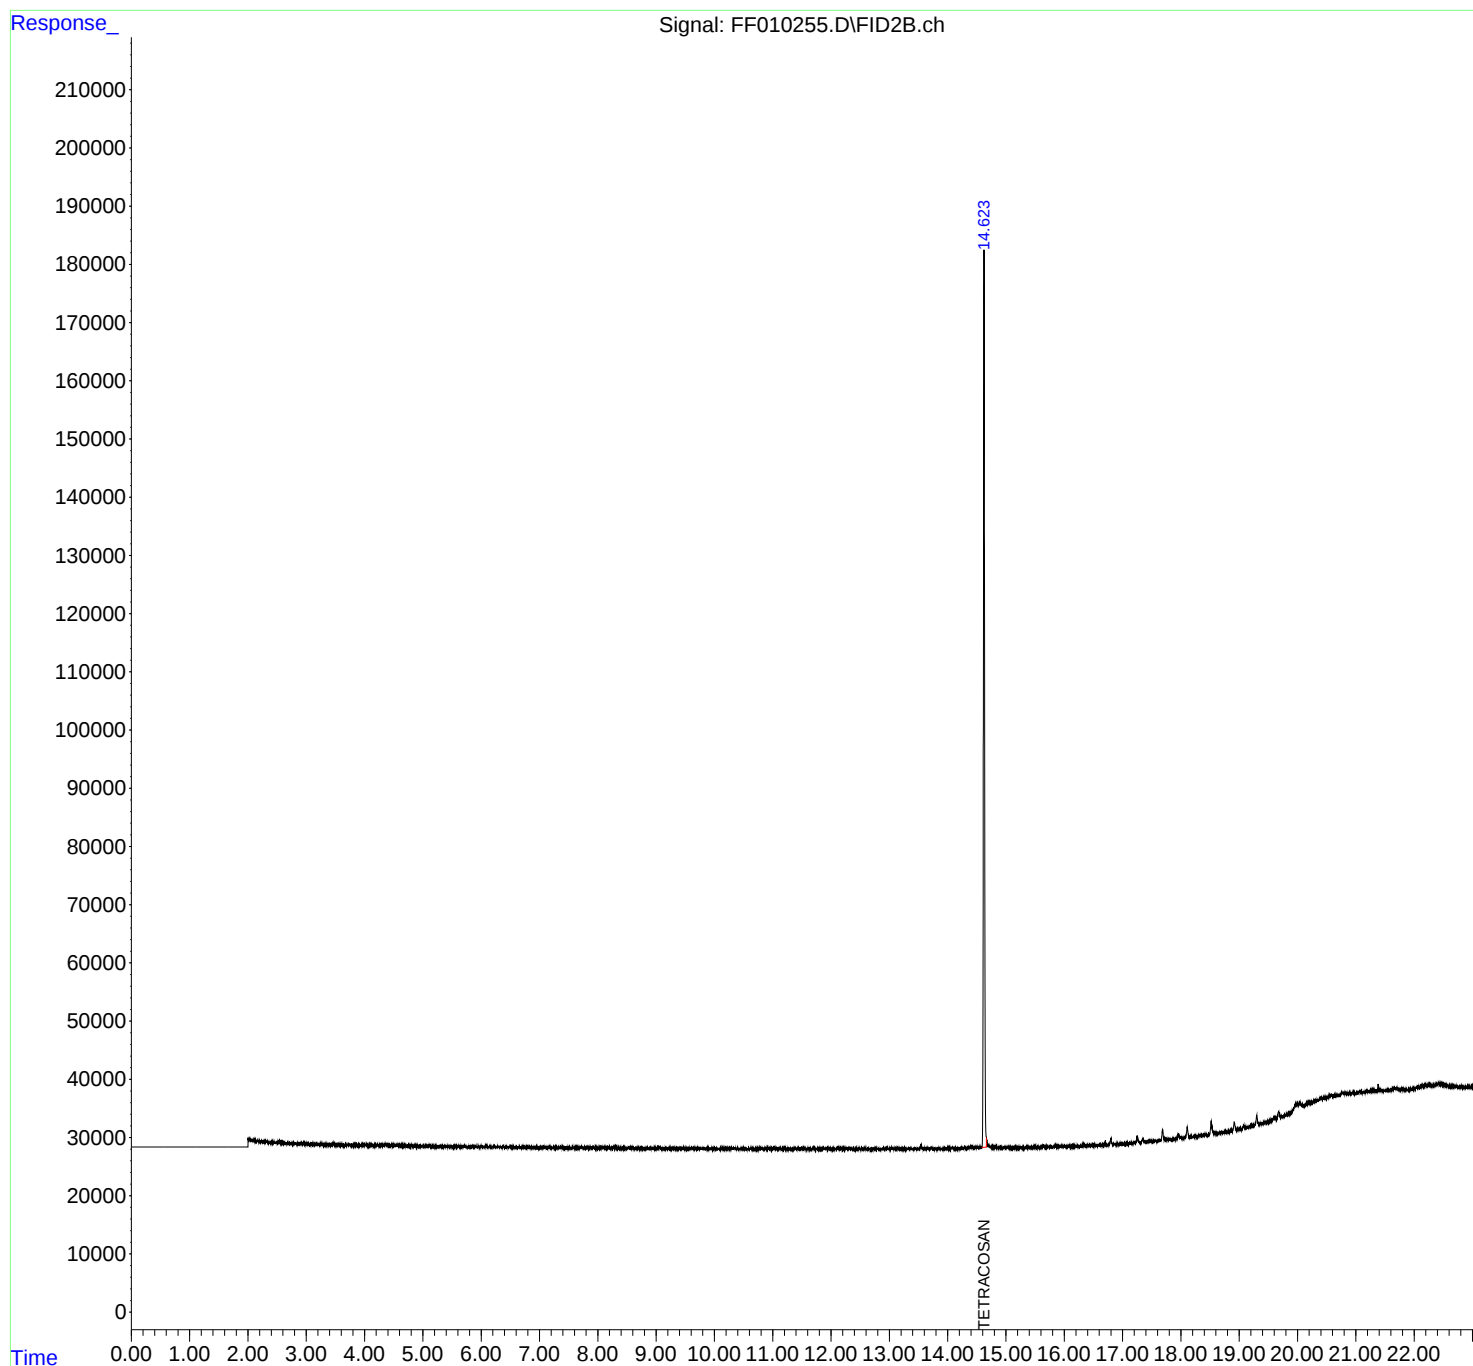

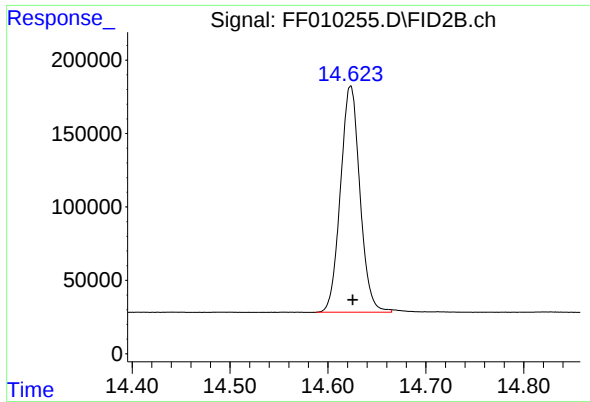

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.623 min
Delta R.T.: -0.002 min
Response: 2128390
Conc: 17.81 ug/ml

Instrument :

FID_F

ClientSampleId :

PB143835BL

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/05/2022

Supervised By :mohammad ahmed 04/06/2022