

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040519\
 Data File : FF004139.D
 Signal(s) : FID2B.ch
 Acq On : 05 Apr 2019 17:23
 Operator : AJ\SJ
 Sample : K2257-17
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 05 23:24:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.539	1811784	13.937 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.161f	671280	4.721 ug/ml
10)	N-TETRACOSANE	14.742	94111	0.639 ug/ml
11)	N-HEXACOSANE	15.763	138797	0.956 ug/ml
12)	N-OCTACOSANE	16.712	199104	1.385 ug/ml
13)	N-TRIACONTANE	17.599	305964	2.142 ug/ml
14)	N-DOTRIACONTANE	18.430	255881	1.813 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040519\
Data File : FF004139.D
Signal(s) : FID2B.ch
Acq On : 05 Apr 2019 17:23
Operator : AJ\SJ
Sample : K2257-17
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 05 23:24:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

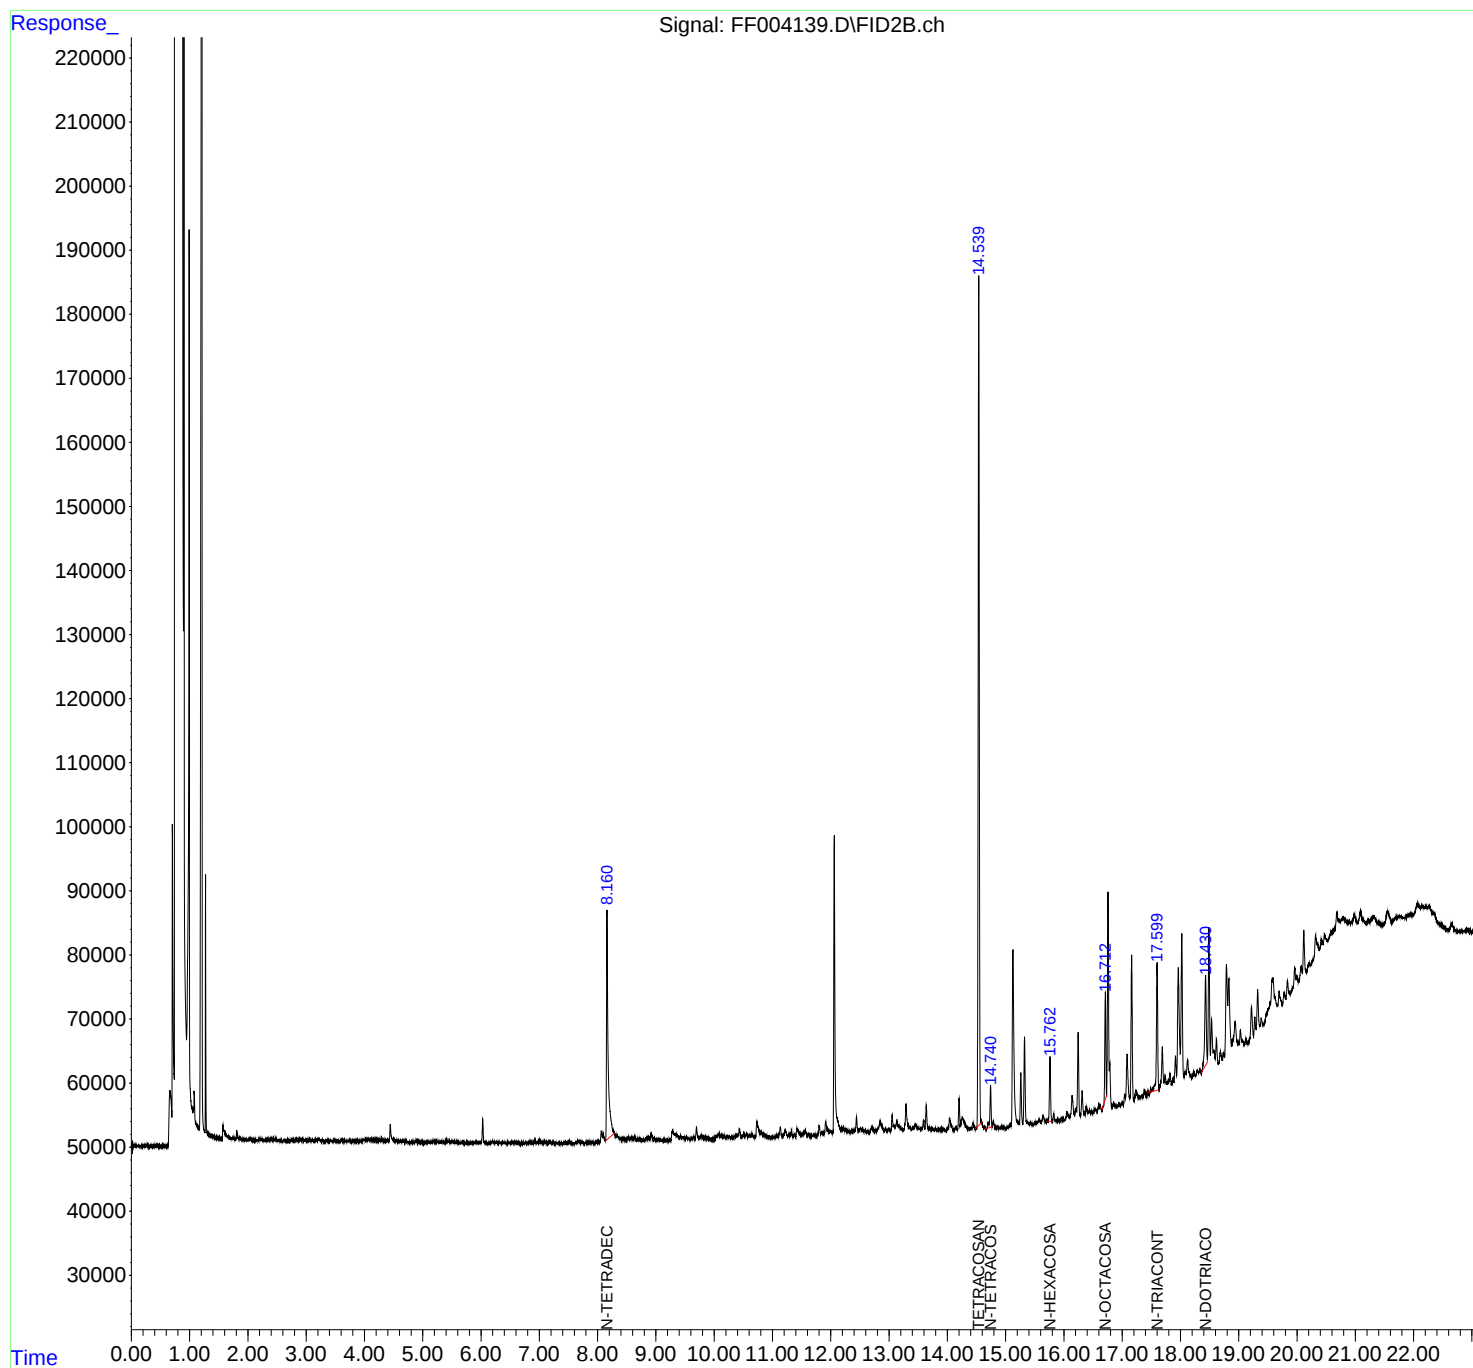

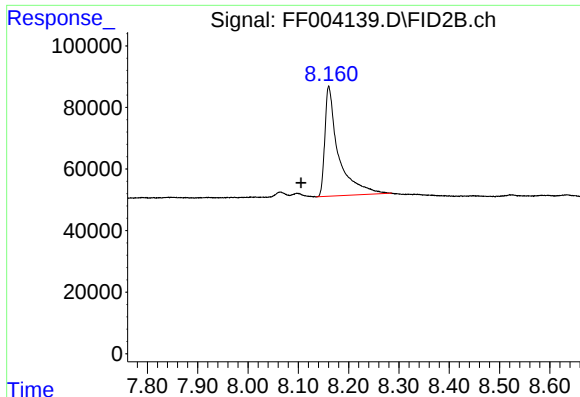


#4 N-TETRADECANE

R.T.: 8.161 min
Delta R.T.: 0.055 min
Response: 671280
Conc: 4.72 ug/ml

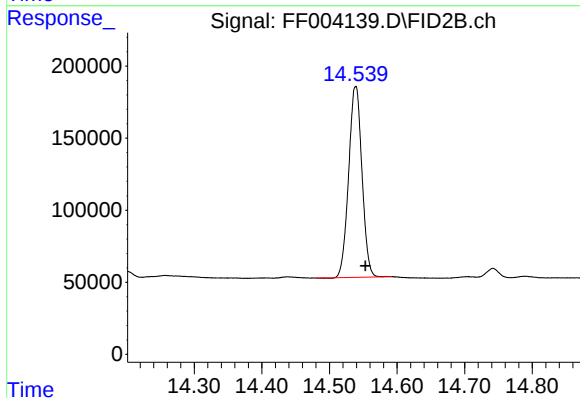


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.539 min
Delta R.T.: -0.015 min
Response: 1811784
Conc: 13.94 ug/ml

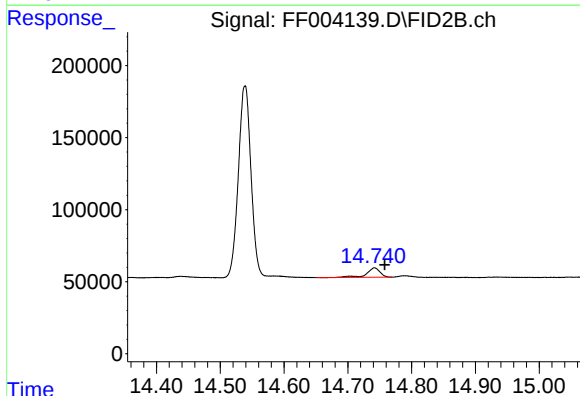


#10 N-TETRACOSANE

R.T.: 14.742 min
Delta R.T.: -0.016 min
Response: 94111
Conc: 0.64 ug/ml

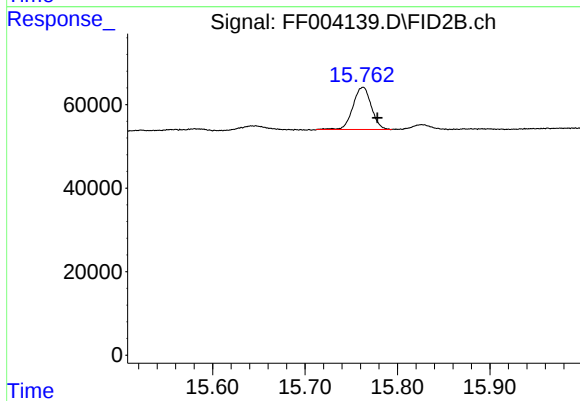


#11 N-HEXACOSANE

R.T.: 15.763 min
Delta R.T.: -0.016 min
Response: 138797
Conc: 0.96 ug/ml

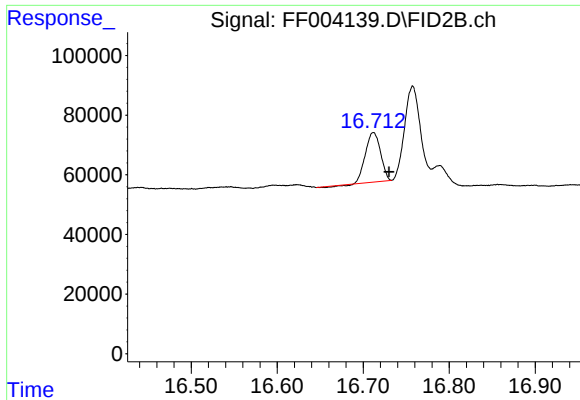


#12 N-OCTACOSANE

R.T.: 16.712 min
Delta R.T.: -0.018 min
Response: 199104
Conc: 1.38 ug/ml

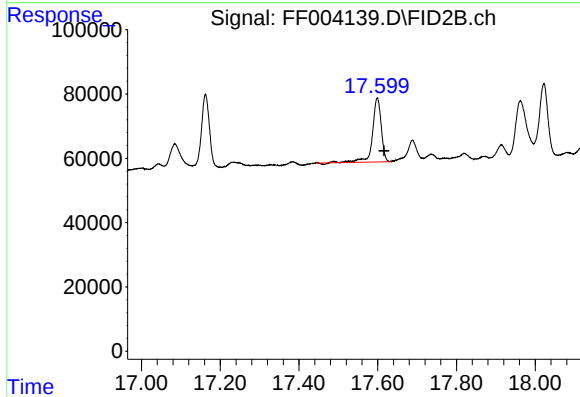

#13 N-TRIACONTANE

R.T.: 17.599 min
Delta R.T.: -0.017 min
Response: 305964
Conc: 2.14 ug/ml

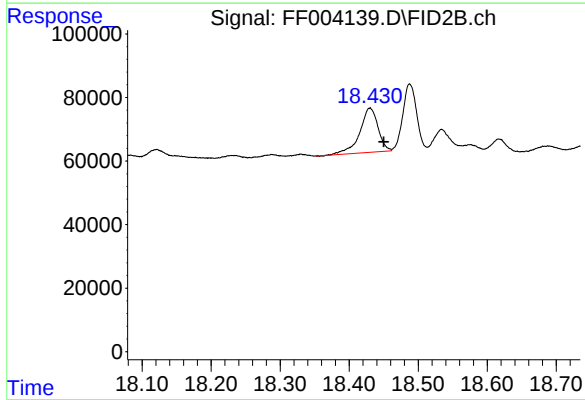

#14 N-DOTRIACONTANE

R.T.: 18.430 min
Delta R.T.: -0.020 min
Response: 255881
Conc: 1.81 ug/ml