

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040522\
Data File : FF010263.D
Signal(s) : FID2B.ch
Acq On : 05 Apr 2022 12:13
Operator : AJ\MA
Sample : N2246-03 500X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 06 02:01:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

1)	N-OCTANE	2.269	93957	0.717 ug/ml
2)	N-DECANE	4.307f	246893	1.857 ug/ml
3)	N-DODECANE	6.391	202634	1.522 ug/ml
5)	N-HEXADECANE	9.725	145064	1.093 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040522\
Data File : FF010263.D
Signal(s) : FID2B.ch
Acq On : 05 Apr 2022 12:13
Operator : AJ\MA
Sample : N2246-03 500X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 06 02:01:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

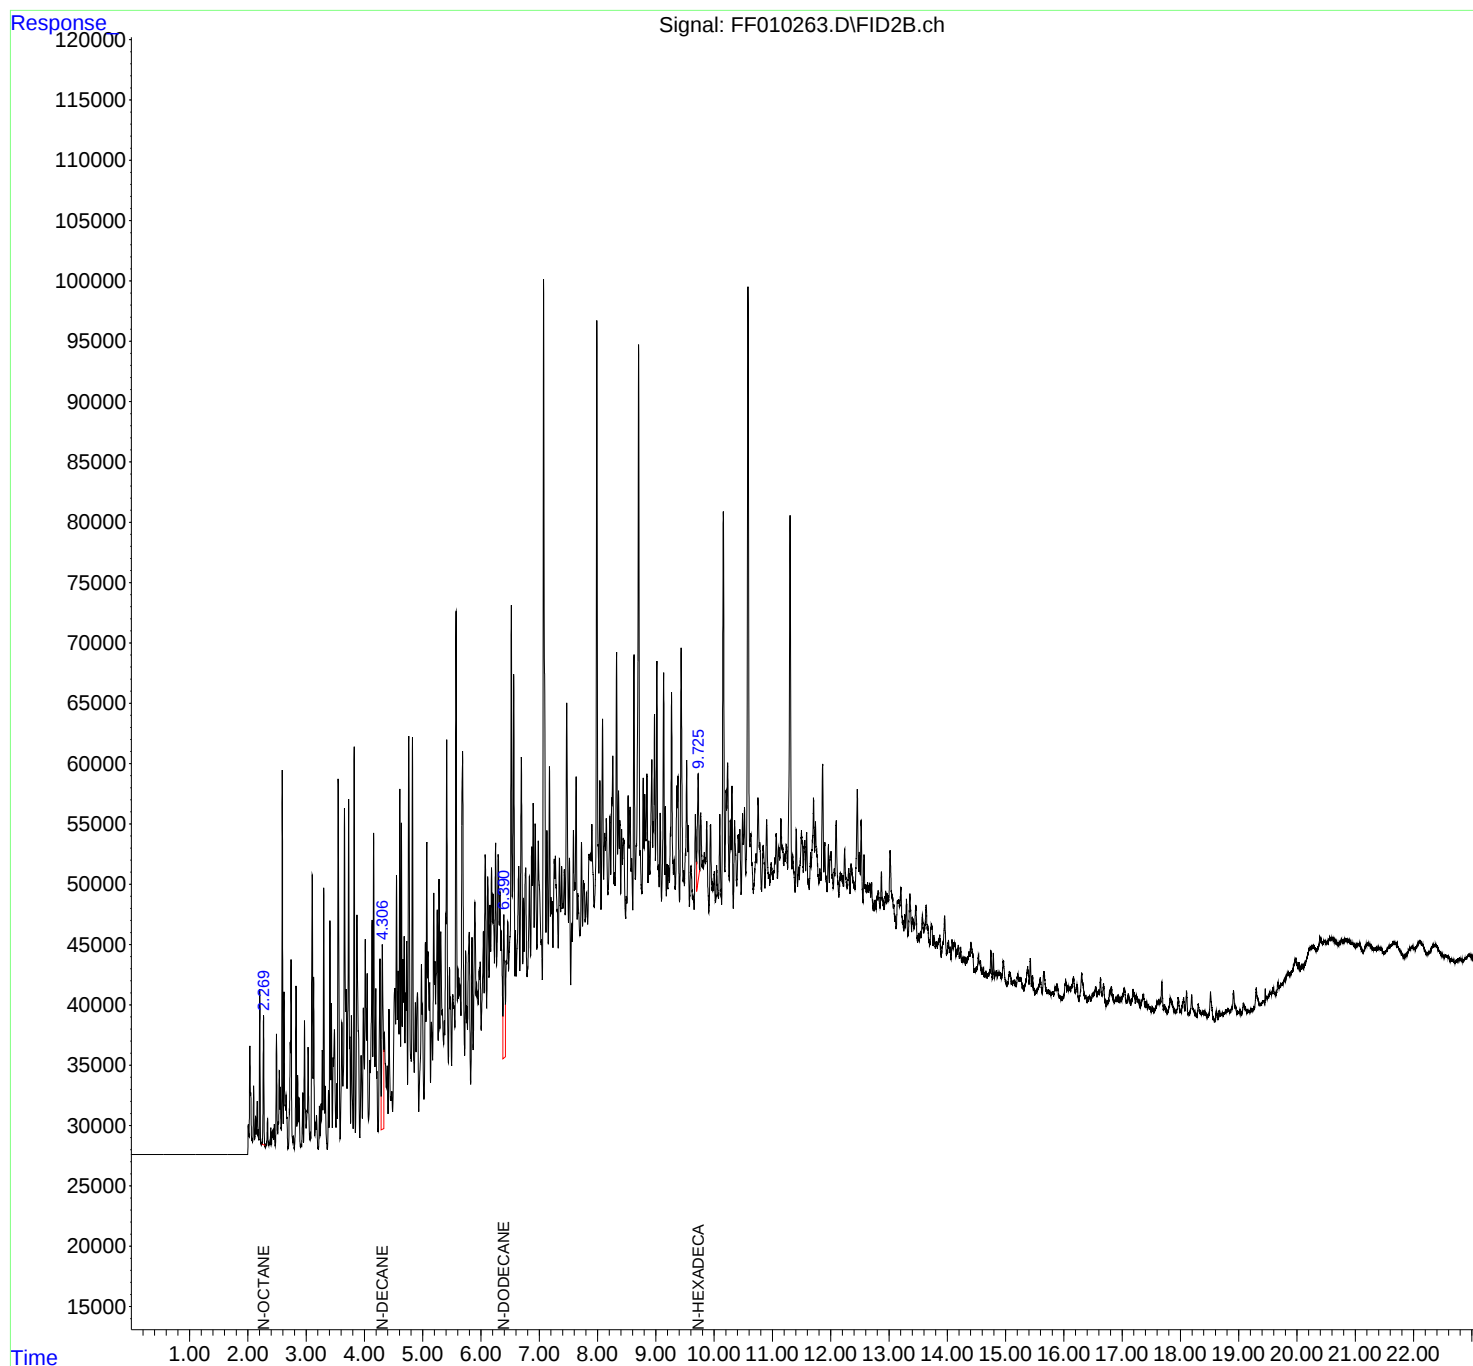


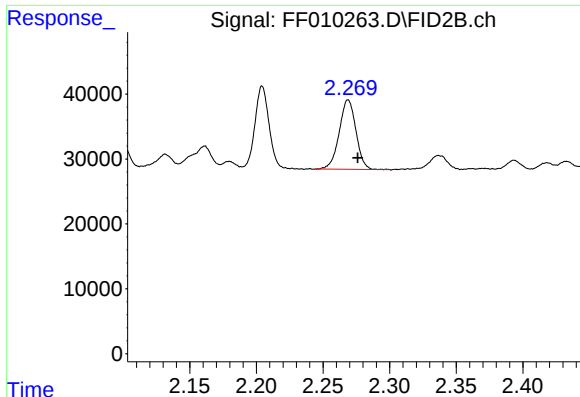

#1 N-OCTANE


R.T.: 2.269 min
Delta R.T.: -0.007 min
Response: 93957
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :

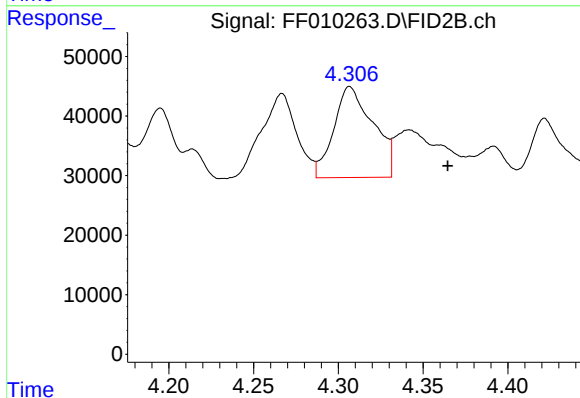


#2 N-DECANE

R.T.: 4.307 min
Delta R.T.: -0.057 min
Response: 246893
Conc: 1.86 ug/ml

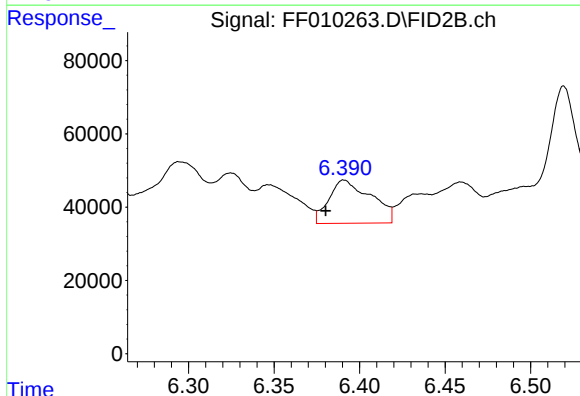


#3 N-DODECANE

R.T.: 6.391 min
Delta R.T.: 0.011 min
Response: 202634
Conc: 1.52 ug/ml

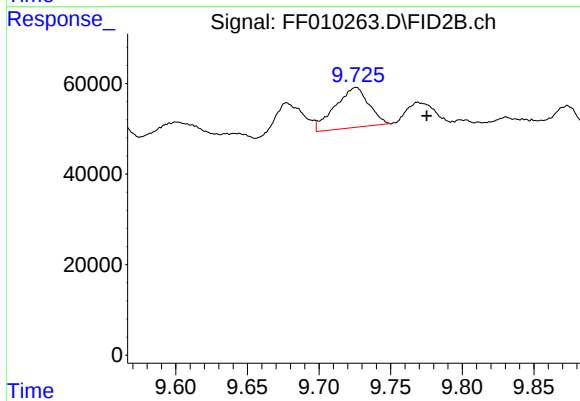

#5 N-HEXADECANE

R.T.: 9.725 min
Delta R.T.: -0.050 min
Response: 145064
Conc: 1.09 ug/ml

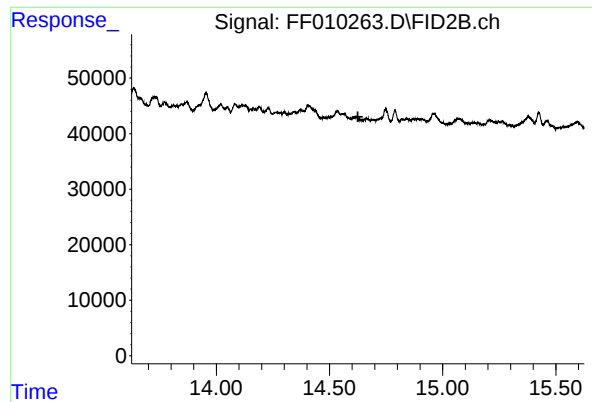

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.625 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :