

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040522\
Data File : FF010262.D
Signal(s) : FID2B.ch
Acq On : 05 Apr 2022 11:03
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Apr 06 02:00:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.376	3894488	29.249 ug/ml
12)	N-OCTACOSANE	16.799	4087119	30.837 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040522\
Data File : FF010262.D
Signal(s) : FID2B.ch
Acq On : 05 Apr 2022 11:03
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Apr 06 02:00:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

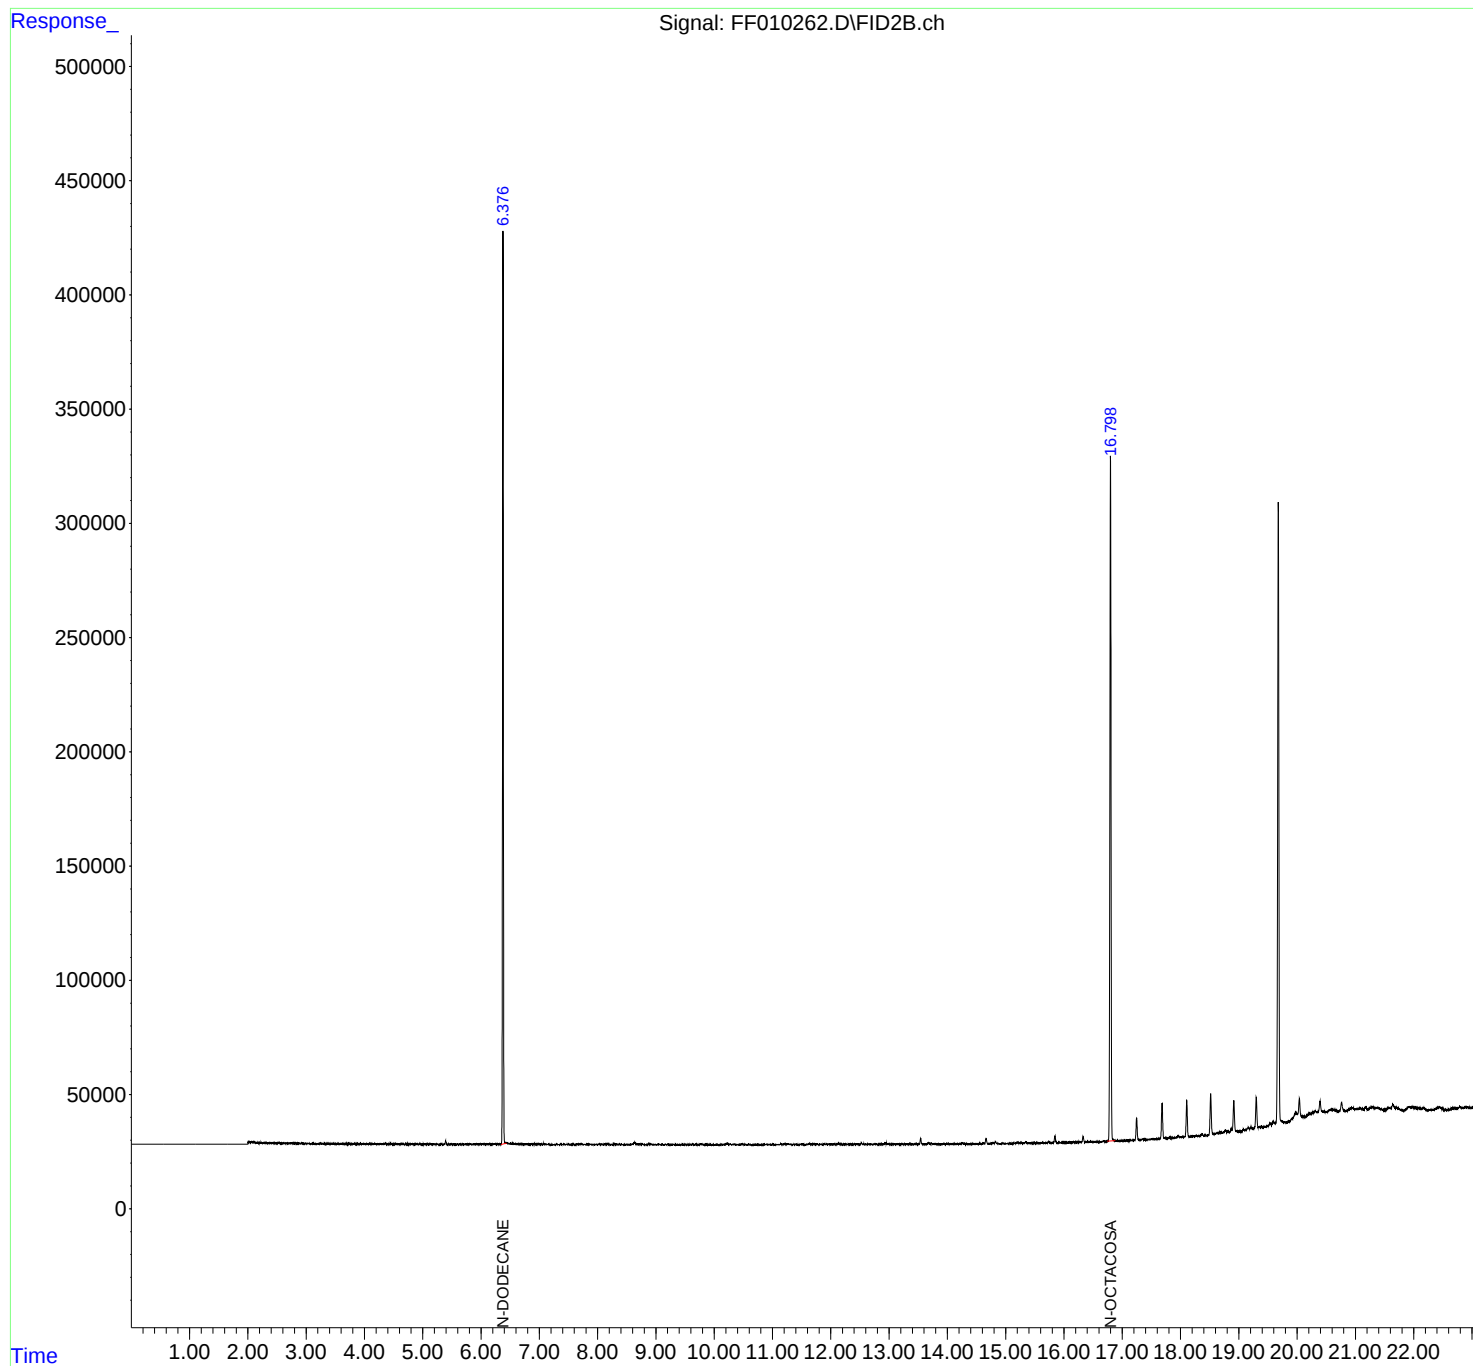


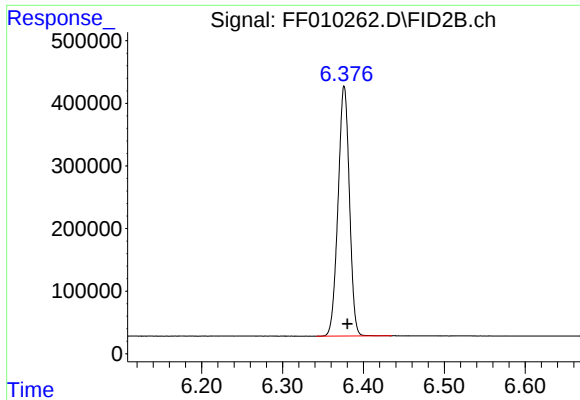

#3 N-DODECANE


R.T.: 6.376 min
Delta R.T.: -0.004 min
Response: 3894488
Conc: 29.25 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

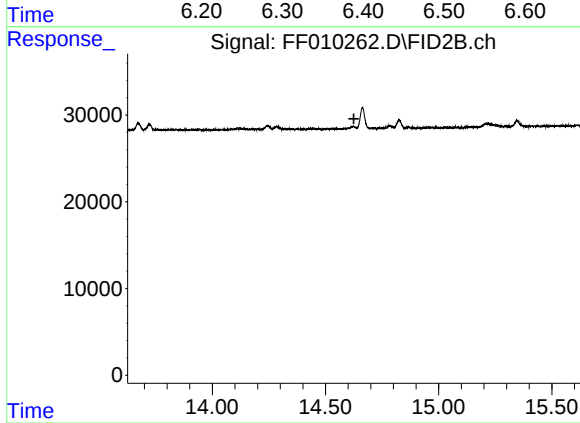

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.625 min
Response: 0
Conc: N.D.

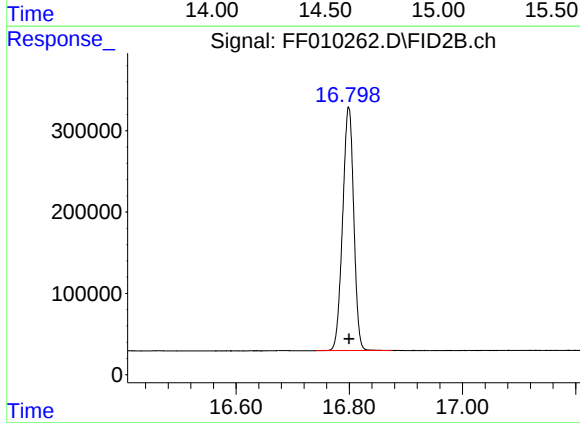

#12 N-OCTACOSANE

R.T.: 16.799 min
Delta R.T.: 0.000 min
Response: 4087119
Conc: 30.84 ug/ml