

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF040622\  
 Data File : FF010272.D  
 Signal(s) : FID2B.ch  
 Acq On : 06 Apr 2022 16:18  
 Operator : AJ\MA  
 Sample : N2254-01  
 Misc :  
 ALS Vial : 57 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 WC-14A-1A-4-1

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 04/07/2022  
 Supervised By :mohammad ahmed 04/07/2022

Integration File: Sample.e  
 Quant Time: Apr 07 00:39:19 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF040122.M  
 Quant Title :  
 QLast Update : Fri Apr 01 11:58:56 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.606 | 571964   | 4.785 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF040622\  
Data File : FF010272.D  
Signal(s) : FID2B.ch  
Acq On : 06 Apr 2022 16:18  
Operator : AJ\MA  
Sample : N2254-01  
Misc :  
ALS Vial : 57 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
WC-14A-1A-4-1


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/07/2022  
Supervised By :mohammad ahmed 04/07/2022

Integration File: Sample.e  
Quant Time: Apr 07 00:39:19 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF040122.M  
Quant Title :  
QLast Update : Fri Apr 01 11:58:56 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

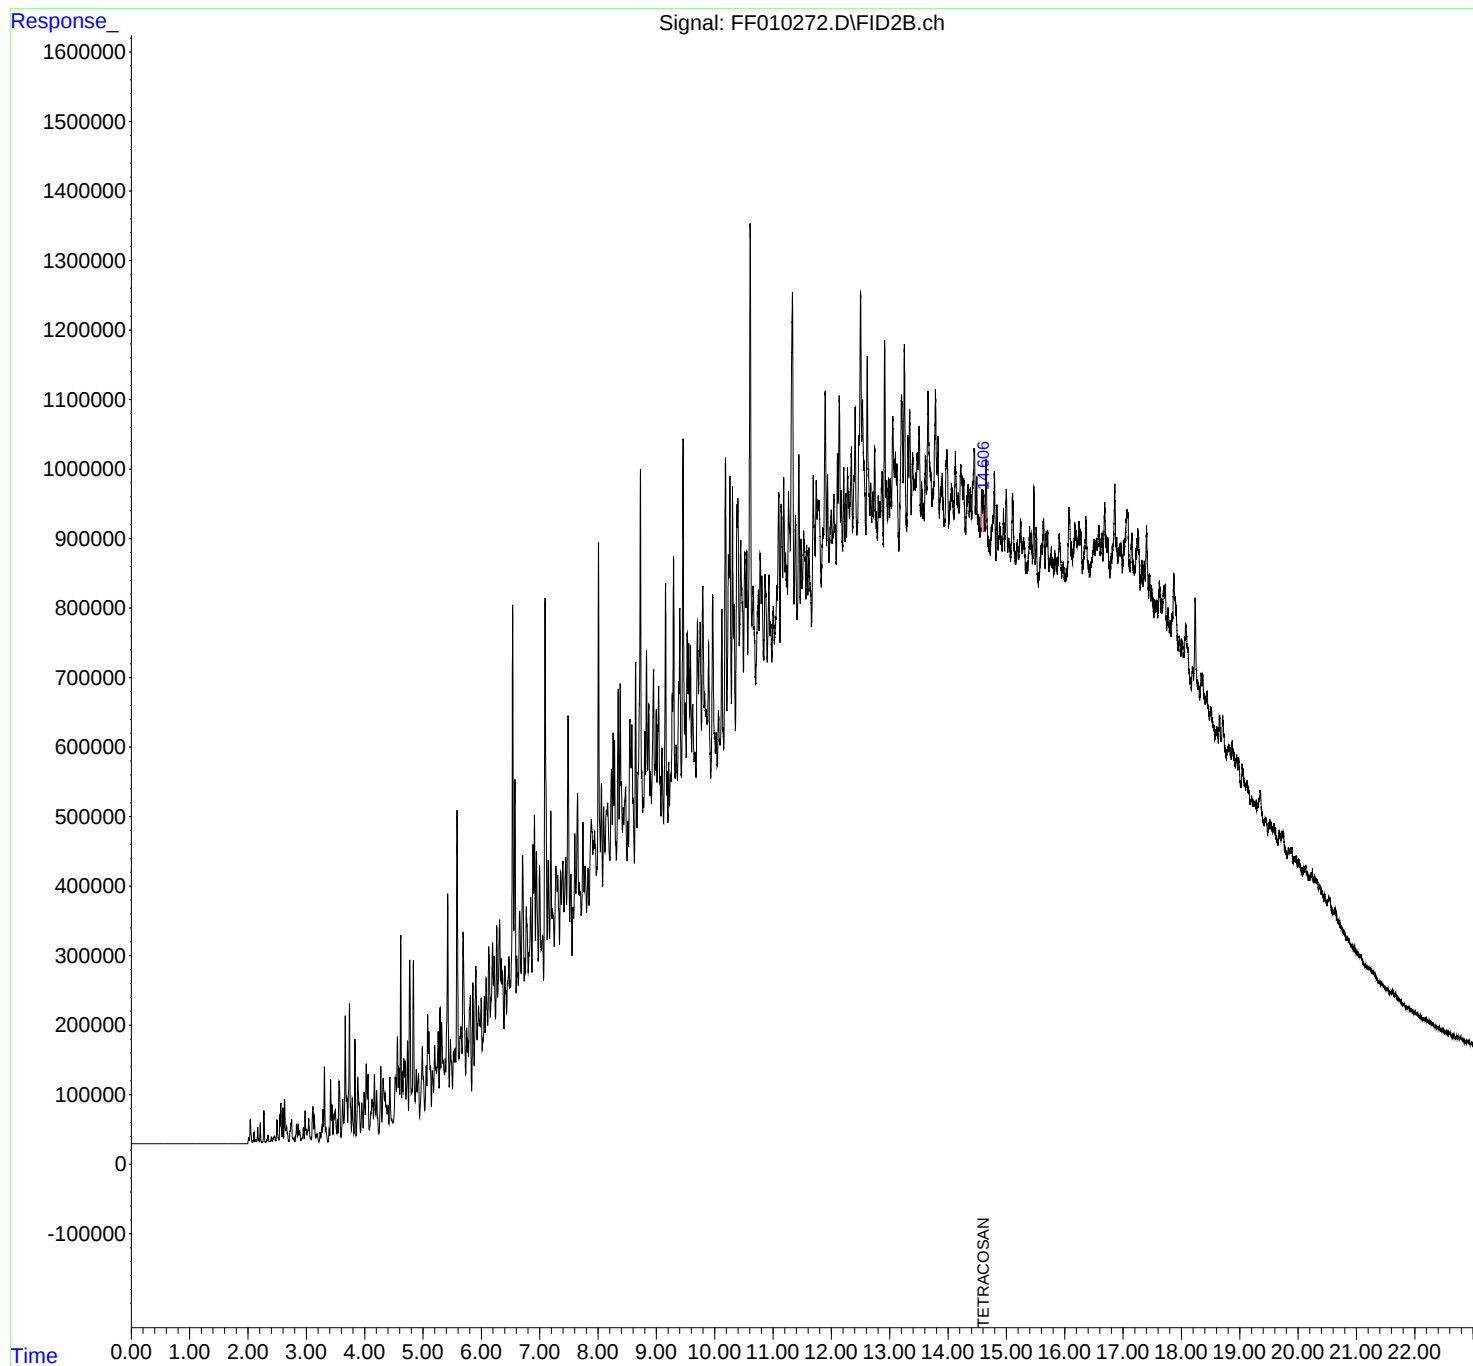

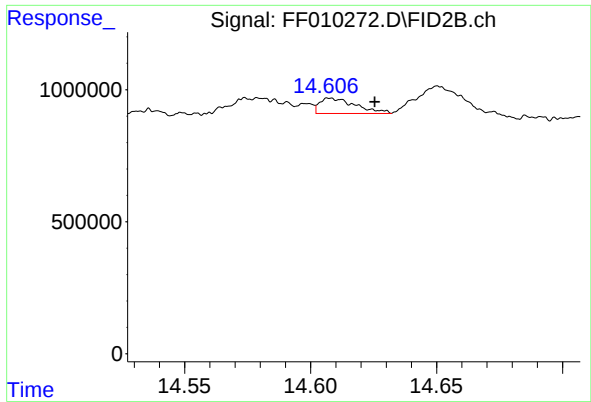

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.606 min  
Delta R.T.: -0.019 min  
Response: 571964  
Conc: 4.79 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
WC-14A-1A-4-1

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/07/2022  
Supervised By :mohammad ahmed 04/07/2022