

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040623\
Data File : FF012380.D
Signal(s) : FID2B.ch
Acq On : 06 Apr 2023 07:51
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 07 05:33:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
8)	N-DOCOSANE	14.107	67007	0.527 ug/ml
10)	N-TETRACOSANE	15.195	443473	3.556 ug/ml
14)	N-DOTRIACONTANE	18.911	115366	1.112 ug/ml
16)	N-HEXATRIACONTANE	20.463	90329	1.031 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040623\
Data File : FF012380.D
Signal(s) : FID2B.ch
Acq On : 06 Apr 2023 07:51
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 07 05:33:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

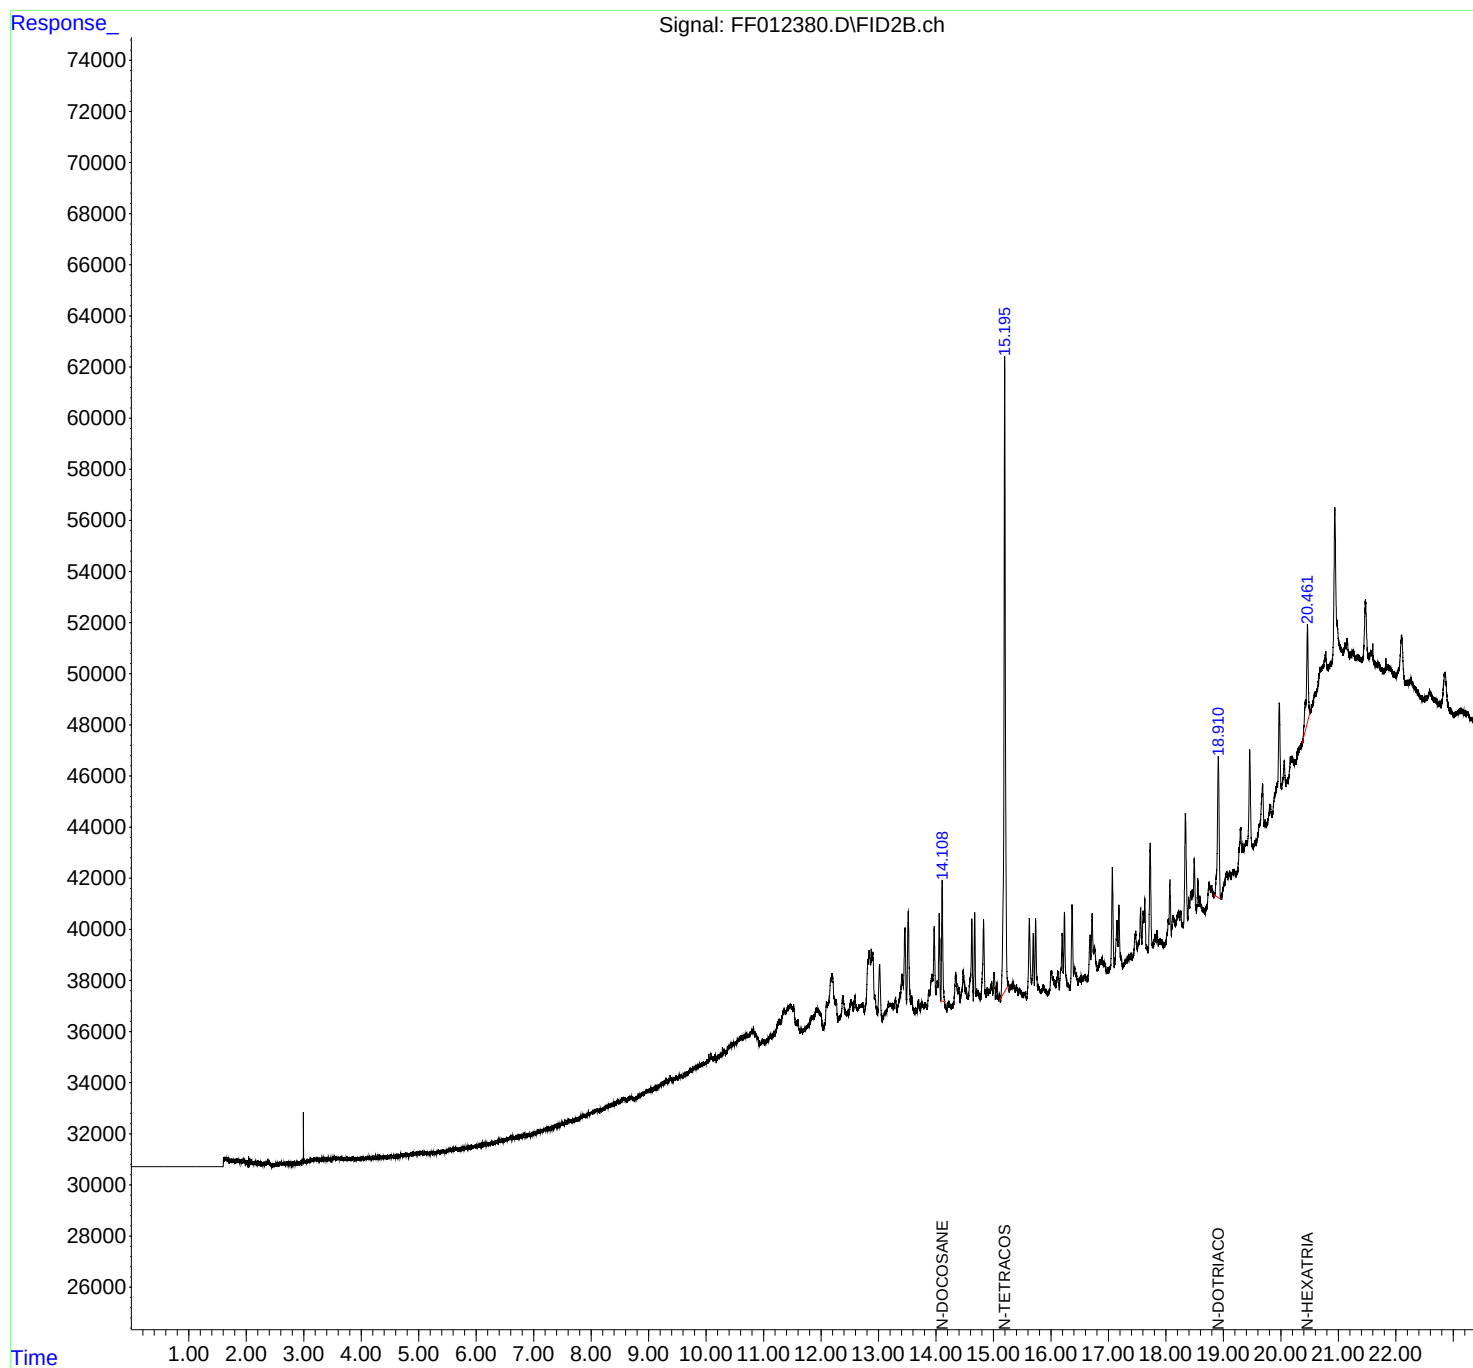


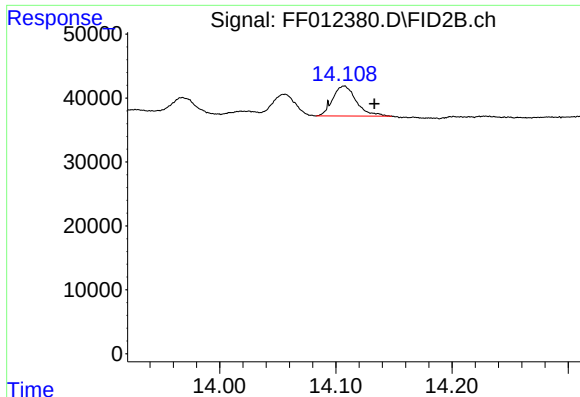

#8 N-DOCOSANE


R.T.: 14.107 min
Delta R.T.: -0.026 min
Response: 67007
Conc: 0.53 ug/ml

Instrument :
FID_F
ClientSampleId :

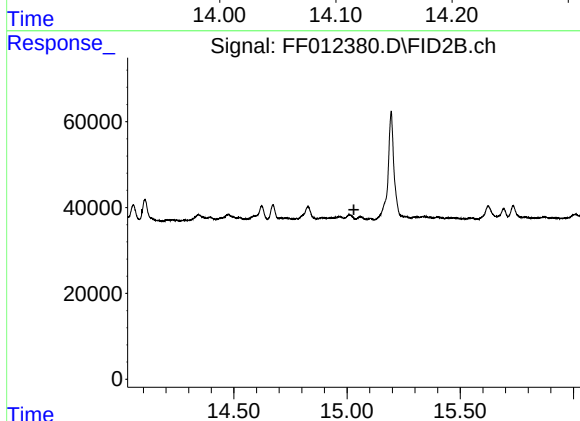


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.030 min
Response: 0
Conc: N.D.

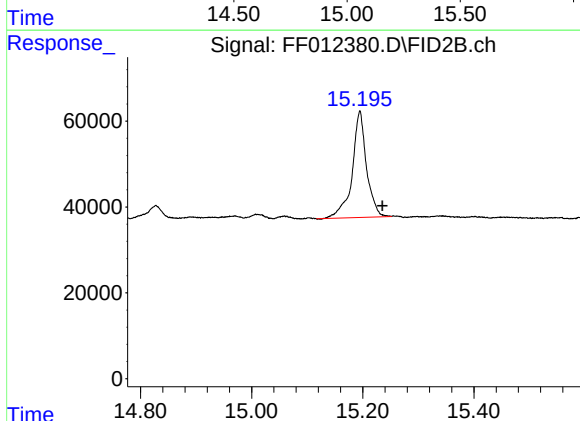


#10 N-TETRACOSANE

R.T.: 15.195 min
Delta R.T.: -0.040 min
Response: 443473
Conc: 3.56 ug/ml

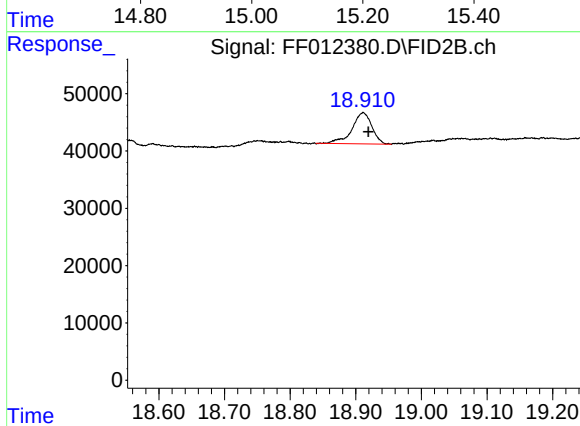

#14 N-DOTRIACONTANE

R.T.: 18.911 min
Delta R.T.: -0.008 min
Response: 115366
Conc: 1.11 ug/ml

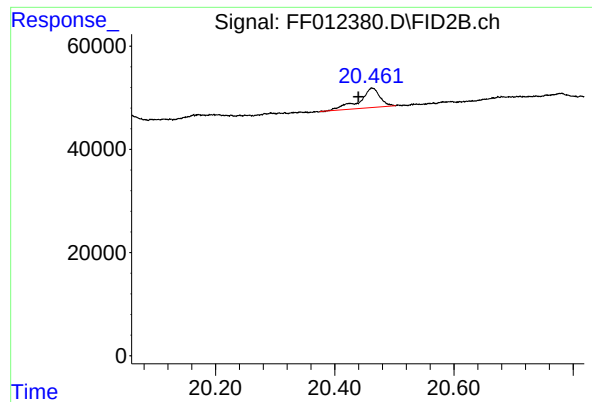

#16 N-HEXATRIACONTANE

R.T.: 20.463 min
Delta R.T.: 0.023 min
Response: 90329
Conc: 1.03 ug/ml

Instrument :

FID_F

ClientSampleId :