

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040623\
 Data File : FF012381.D
 Signal(s) : FID2B.ch
 Acq On : 06 Apr 2023 08:20
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 07 05:33:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.015	2005421	17.920 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.076	74115	0.674 ug/ml
14) N-DOTRIACONTANE	18.906	106439	1.026 ug/ml
15) N-TETRATRIACONTANE	19.689	82375	0.871 ug/ml
16) N-HEXATRIACONTANE	20.430	47766	0.545 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040623\
Data File : FF012381.D
Signal(s) : FID2B.ch
Acq On : 06 Apr 2023 08:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 07 05:33:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

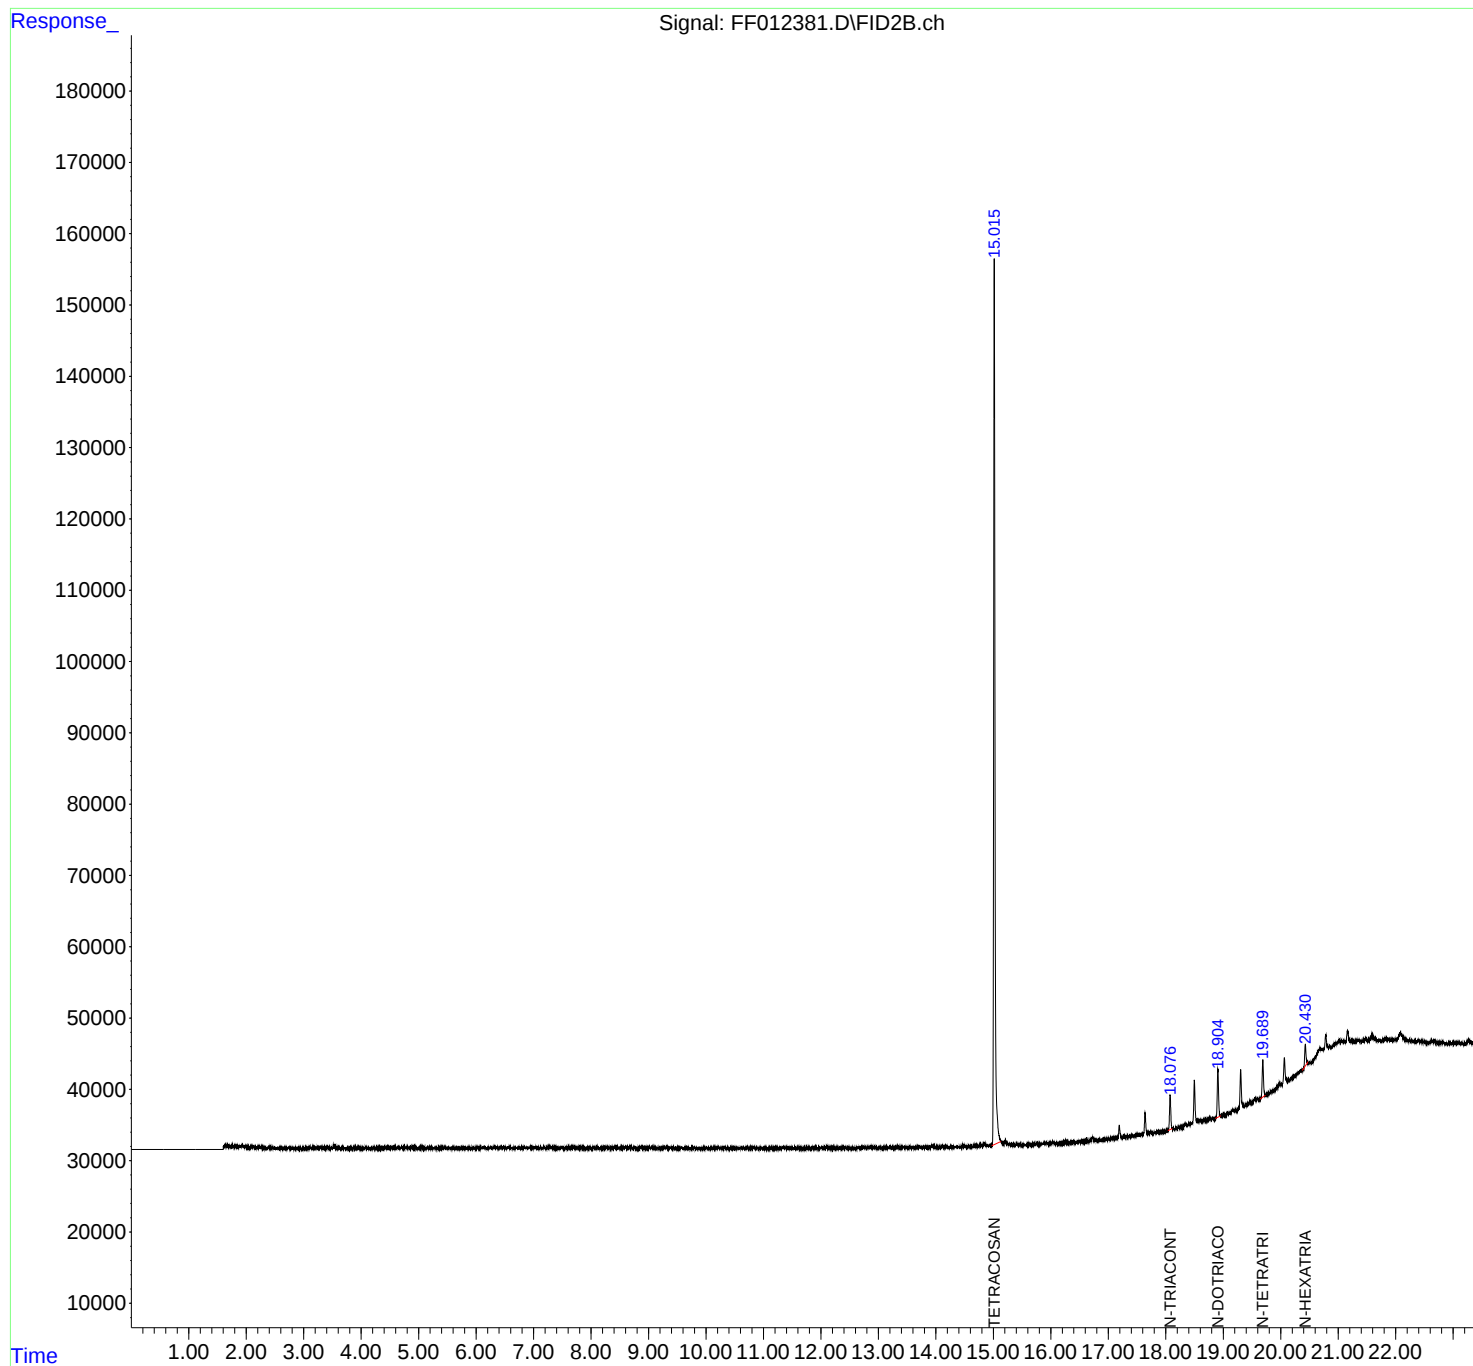


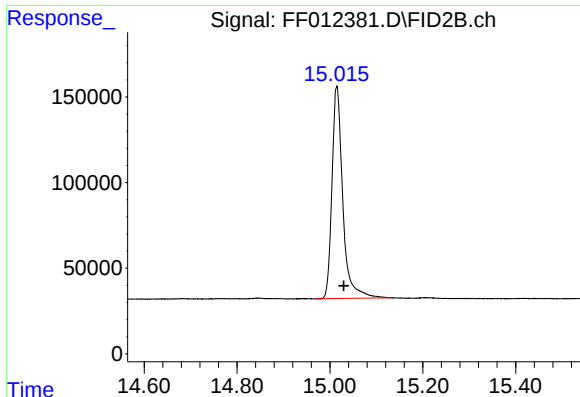

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.015 min
Delta R.T.: -0.015 min
Response: 2005421
Conc: 17.92 ug/ml

Instrument :
FID_F
ClientSampleId :

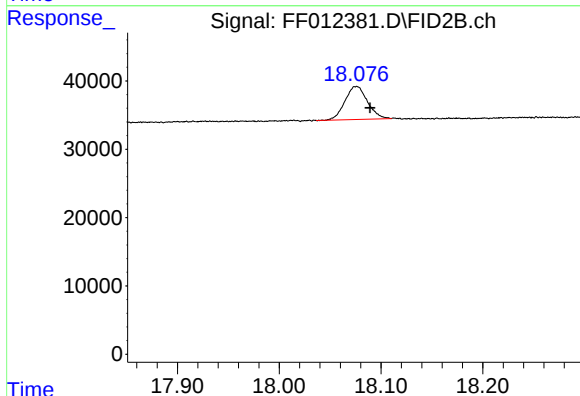


#13 N-TRIACONTANE

R.T.: 18.076 min
Delta R.T.: -0.014 min
Response: 74115
Conc: 0.67 ug/ml

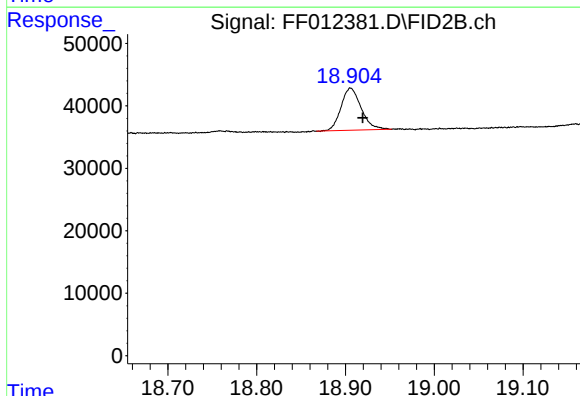


#14 N-DOTRIACONTANE

R.T.: 18.906 min
Delta R.T.: -0.014 min
Response: 106439
Conc: 1.03 ug/ml

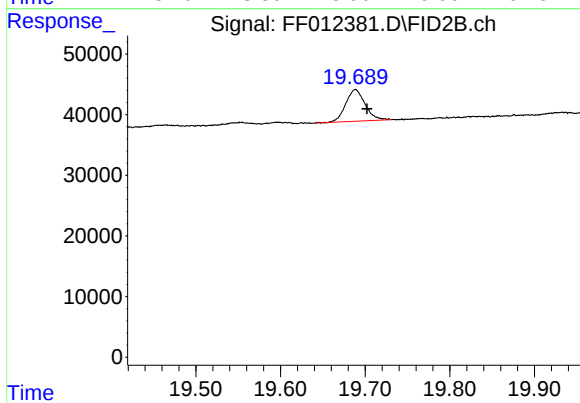

#15 N-TETRATRIACONTANE

R.T.: 19.689 min
Delta R.T.: -0.014 min
Response: 82375
Conc: 0.87 ug/ml

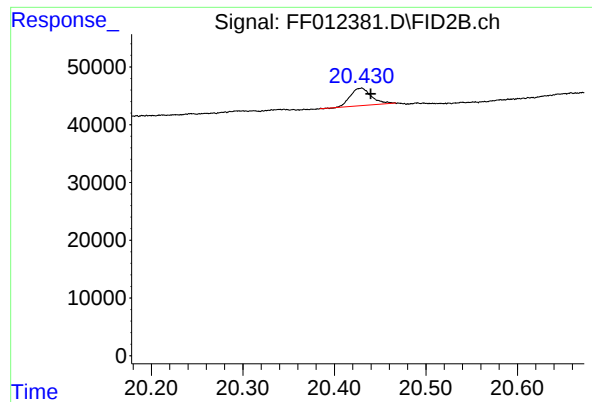

#16 N-HEXATRIACONTANE

R.T.: 20.430 min
Delta R.T.: -0.010 min
Response: 47766
Conc: 0.55 ug/ml

Instrument :

FID_F

ClientSampleId :