

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040623\
 Data File : FF012383.D
 Signal(s) : FID2B.ch
 Acq On : 06 Apr 2023 09:19
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 07 05:33:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.744	1543515	12.451 ug/ml
12) N-OCTACOSANE	17.187	1748154	15.197 ug/ml
13) N-TRIACONTANE	18.072	316969	2.881 ug/ml
14) N-DOTRIACONTANE	18.903	438085	4.221 ug/ml
15) N-TETRATRIACONTANE	19.686	352206	3.723 ug/ml
16) N-HEXATRIACONTANE	20.427	241729	2.759 ug/ml
17) N-OCTATRIACONTANE	21.160	153932	1.859 ug/ml
18) N-TETRACONTANE	22.066	100496	1.230 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040623\
Data File : FF012383.D
Signal(s) : FID2B.ch
Acq On : 06 Apr 2023 09:19
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 07 05:33:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

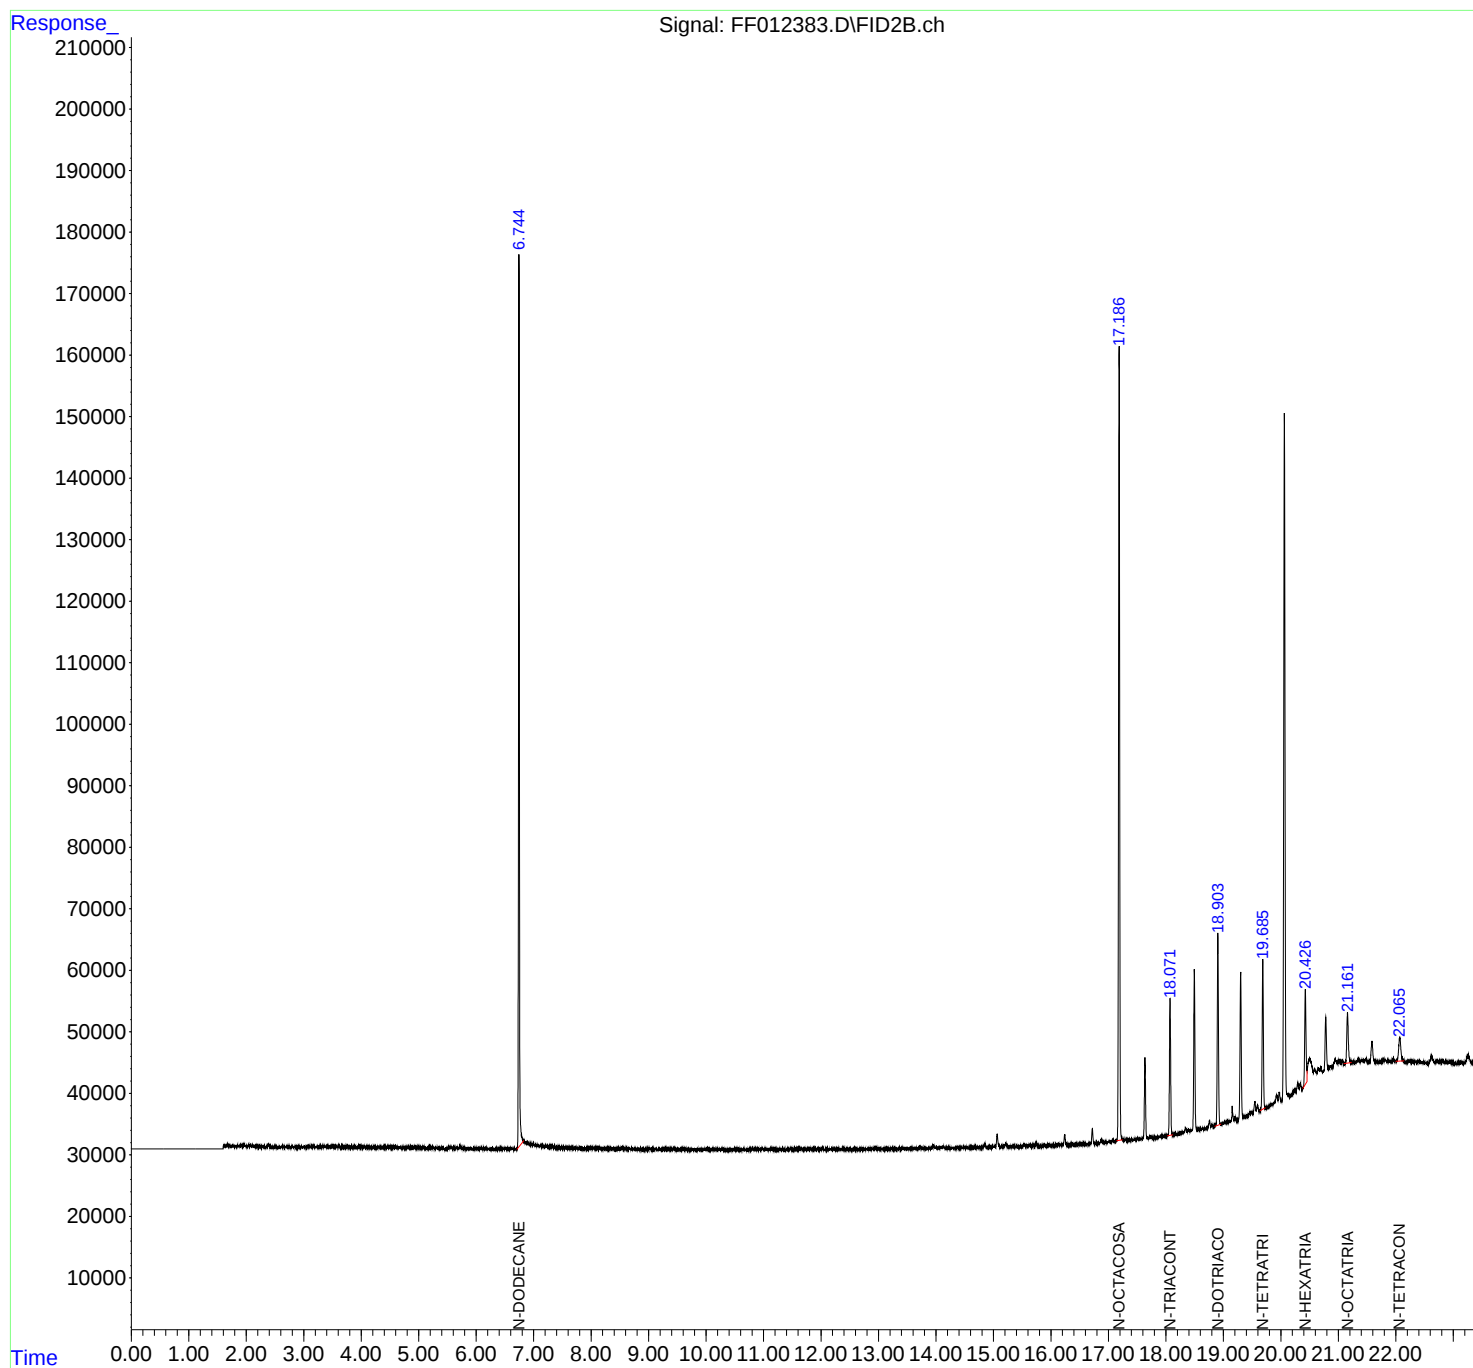


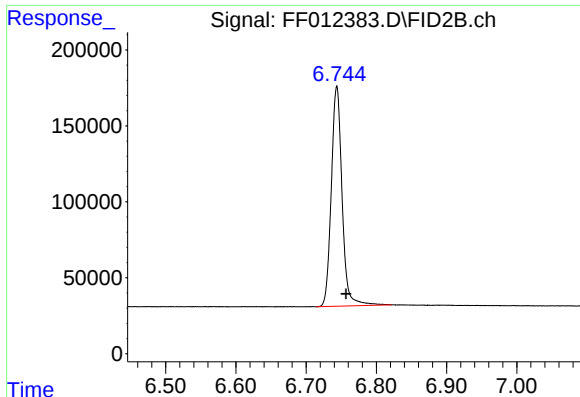

#3 N-DODECANE


R.T.: 6.744 min
Delta R.T.: -0.013 min
Response: 1543515
Conc: 12.45 ug/ml

Instrument :
FID_F
ClientSampleId :

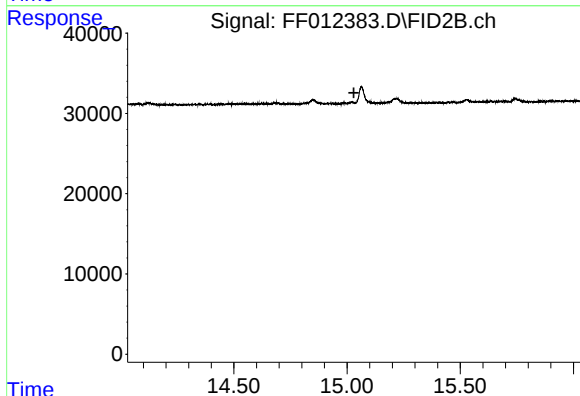


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.030 min
Response: 0
Conc: N.D.

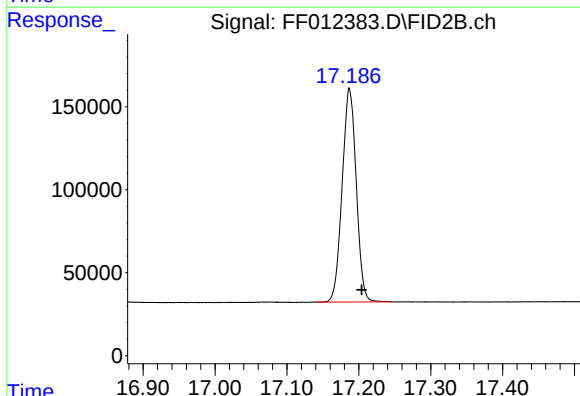


#12 N-OCTACOSANE

R.T.: 17.187 min
Delta R.T.: -0.017 min
Response: 1748154
Conc: 15.20 ug/ml

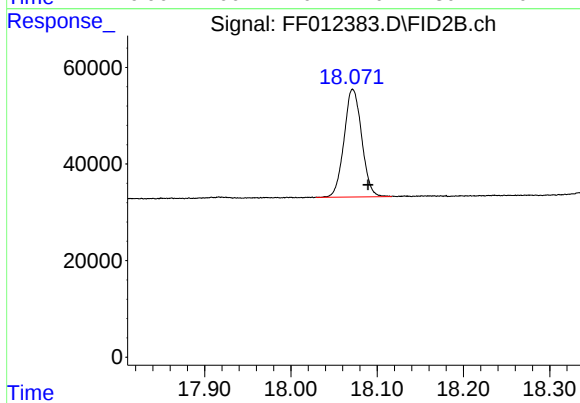

#13 N-TRIACONTANE


R.T.: 18.072 min
Delta R.T.: -0.018 min
Response: 316969
Conc: 2.88 ug/ml

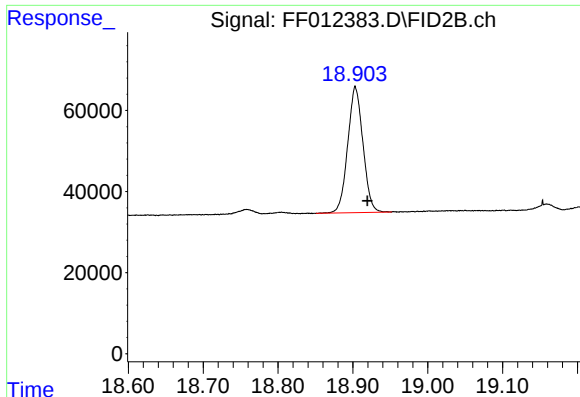

#14 N-DOTRIACONTANE


R.T.: 18.903 min
Delta R.T.: -0.016 min
Response: 438085
Conc: 4.22 ug/ml

Instrument :
FID_F
ClientSampleId :

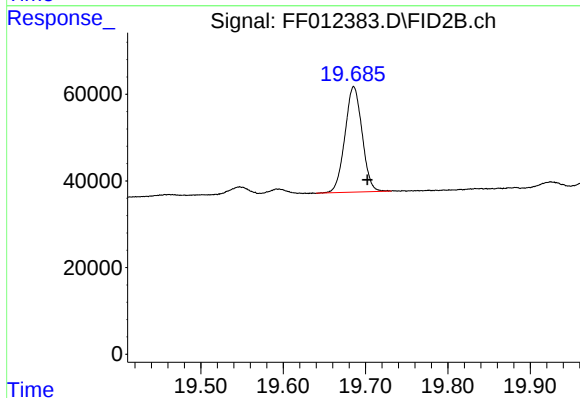


#15 N-TETRATRIACONTANE

R.T.: 19.686 min
Delta R.T.: -0.016 min
Response: 352206
Conc: 3.72 ug/ml

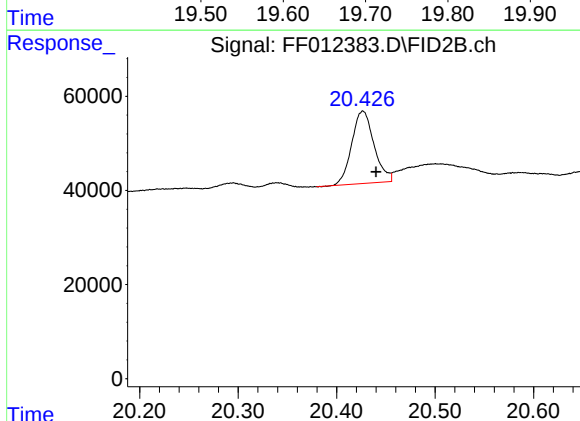


#16 N-HEXATRIACONTANE

R.T.: 20.427 min
Delta R.T.: -0.013 min
Response: 241729
Conc: 2.76 ug/ml

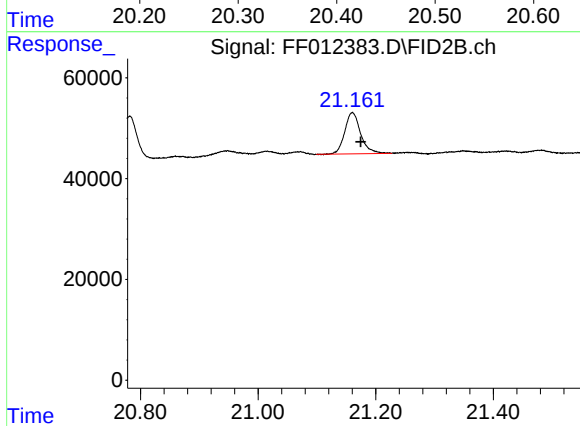

#17 N-OCTATRIACONTANE

R.T.: 21.160 min
Delta R.T.: -0.014 min
Response: 153932
Conc: 1.86 ug/ml

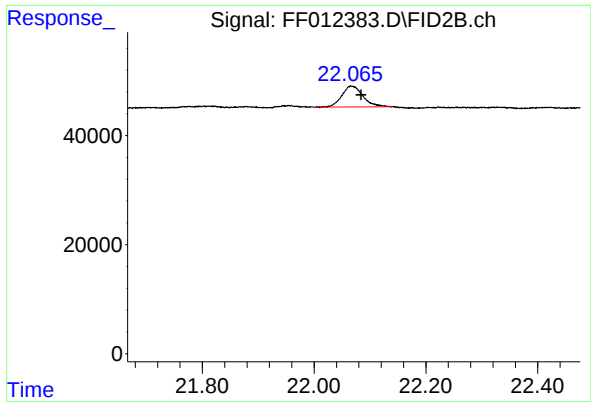

#18 N-TETRACONTANE

R.T.: 22.066 min
Delta R.T.: -0.018 min
Response: 100496
Conc: 1.23 ug/ml

Instrument :
FID_F
ClientSampleId :