

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040623\
 Data File : FF012393.D
 Signal(s) : FID2B.ch
 Acq On : 06 Apr 2023 17:58
 Operator : YP\AJ
 Sample : 02213-08
 Misc : 5 PPM WATER LOQ
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 LOQ-WATER-02-QT2-2023

Integration File: autoint1.e
 Quant Time: Apr 07 05:34:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.017	1646273	14.710 ug/ml
Target Compounds			
2) N-DECANE	4.581	452391	3.613 ug/ml
3) N-DODECANE	6.744	409157	3.300 ug/ml
4) N-TETRADECANE	8.572	410477	3.150 ug/ml
5) N-HEXADECANE	10.176	471565	3.534 ug/ml
6) N-OCTADECANE	11.616	499953	3.722 ug/ml
7) N-EICOSANE	12.923	490684	3.689 ug/ml
8) N-DOCOSANE	14.119	488536	3.845 ug/ml
10) N-TETRACOSANE	15.221	487208	3.907 ug/ml
11) N-HEXACOSANE	16.241	461782	3.857 ug/ml
12) N-OCTACOSANE	17.189	456864	3.972 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040623\
Data File : FF012393.D
Signal(s) : FID2B.ch
Acq On : 06 Apr 2023 17:58
Operator : YP\AJ
Sample : 02213-08
Misc : 5 PPM WATER LOQ
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
LOQ-WATER-02-QT2-2023

Integration File: autoint1.e
Quant Time: Apr 07 05:34:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

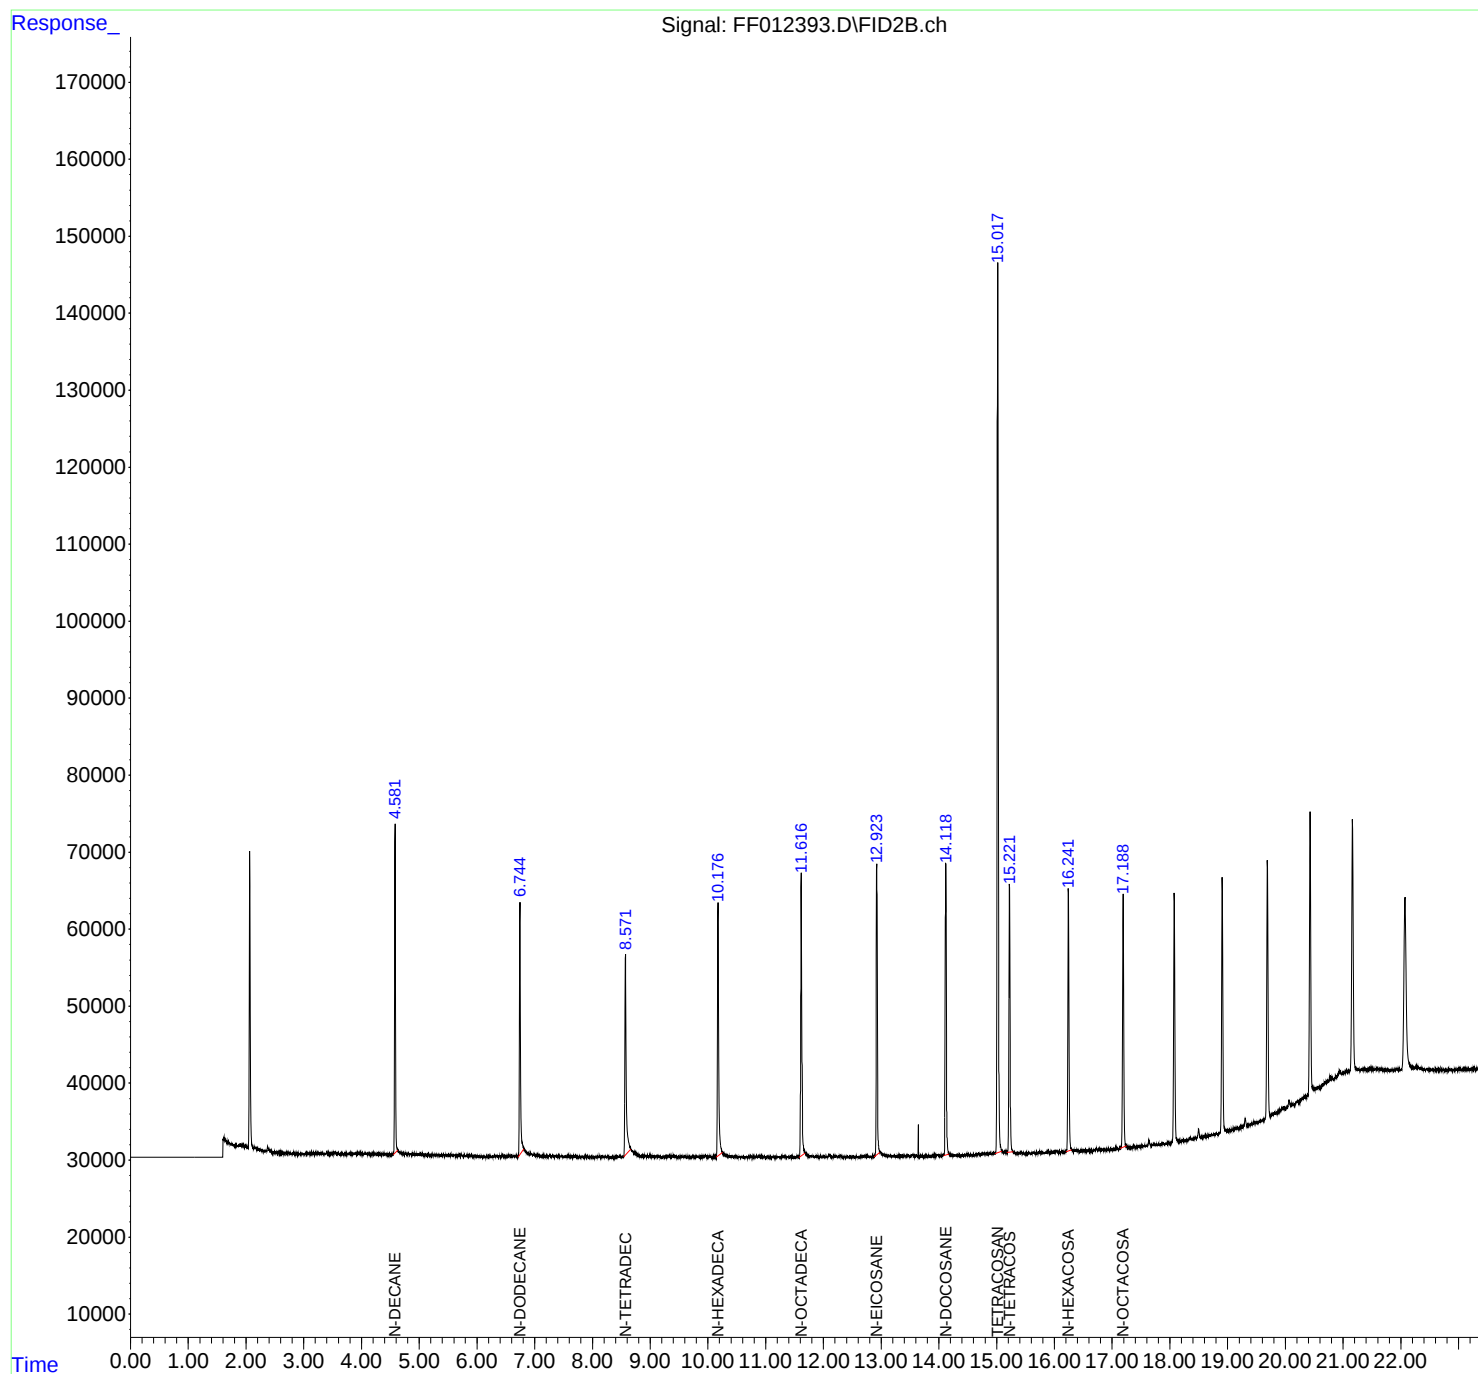


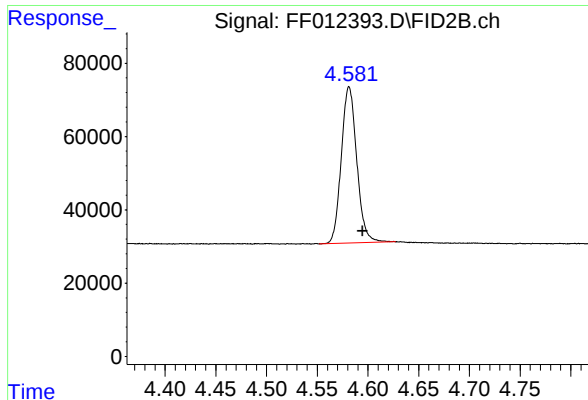

#2 N-DECANE


R.T.: 4.581 min
Delta R.T.: -0.013 min
Response: 452391
Conc: 3.61 ug/ml

Instrument :
FID_F
ClientSampleId :
LOQ-WATER-02-QT2-2023

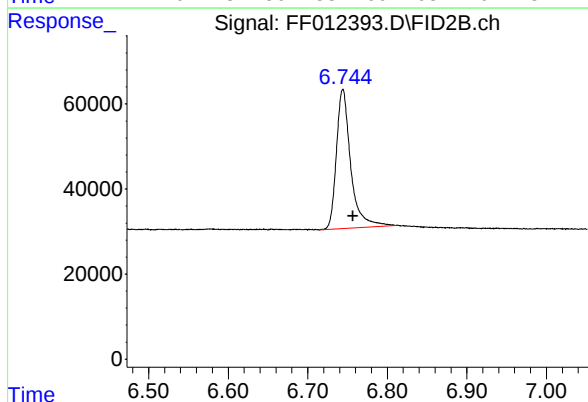


#3 N-DODECANE

R.T.: 6.744 min
Delta R.T.: -0.013 min
Response: 409157
Conc: 3.30 ug/ml

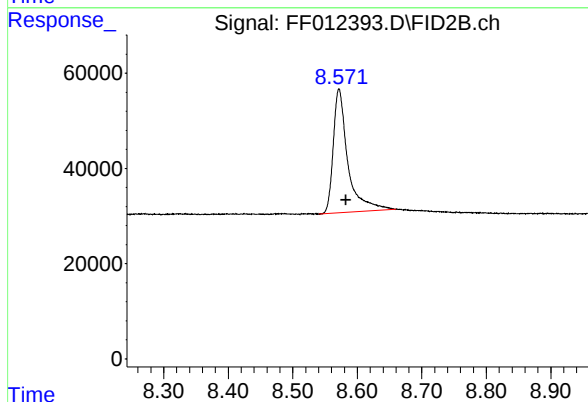


#4 N-TETRADECANE

R.T.: 8.572 min
Delta R.T.: -0.011 min
Response: 410477
Conc: 3.15 ug/ml

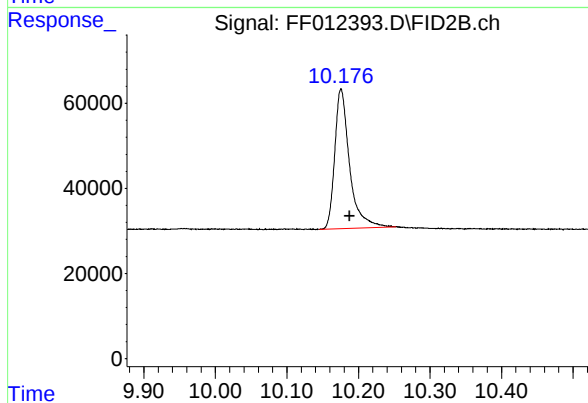

#5 N-HEXADECANE


R.T.: 10.176 min
Delta R.T.: -0.012 min
Response: 471565
Conc: 3.53 ug/ml

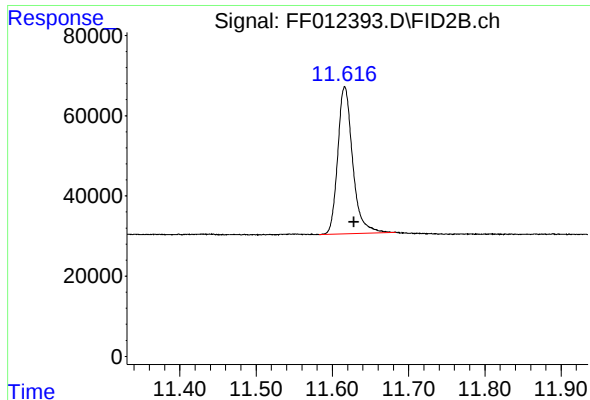

#6 N-OCTADECANE


R.T.: 11.616 min
Delta R.T.: -0.012 min
Response: 499953
Conc: 3.72 ug/ml

Instrument :
FID_F
ClientSampleId :
LOQ-WATER-02-QT2-2023

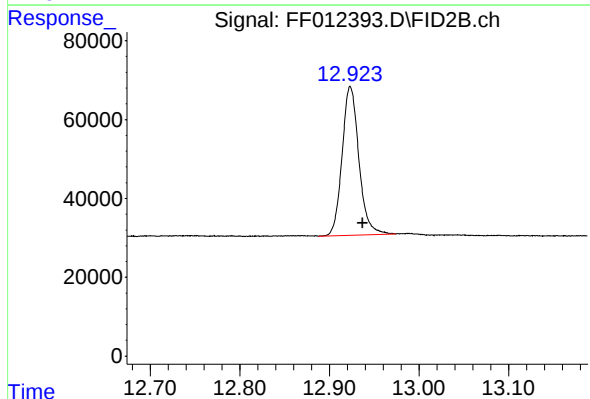


#7 N-EICOSANE

R.T.: 12.923 min
Delta R.T.: -0.014 min
Response: 490684
Conc: 3.69 ug/ml

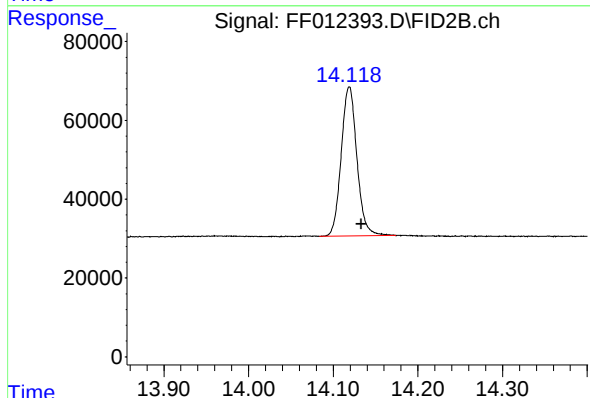


#8 N-DOCOSANE

R.T.: 14.119 min
Delta R.T.: -0.014 min
Response: 488536
Conc: 3.84 ug/ml

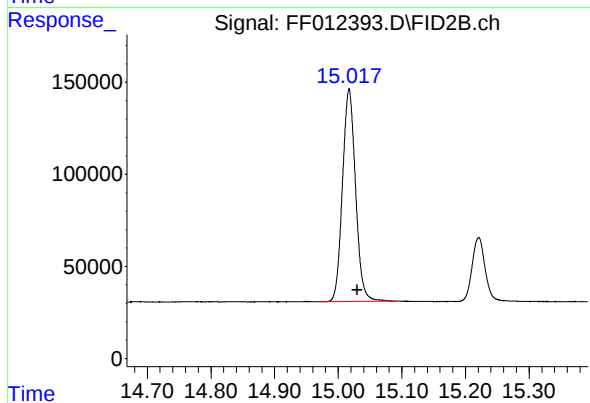

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.017 min
Delta R.T.: -0.013 min
Response: 1646273
Conc: 14.71 ug/ml

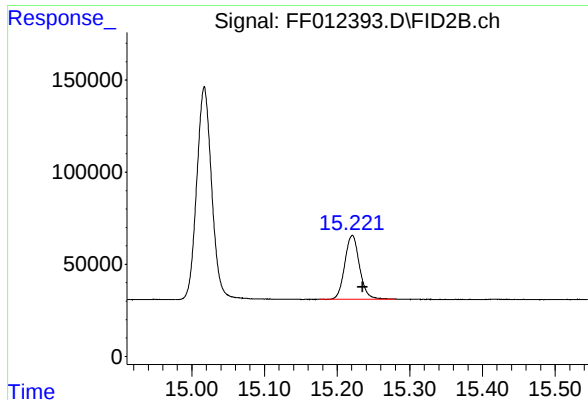

#10 N-TETRACOSANE


R.T.: 15.221 min
Delta R.T.: -0.014 min
Response: 487208
Conc: 3.91 ug/ml

Instrument :
FID_F
ClientSampleId :
LOQ-WATER-02-QT2-2023

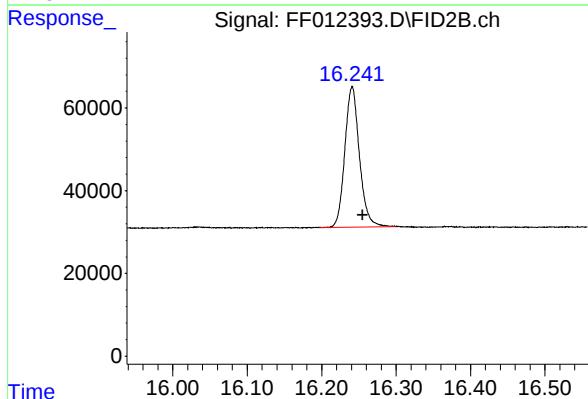

#11 N-HEXACOSANE

R.T.: 16.241 min
Delta R.T.: -0.014 min
Response: 461782
Conc: 3.86 ug/ml

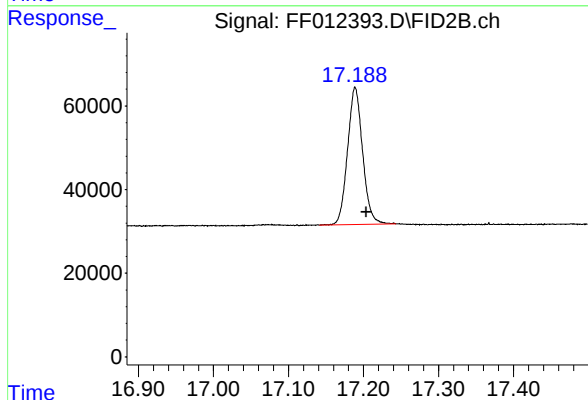

#12 N-OCTACOSANE

R.T.: 17.189 min
Delta R.T.: -0.015 min
Response: 456864
Conc: 3.97 ug/ml