

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040720\
 Data File : FF006784.D
 Signal(s) : FID2B.ch
 Acq On : 07 Apr 2020 17:30
 Operator : DD\AJ
 Sample : L2123-01 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 08 02:08:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.577	104347	0.811 ug/ml
Target Compounds			
7) N-EICOSANE	12.556f	458501	3.085 ug/ml
10) N-TETRACOSANE	14.772	215274	1.457 ug/ml
12) N-OCTACOSANE	16.771	76930	0.537 ug/ml
13) N-TRIACONTANE	17.625	174530	1.233 ug/ml
14) N-DOTRIACONTANE	18.454	225006	1.669 ug/ml
15) N-TETRATRIACONTANE	19.237	64033	0.567 ug/ml
16) N-HEXATRIACONTANE	19.975	160086	1.743 ug/ml
17) N-OCTATRIACONTANE	20.687	27875	0.404 ug/ml
18) N-TETRACONTANE	21.570	332396	4.803 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040720\
Data File : FF006784.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2020 17:30
Operator : DD\AJ
Sample : L2123-01 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 08 02:08:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

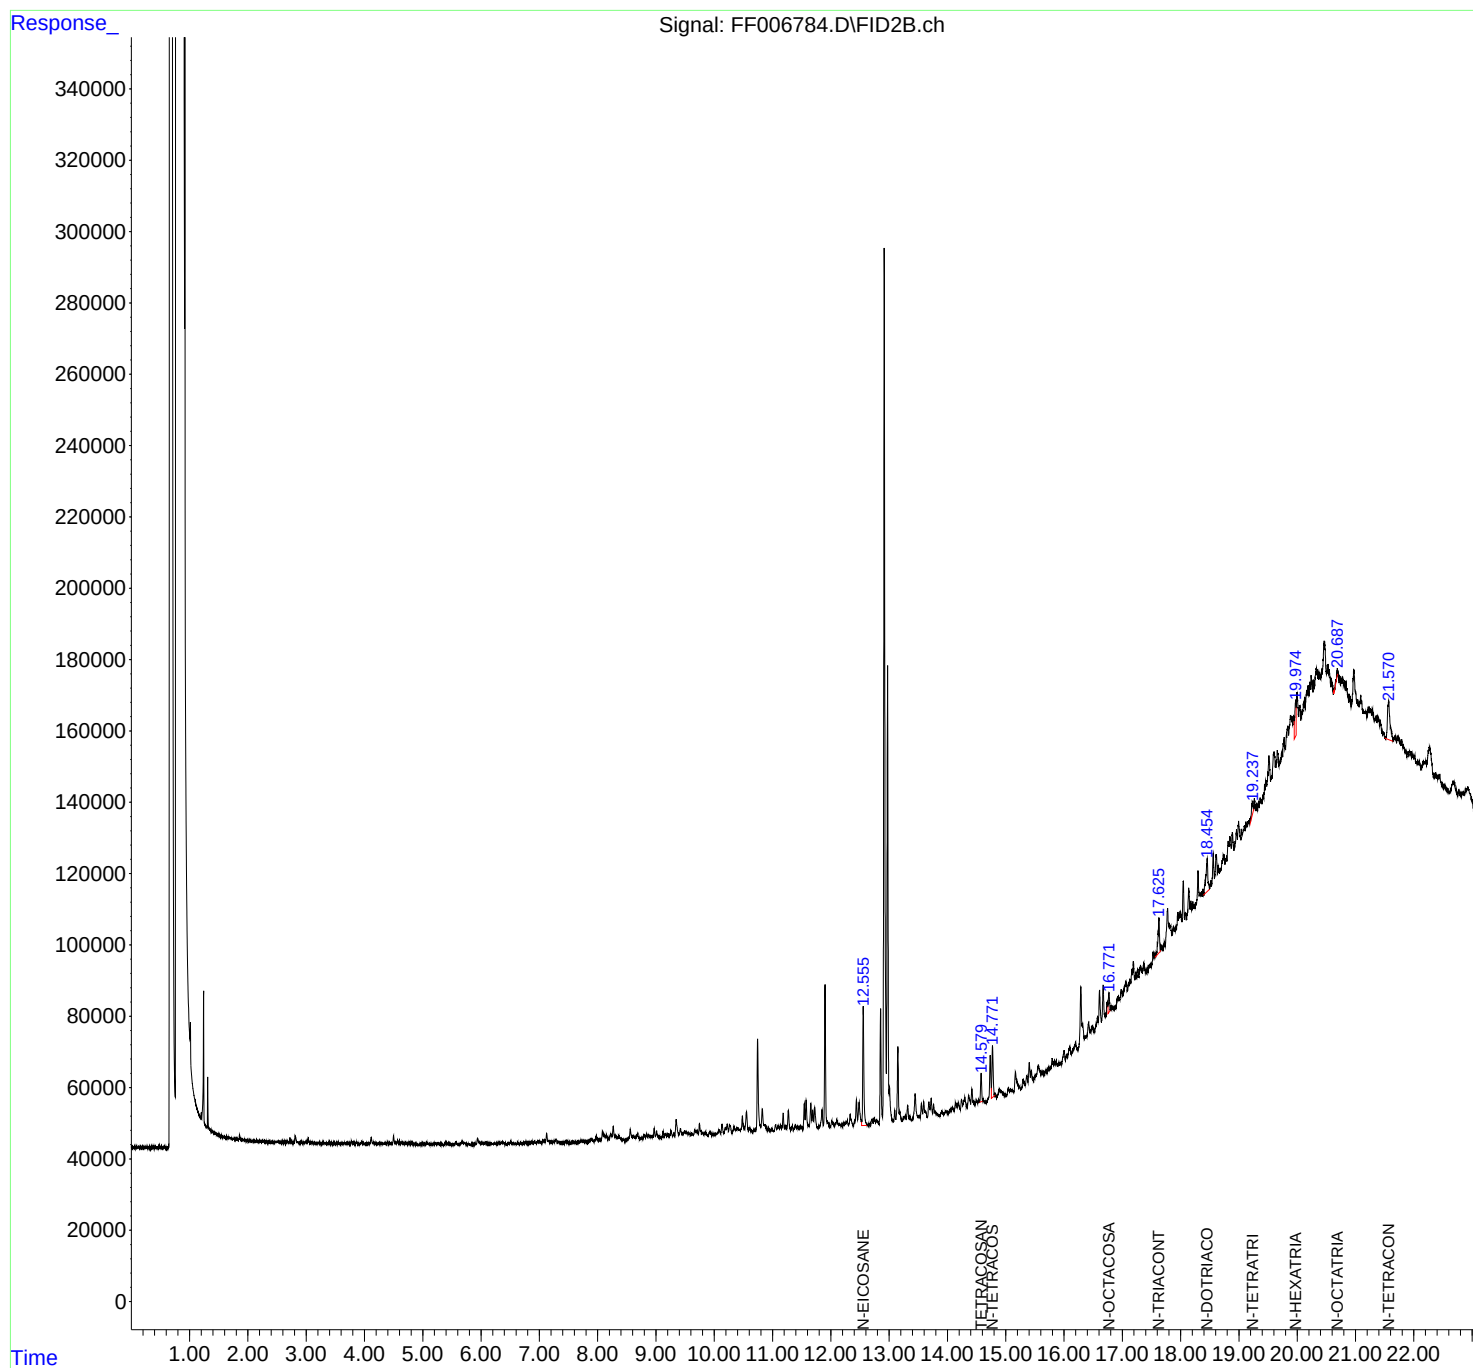

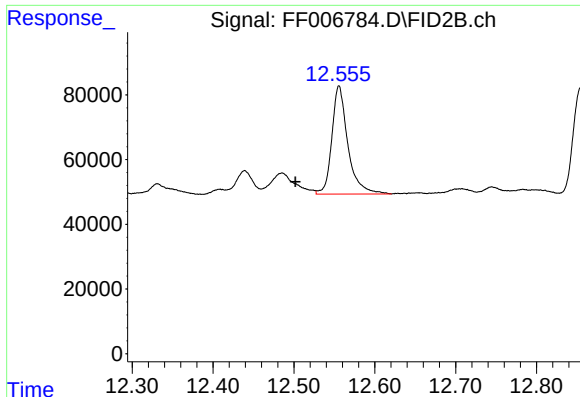


#7 N-EICOSANE

R.T.: 12.556 min
Delta R.T.: 0.054 min
Response: 458501
Conc: 3.08 ug/ml

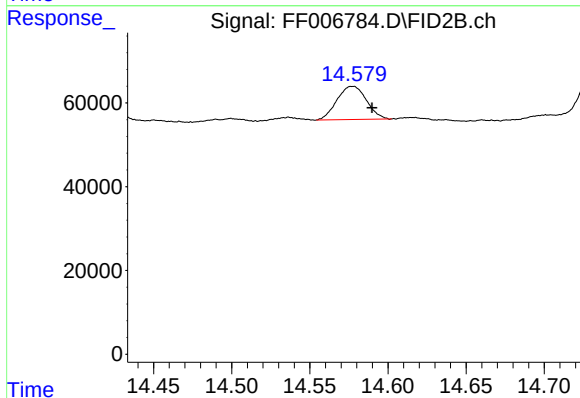


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.577 min
Delta R.T.: -0.012 min
Response: 104347
Conc: 0.81 ug/ml

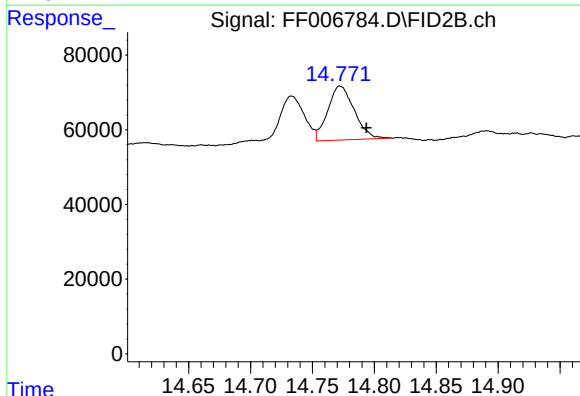


#10 N-TETRACOSANE

R.T.: 14.772 min
Delta R.T.: -0.021 min
Response: 215274
Conc: 1.46 ug/ml

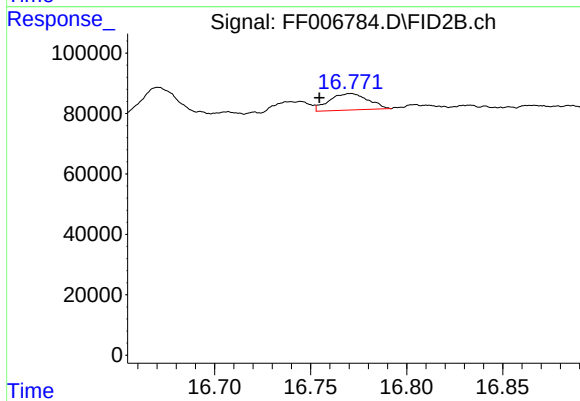


#12 N-OCTACOSANE

R.T.: 16.771 min
Delta R.T.: 0.016 min
Response: 76930
Conc: 0.54 ug/ml

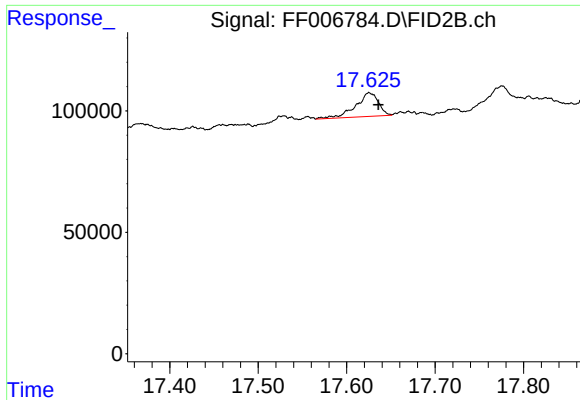


#13 N-TRIACONTANE

R.T.: 17.625 min
Delta R.T.: -0.011 min
Response: 174530
Conc: 1.23 ug/ml

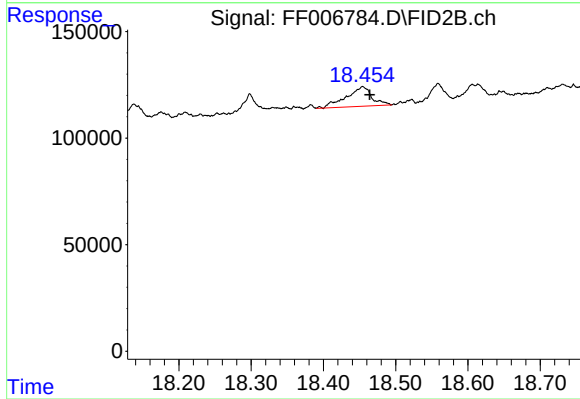


#14 N-DOTRIACONTANE

R.T.: 18.454 min
Delta R.T.: -0.010 min
Response: 225006
Conc: 1.67 ug/ml

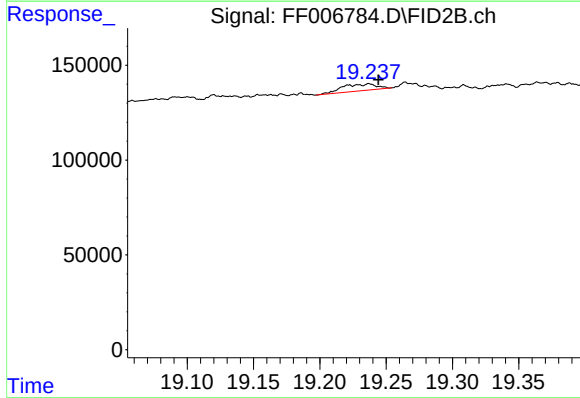


#15 N-TETRATRIACONTANE

R.T.: 19.237 min
Delta R.T.: -0.007 min
Response: 64033
Conc: 0.57 ug/ml

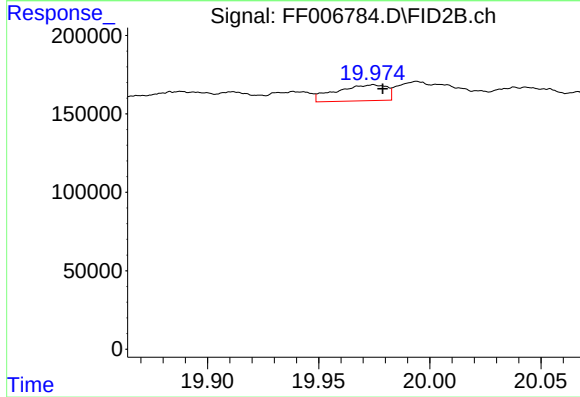


#16 N-HEXATRIACONTANE

R.T.: 19.975 min
Delta R.T.: -0.004 min
Response: 160086
Conc: 1.74 ug/ml

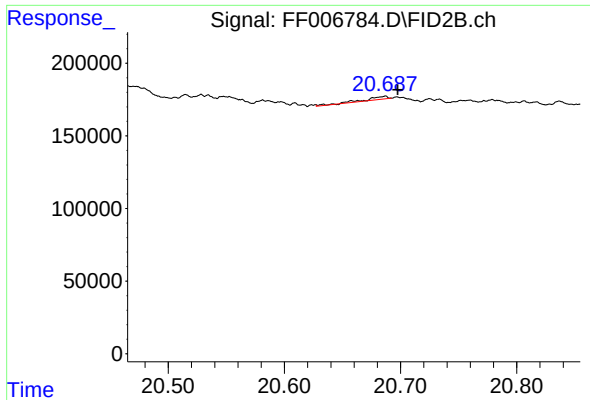

#17 N-OCTATRIACONTANE

R.T.: 20.687 min
Delta R.T.: -0.011 min
Response: 27875
Conc: 0.40 ug/ml

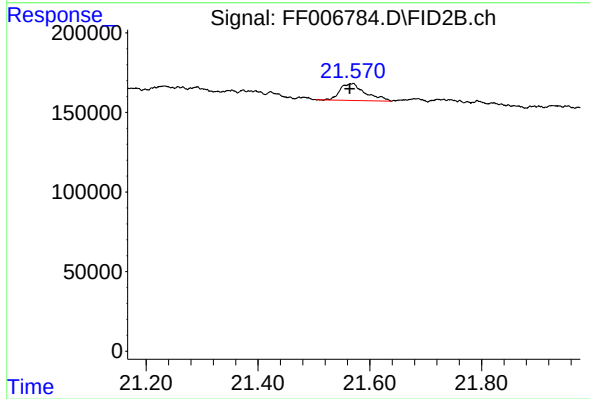

#18 N-TETRACONTANE

R.T.: 21.570 min
Delta R.T.: 0.006 min
Response: 332396
Conc: 4.80 ug/ml