

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040722\
Data File : FF010280.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2022 11:38
Operator : AJ\MA
Sample : N2254-01 100X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 01:54:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

16)	N-HEXATRIACONTANE	19.978f	239546	2.297 ug/ml
-----	-------------------	---------	--------	-------------

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040722\
Data File : FF010280.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2022 11:38
Operator : AJ\MA
Sample : N2254-01 100X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 01:54:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

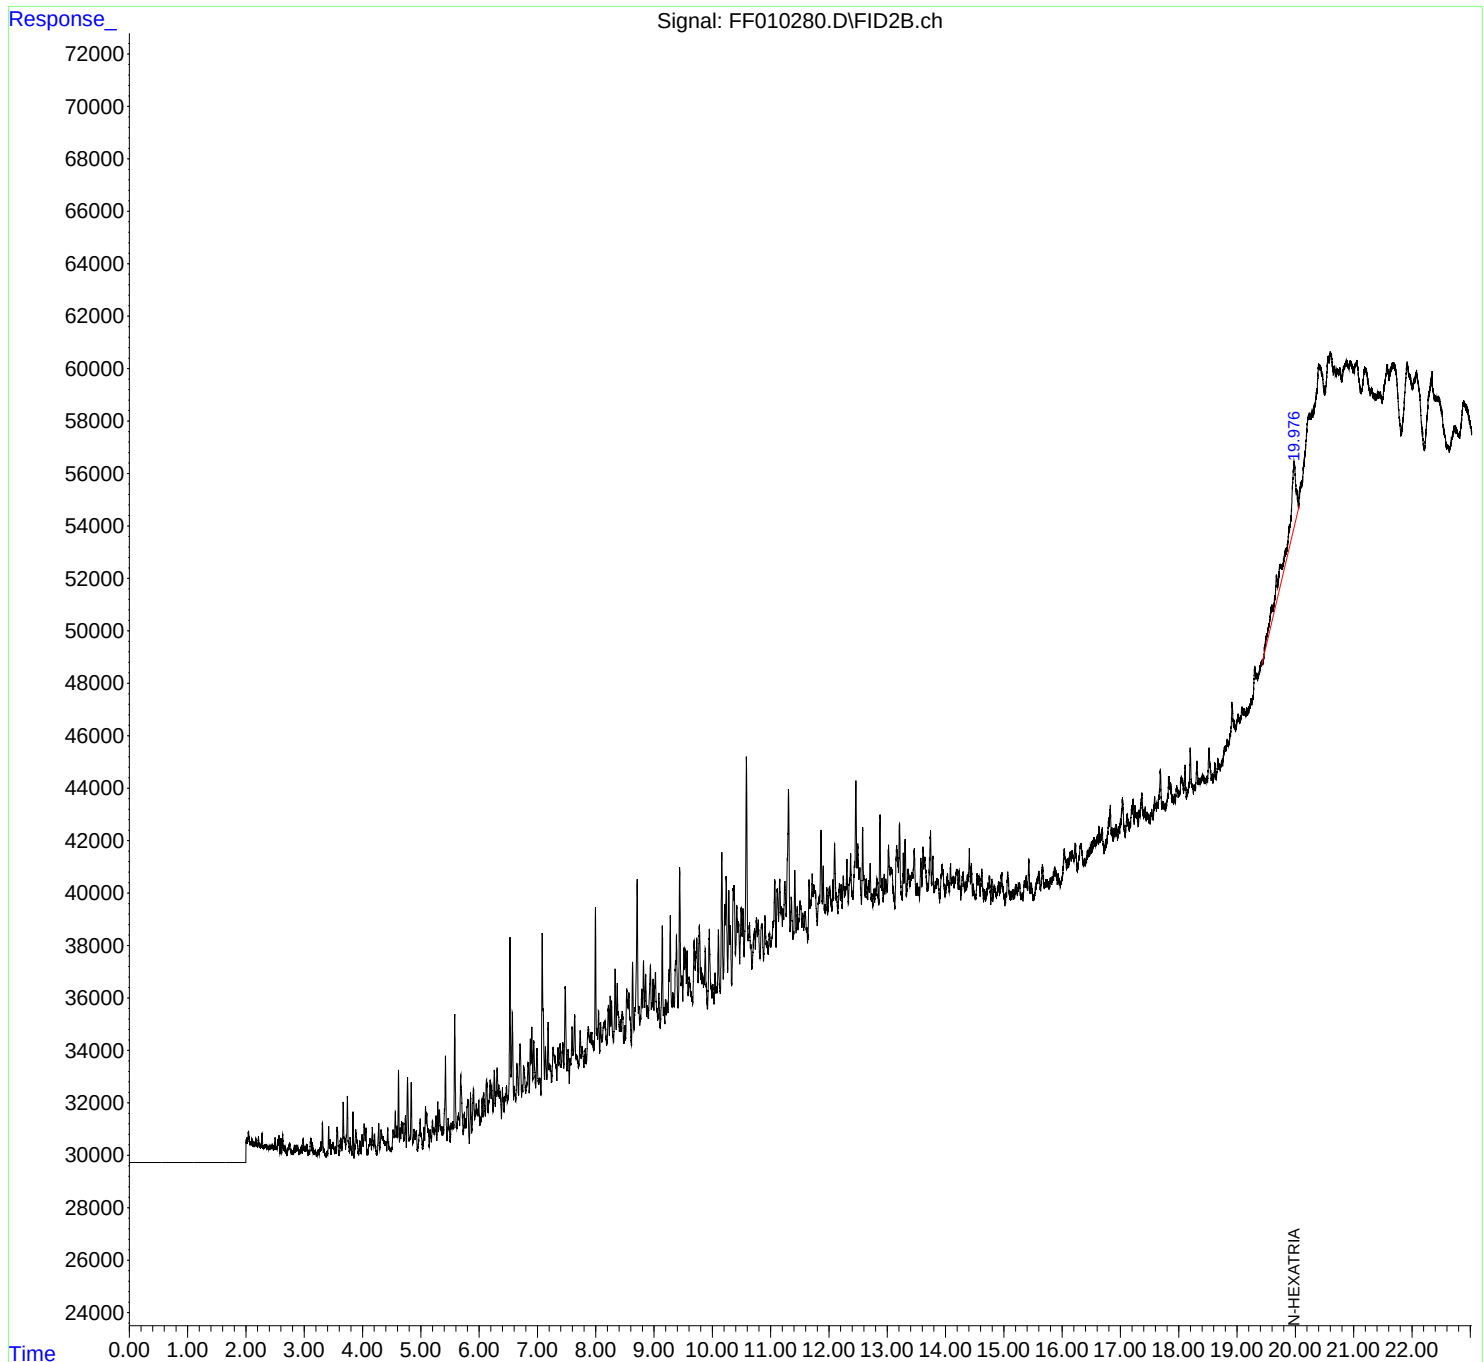


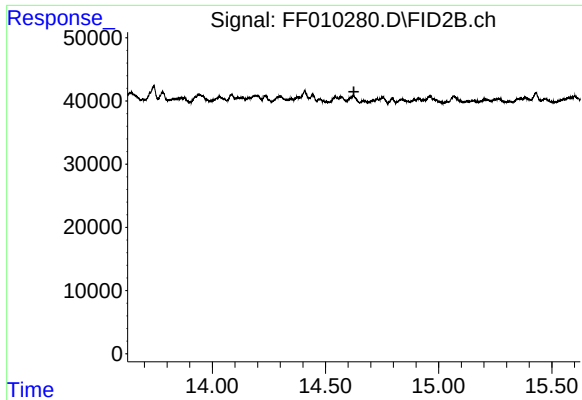

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.625 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

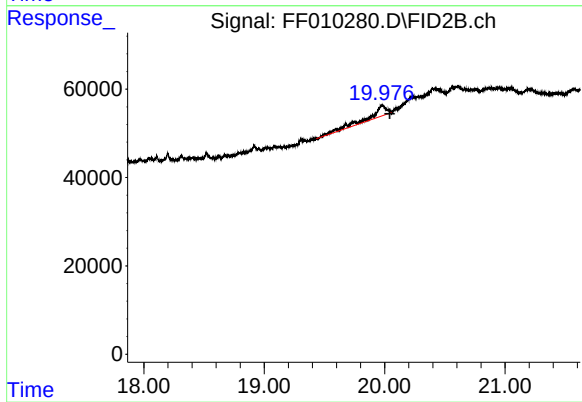

#16 N-HEXATRIACONTANE

R.T.: 19.978 min
Delta R.T.: -0.064 min
Response: 239546
Conc: 2.30 ug/ml