

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040722\
Data File : FF010281.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2022 12:08
Operator : AJ\MA
Sample : N2254-03 500X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 01:55:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

1)	N-OCTANE	2.277	194026	1.481 ug/ml
2)	N-DECANE	4.352	289748	2.179 ug/ml
3)	N-DODECANE	6.400	405388	3.045 ug/ml
4)	N-TETRADECANE	8.221	539505	4.069 ug/ml
5)	N-HEXADECANE	9.777	219979	1.657 ug/ml
7)	N-EICOSANE	12.463f	110975	0.826 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040722\
Data File : FF010281.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2022 12:08
Operator : AJ\MA
Sample : N2254-03 500X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 01:55:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

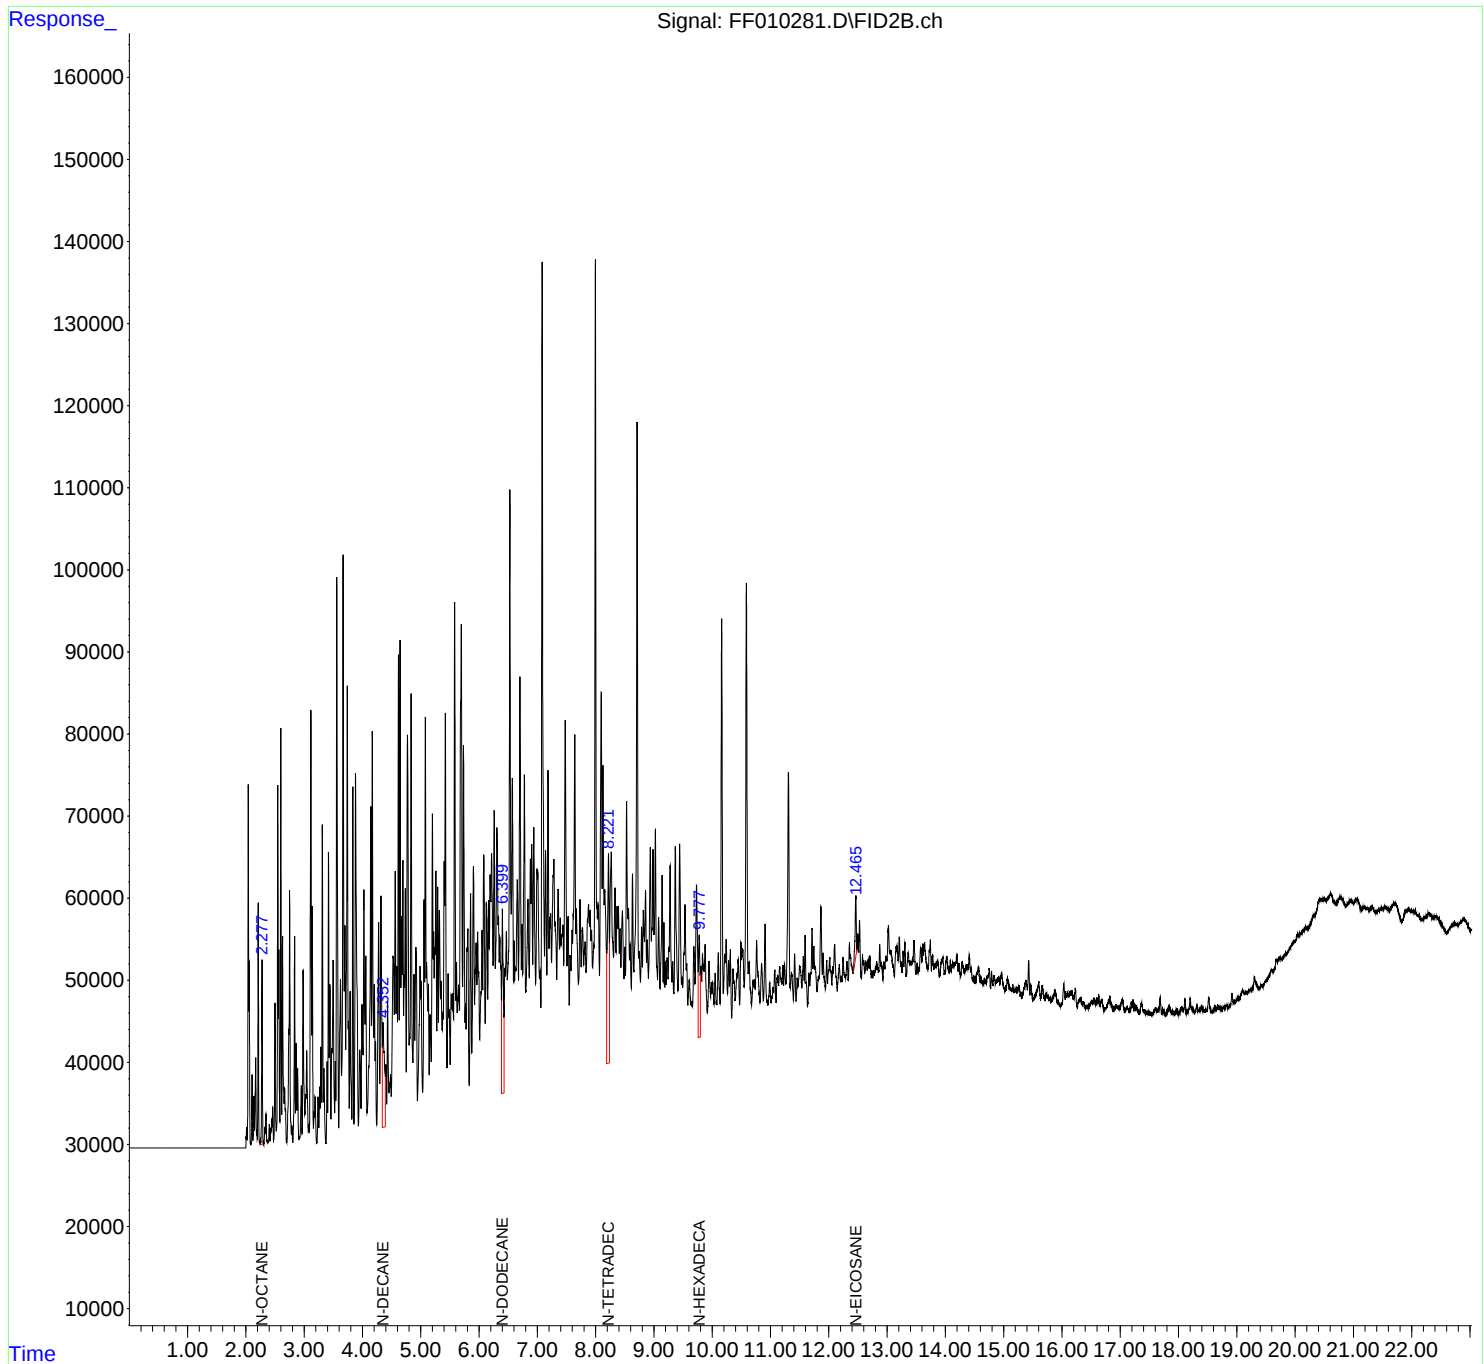


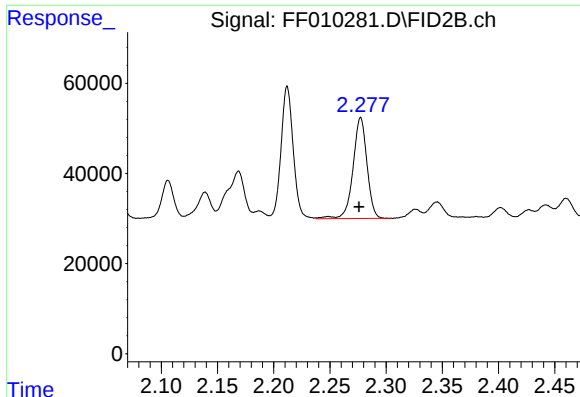

#1 N-OCTANE


R.T.: 2.277 min
Delta R.T.: 0.001 min
Response: 194026
Conc: 1.48 ug/ml

Instrument :
FID_F
ClientSampleId :

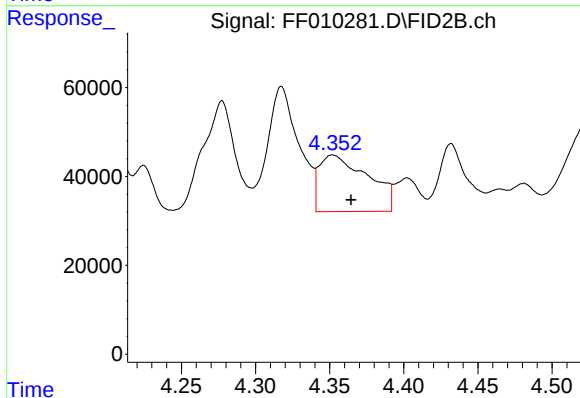


#2 N-DECANE

R.T.: 4.352 min
Delta R.T.: -0.012 min
Response: 289748
Conc: 2.18 ug/ml

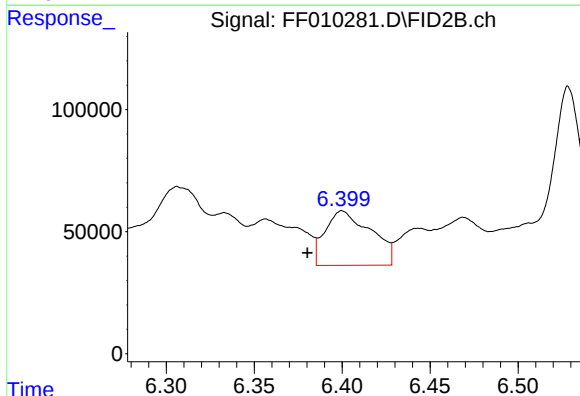


#3 N-DODECANE

R.T.: 6.400 min
Delta R.T.: 0.020 min
Response: 405388
Conc: 3.04 ug/ml

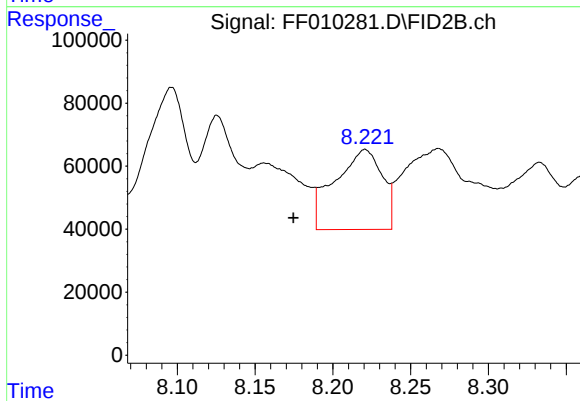

#4 N-TETRADECANE


R.T.: 8.221 min
Delta R.T.: 0.046 min
Response: 539505
Conc: 4.07 ug/ml

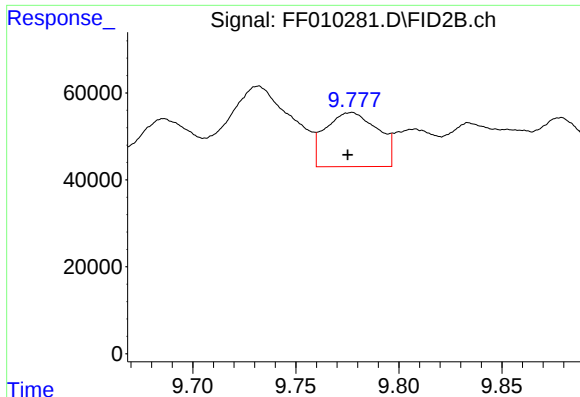

#5 N-HEXADECANE


R.T.: 9.777 min
Delta R.T.: 0.001 min
Response: 219979
Conc: 1.66 ug/ml

Instrument :
FID_F
ClientSampleId :

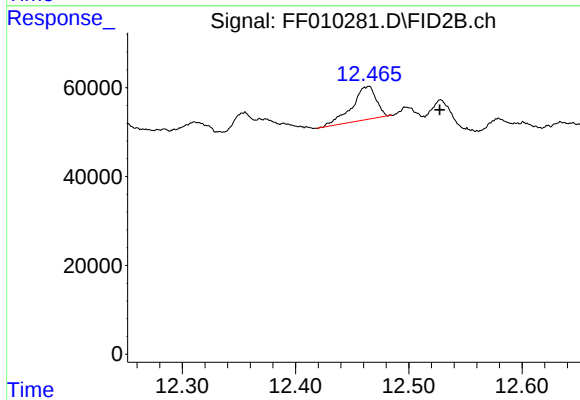

#7 N-EICOSANE

R.T.: 12.463 min
Delta R.T.: -0.064 min
Response: 110975
Conc: 0.83 ug/ml

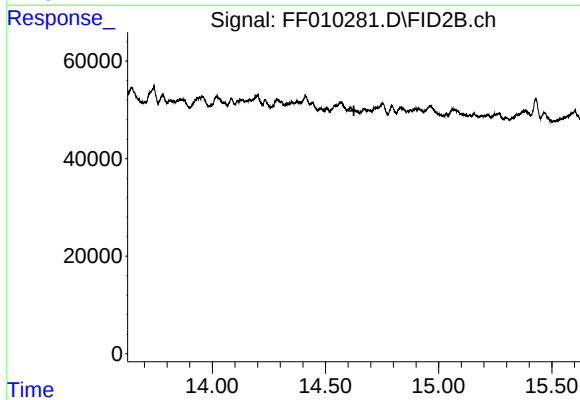

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.625 min
Response: 0
Conc: N.D.