

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040722\
 Data File : FF010294.D
 Signal(s) : FID2B.ch
 Acq On : 07 Apr 2022 20:25
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 08 01:59:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	2538345	21.236 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.694	132618	1.004 ug/ml
14) N-DOTRIACONTANE	18.527	24584	0.190 ug/ml
15) N-TETRATRIACONTANE	19.311	123642	1.062 ug/ml
16) N-HEXATRIACONTANE	20.053	488563	4.684 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040722\
Data File : FF010294.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2022 20:25
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 01:59:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

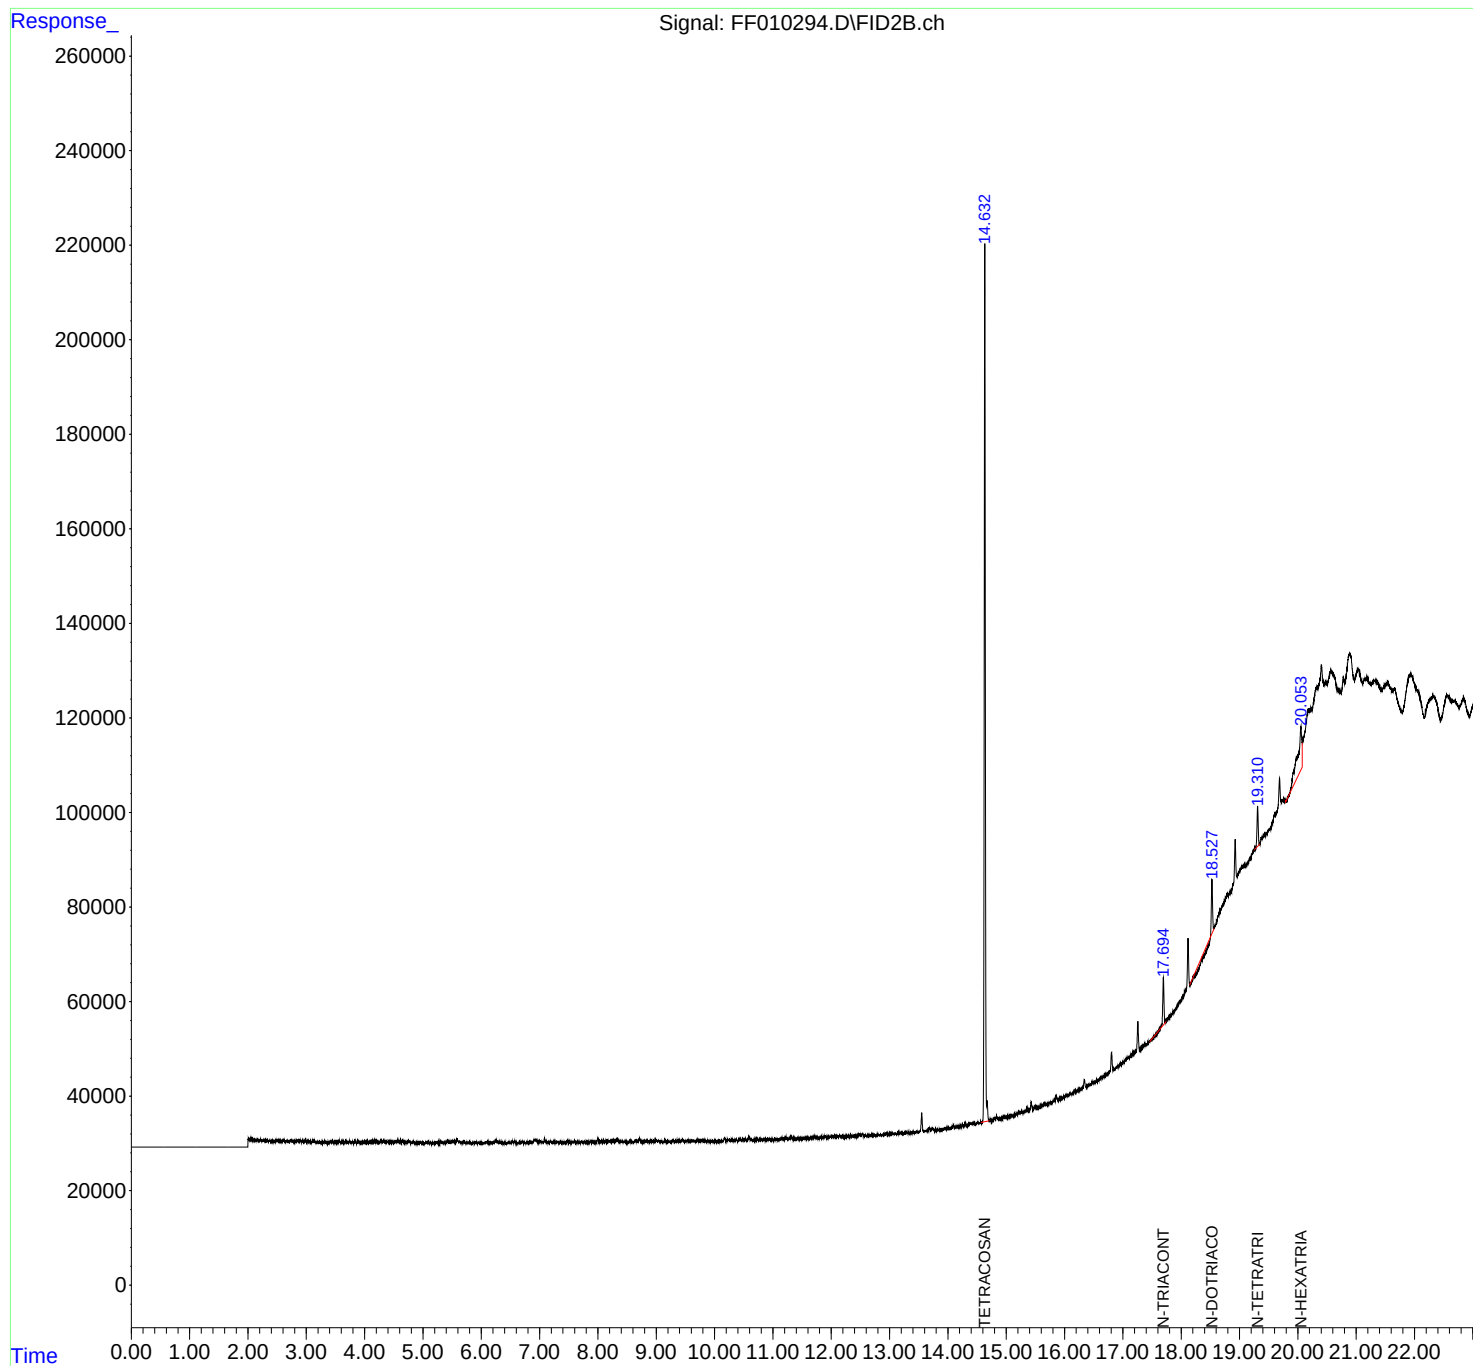


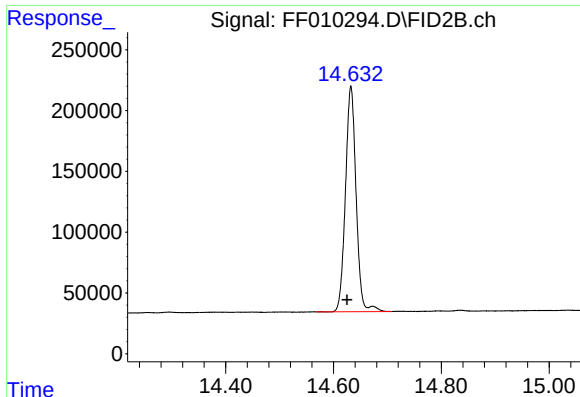

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.632 min
Delta R.T.: 0.007 min
Response: 2538345
Conc: 21.24 ug/ml

Instrument :
FID_F
ClientSampleId :

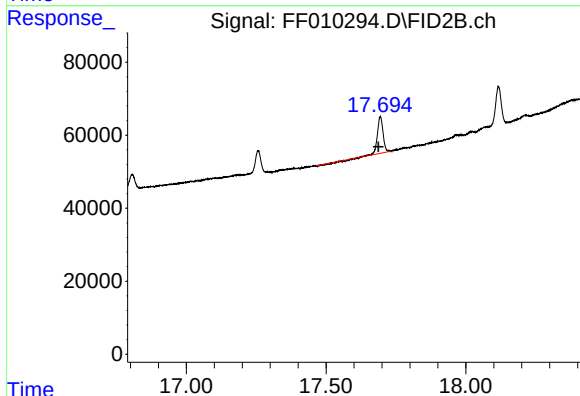


#13 N-TRIACONTANE

R.T.: 17.694 min
Delta R.T.: 0.007 min
Response: 132618
Conc: 1.00 ug/ml

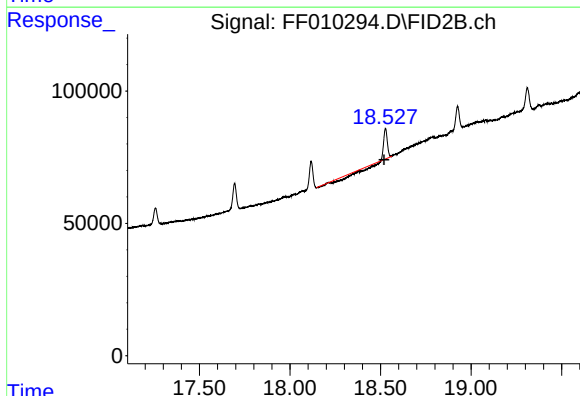


#14 N-DOTRIACONTANE

R.T.: 18.527 min
Delta R.T.: 0.007 min
Response: 24584
Conc: 0.19 ug/ml

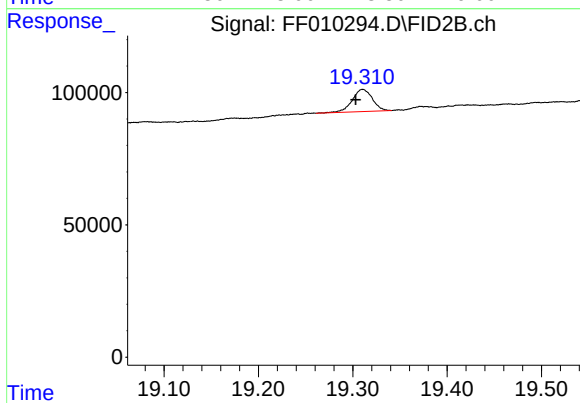

#15 N-TETRATRIACONTANE

R.T.: 19.311 min
Delta R.T.: 0.007 min
Response: 123642
Conc: 1.06 ug/ml

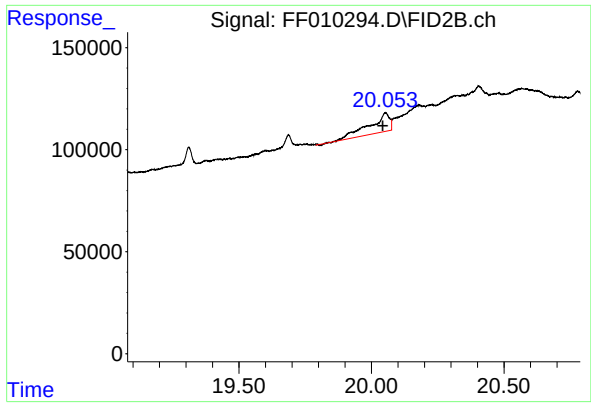

#16 N-HEXATRIACONTANE

R.T.: 20.053 min
Delta R.T.: 0.010 min
Response: 488563
Conc: 4.68 ug/ml

Instrument :
FID_F
ClientSampleId :