

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040722\
Data File : FF010287.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2022 16:54
Operator : AJ\MA
Sample : N2301-02
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-14A-1A-4-GR-2

Integration File: Sample.e
Quant Time: Apr 08 01:58:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.639	1944541	16.268 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040722\
Data File : FF010287.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2022 16:54
Operator : AJ\MA
Sample : N2301-02
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-14A-1A-4-GR-2

Integration File: Sample.e
Quant Time: Apr 08 01:58:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

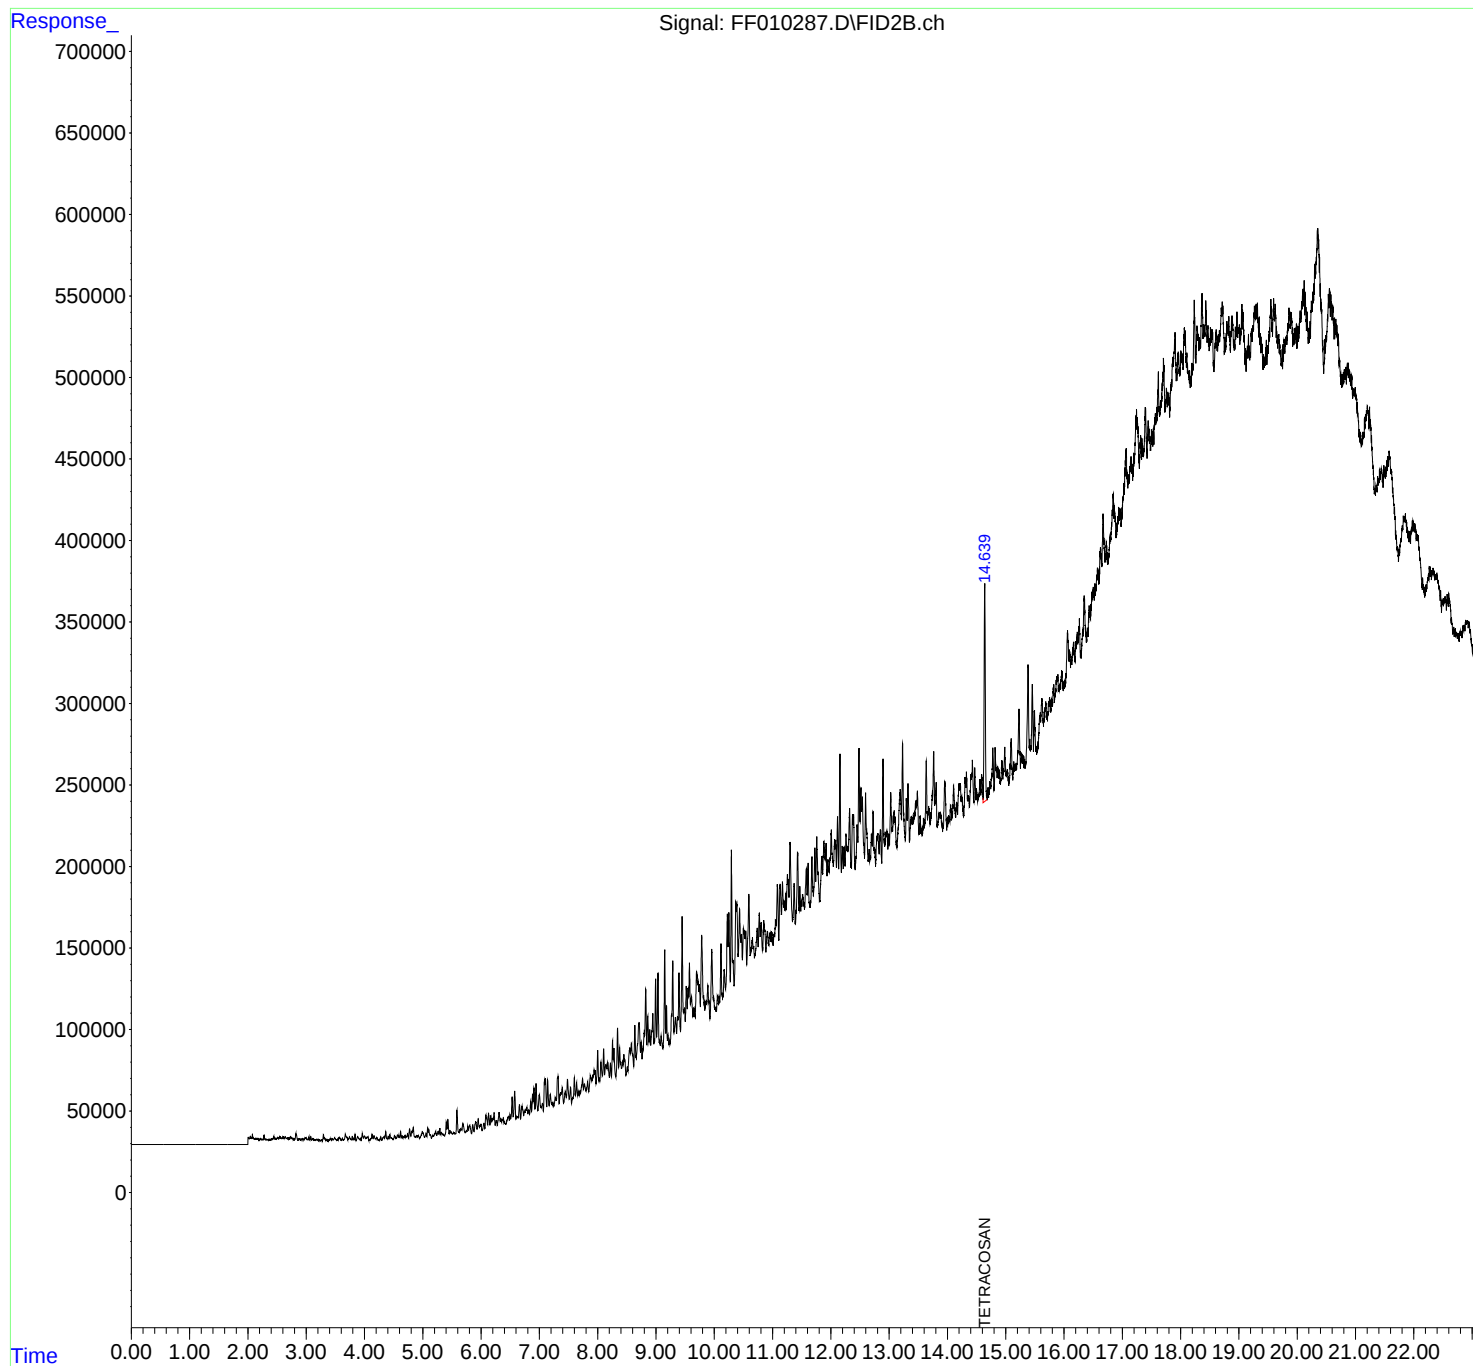

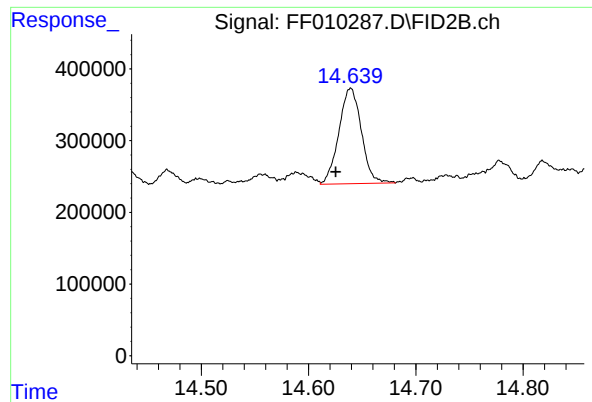

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.639 min
Delta R.T.: 0.014 min
Response: 1944541
Conc: 16.27 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-14A-1A-4-GR-2