

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040723\
 Data File : FF012396.D
 Signal(s) : FID2B.ch
 Acq On : 07 Apr 2023 08:21
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 10 02:38:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
8) N-DOCOSANE	14.107	63735	0.502 ug/ml
10) N-TETRACOSANE	15.194	377896	3.030 ug/ml
14) N-DOTRIACONTANE	18.910	106534	1.026 ug/ml
16) N-HEXATRIACONTANE	20.466	42753	0.488 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040723\
Data File : FF012396.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2023 08:21
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 02:38:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

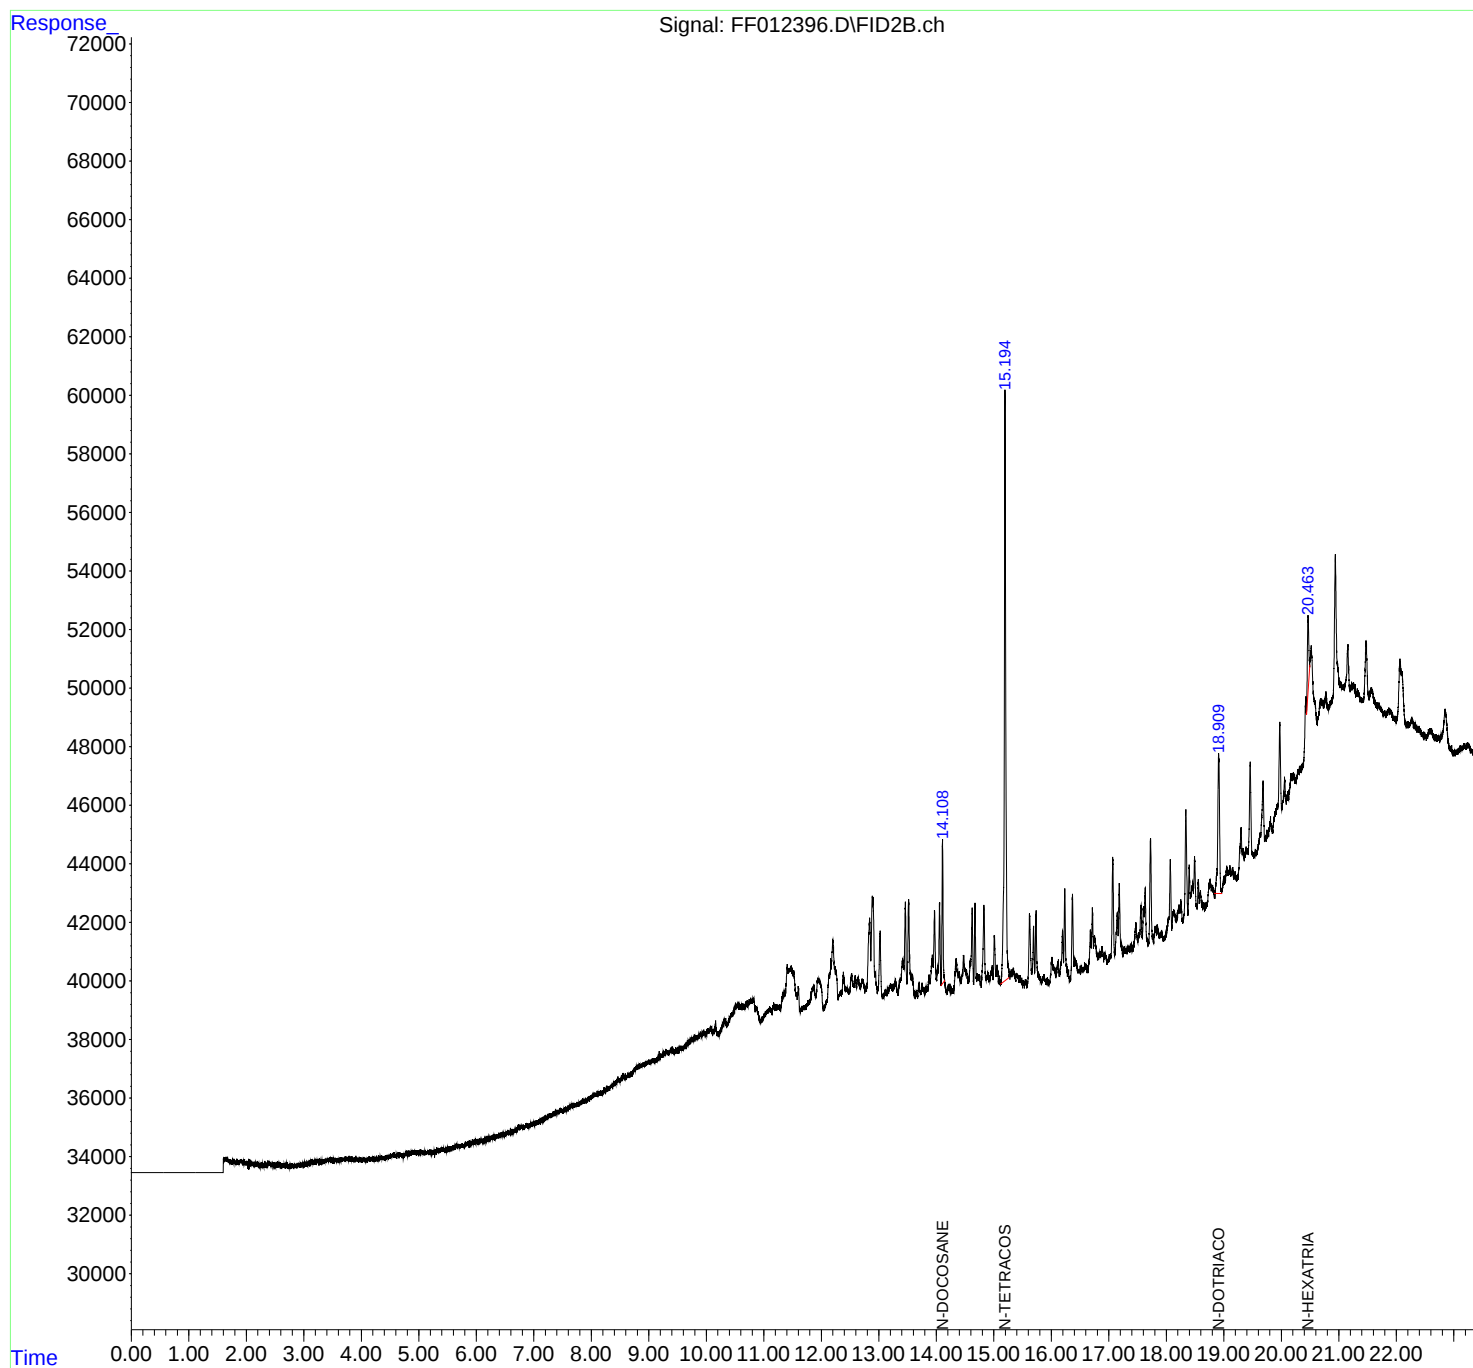


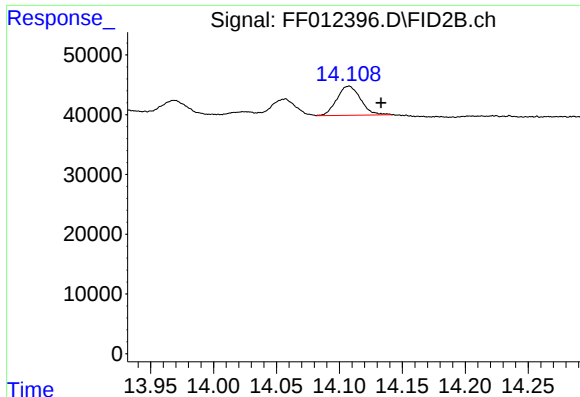

#8 N-DOCOSANE


R.T.: 14.107 min
Delta R.T.: -0.026 min
Response: 63735
Conc: 0.50 ug/ml

Instrument :
FID_F
ClientSampleId :

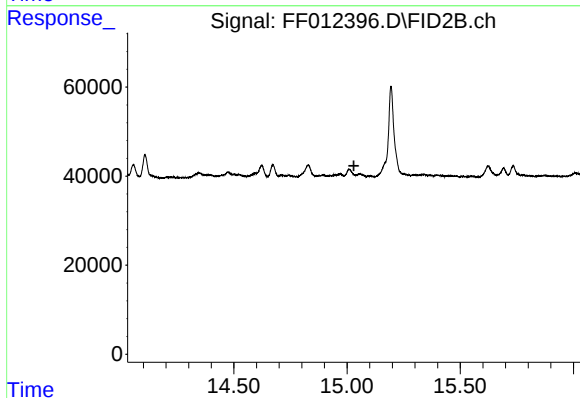


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.030 min
Response: 0
Conc: N.D.

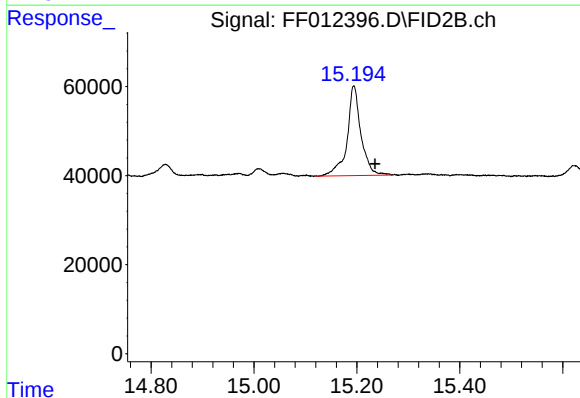


#10 N-TETRACOSANE

R.T.: 15.194 min
Delta R.T.: -0.041 min
Response: 377896
Conc: 3.03 ug/ml

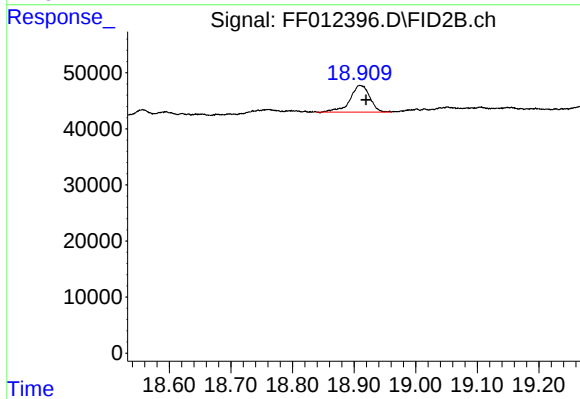

#14 N-DOTRIACONTANE

R.T.: 18.910 min
Delta R.T.: -0.010 min
Response: 106534
Conc: 1.03 ug/ml

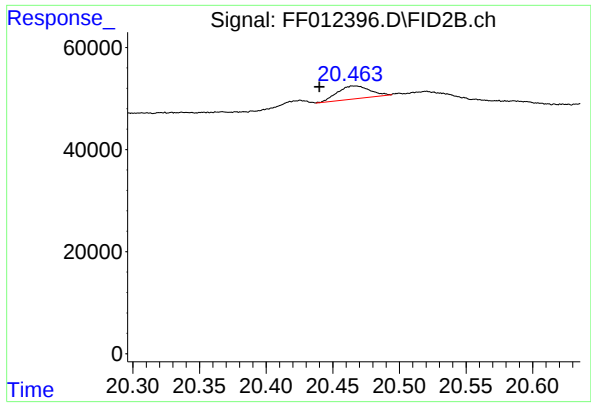

#16 N-HEXATRIACONTANE

R.T.: 20.466 min
Delta R.T.: 0.026 min
Response: 42753
Conc: 0.49 ug/ml

Instrument :
FID_F
ClientSampleId :