

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040723\
 Data File : FF012399.D
 Signal(s) : FID2B.ch
 Acq On : 07 Apr 2023 10:30
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 10 02:39:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.737	1695377	13.676 ug/ml
12)	N-OCTACOSANE	17.187	1903962	16.552 ug/ml
13)	N-TRIACONTANE	18.073	377355	3.429 ug/ml
14)	N-DOTRIACONTANE	18.903	520686	5.017 ug/ml
15)	N-TETRATRIACONTANE	19.686	421063	4.451 ug/ml
16)	N-HEXATRIACONTANE	20.427	264611	3.020 ug/ml
17)	N-OCTATRIACONTANE	21.162	186017	2.247 ug/ml
18)	N-TETRACONTANE	22.070	137514	1.683 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040723\
Data File : FF012399.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2023 10:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 02:39:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

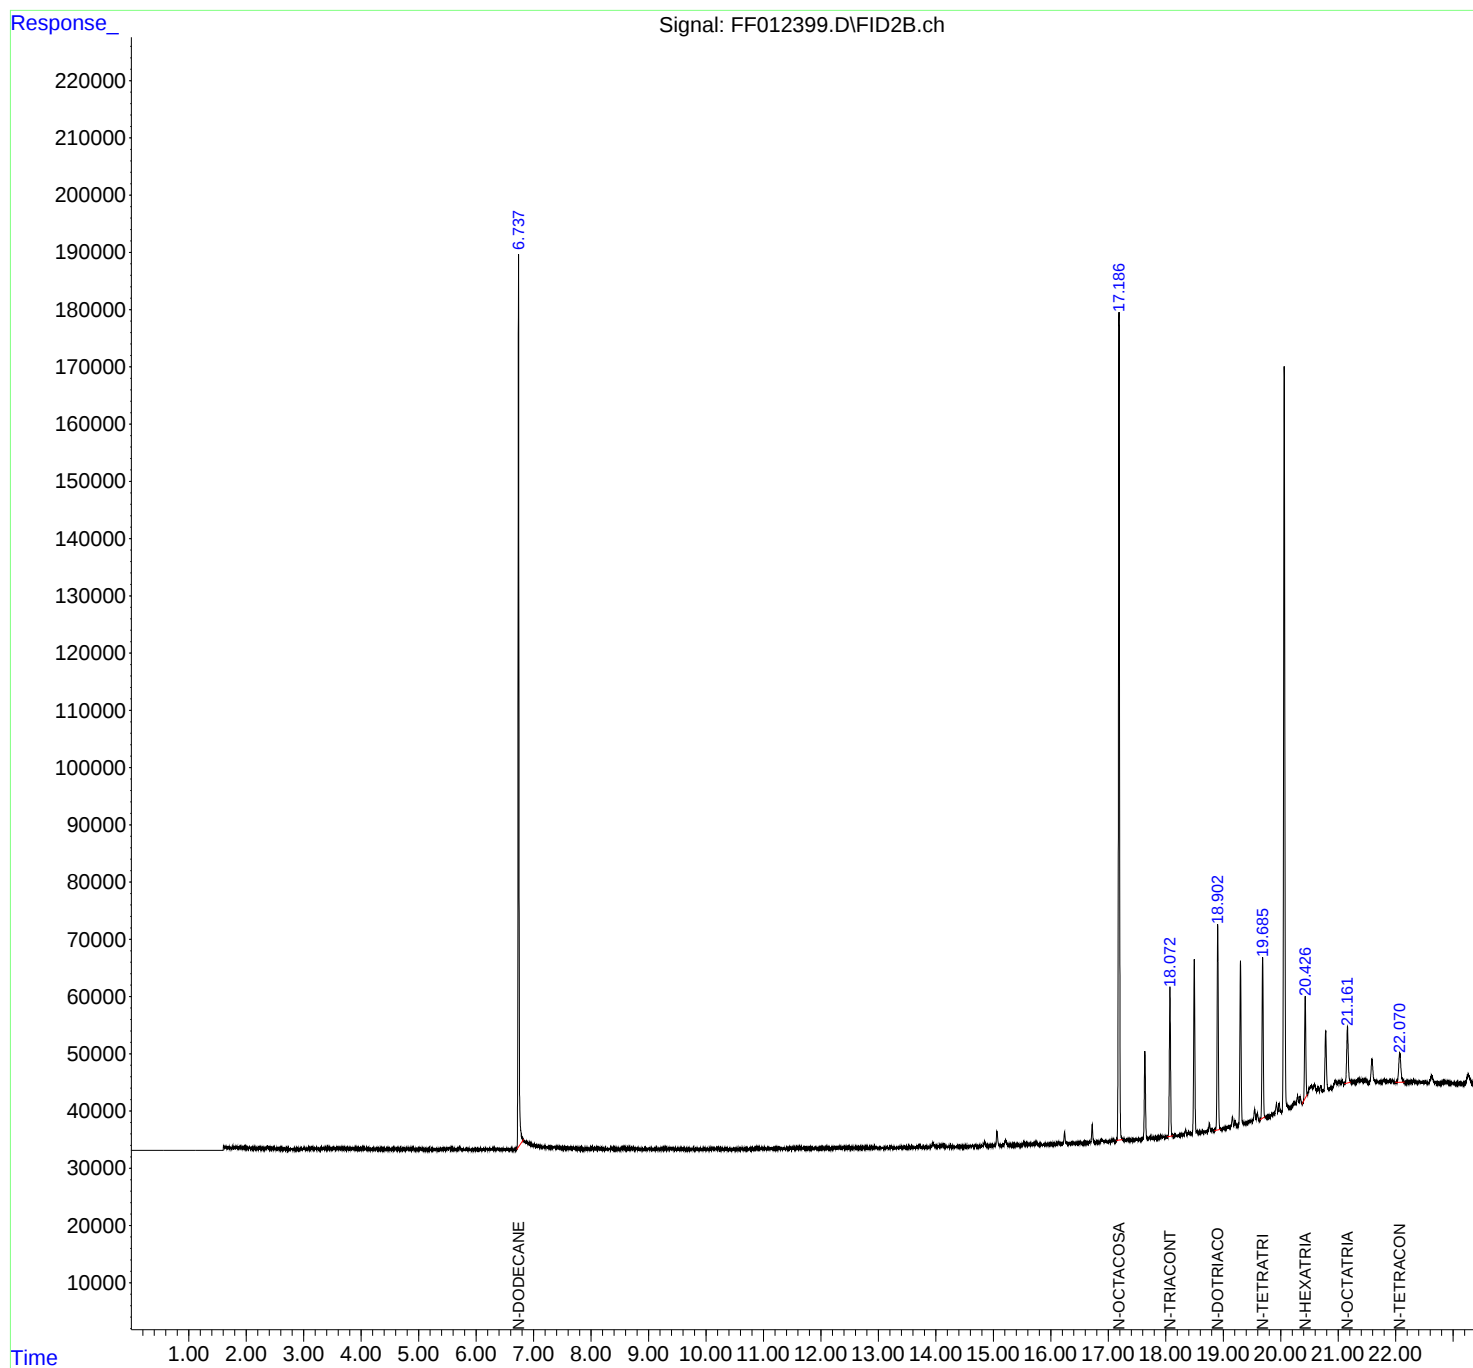


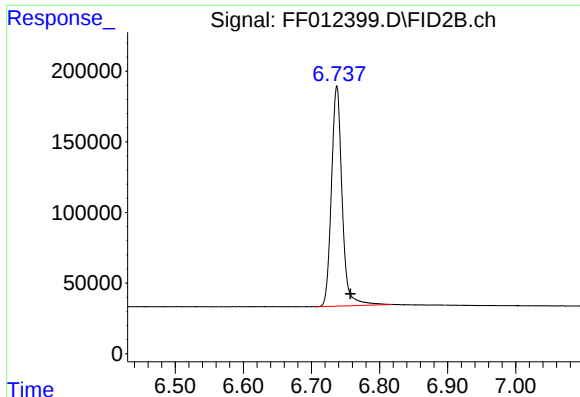

#3 N-DODECANE


R.T.: 6.737 min
Delta R.T.: -0.020 min
Response: 1695377
Conc: 13.68 ug/ml

Instrument :
FID_F
ClientSampleId :

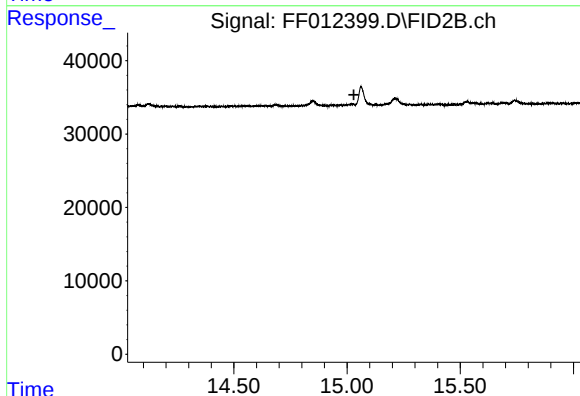


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.030 min
Response: 0
Conc: N.D.

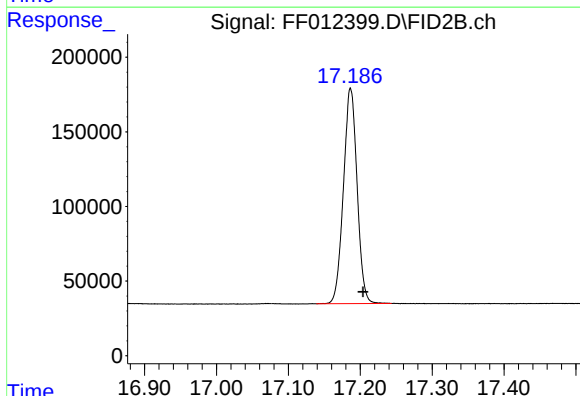


#12 N-OCTACOSANE

R.T.: 17.187 min
Delta R.T.: -0.018 min
Response: 1903962
Conc: 16.55 ug/ml

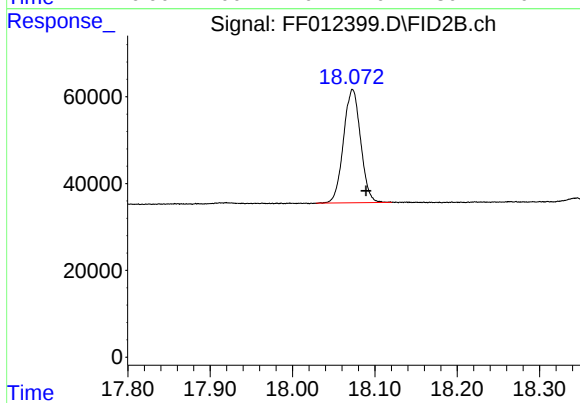

#13 N-TRIACONTANE

R.T.: 18.073 min
Delta R.T.: -0.016 min
Response: 377355
Conc: 3.43 ug/ml

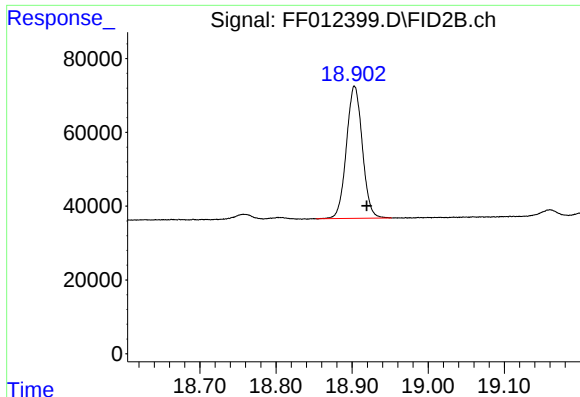


#14 N-DOTRIACONTANE

R.T.: 18.903 min
Delta R.T.: -0.016 min
Response: 520686
Conc: 5.02 ug/ml

Instrument :


FID_F

ClientSampleId :

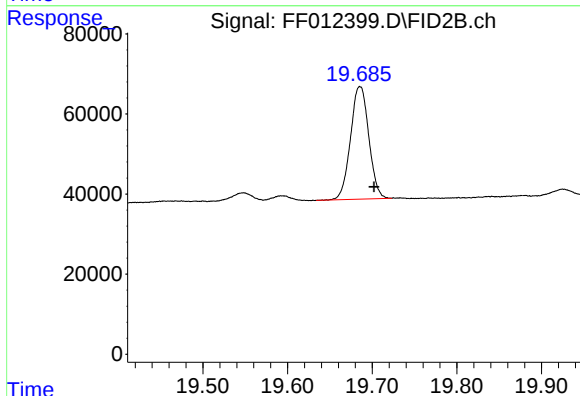


#15 N-TETRATRIACONTANE

R.T.: 19.686 min
Delta R.T.: -0.017 min
Response: 421063
Conc: 4.45 ug/ml

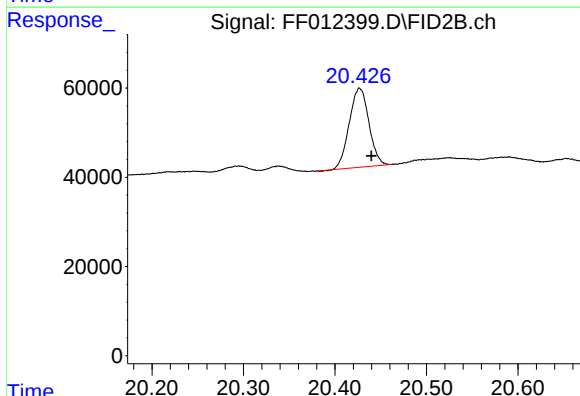


#16 N-HEXATRIACONTANE

R.T.: 20.427 min
Delta R.T.: -0.013 min
Response: 264611
Conc: 3.02 ug/ml

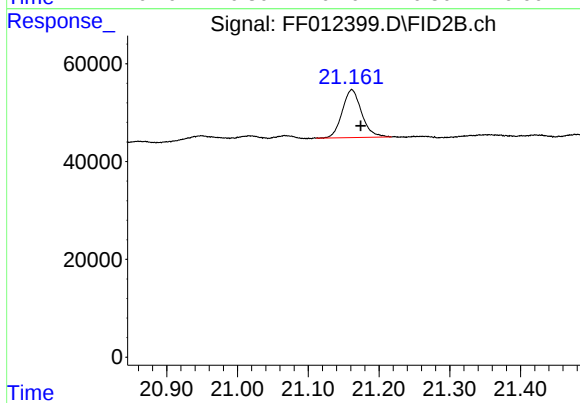

#17 N-OCTATRIACONTANE

R.T.: 21.162 min
Delta R.T.: -0.013 min
Response: 186017
Conc: 2.25 ug/ml

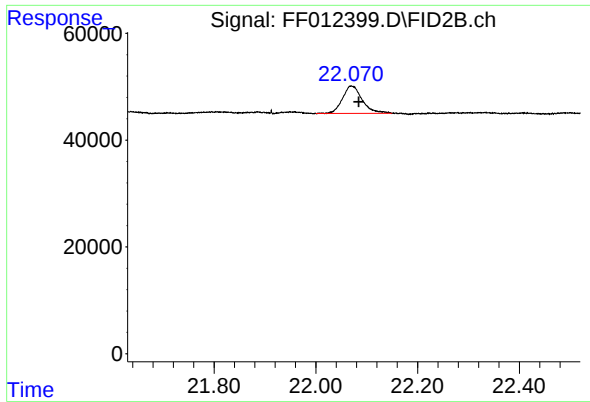

#18 N-TETRACONTANE

R.T.: 22.070 min
Delta R.T.: -0.015 min
Response: 137514
Conc: 1.68 ug/ml

Instrument :
FID_F
ClientSampleId :