

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040723\
Data File : FF012399.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2023 10:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 10 02:39:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.737	1695377	13.676 ug/ml
12)	N-OCTACOSANE	17.187	1903962	16.552 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040723\
Data File : FF012399.D
Signal(s) : FID2B.ch
Acq On : 07 Apr 2023 10:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Apr 10 02:39:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

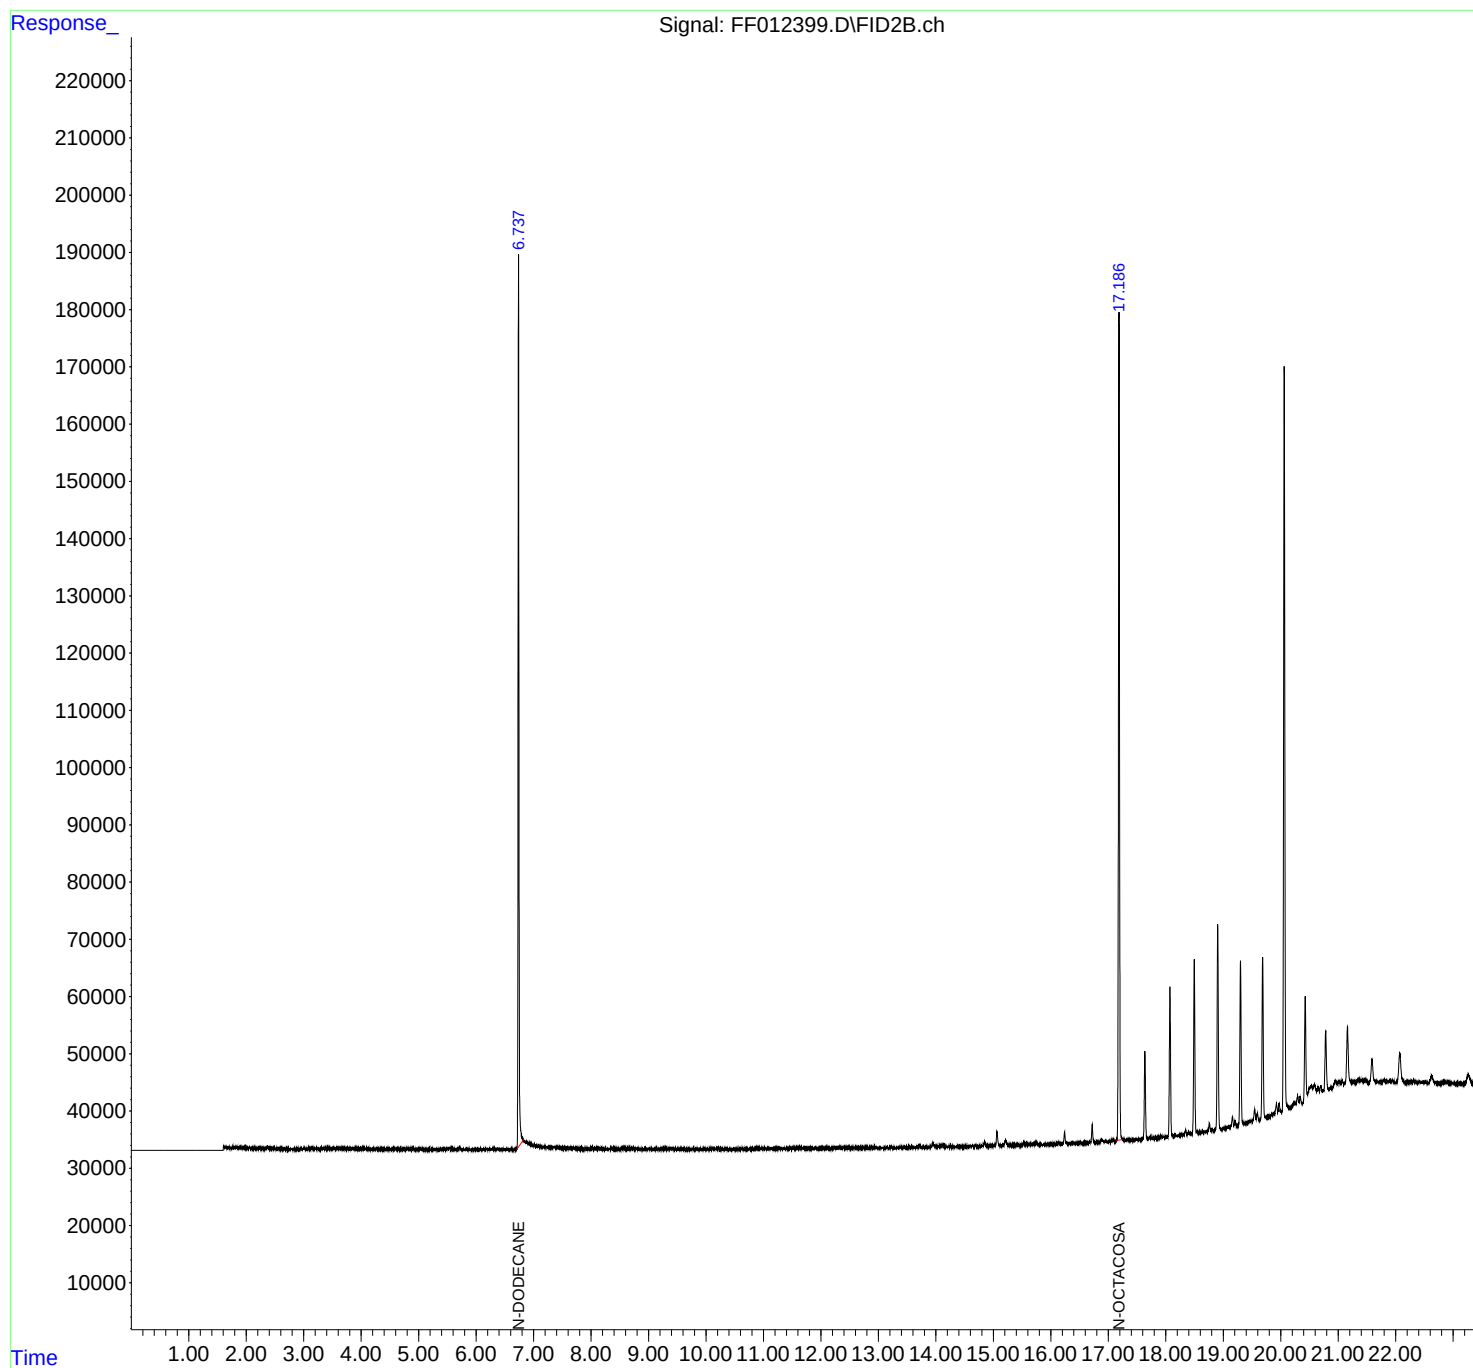


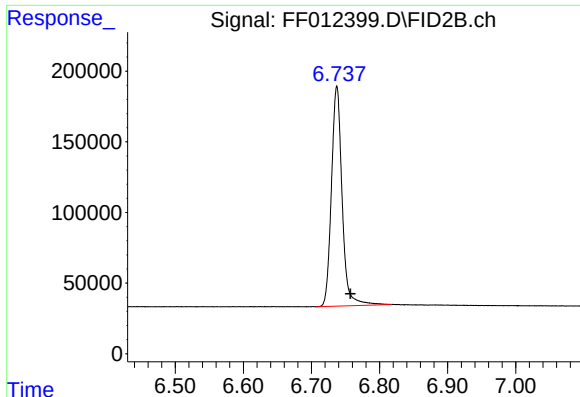

#3 N-DODECANE


R.T.: 6.737 min
Delta R.T.: -0.020 min
Response: 1695377
Conc: 13.68 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

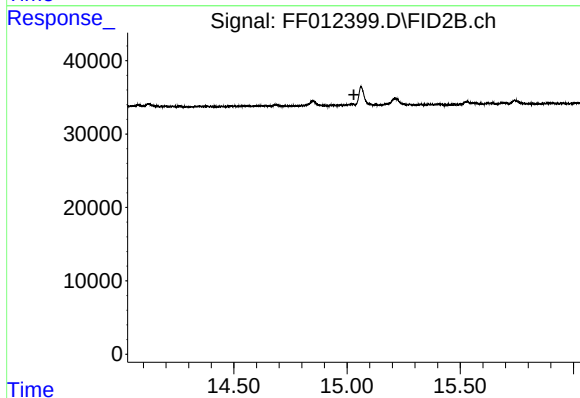

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.030 min
Response: 0
Conc: N.D.

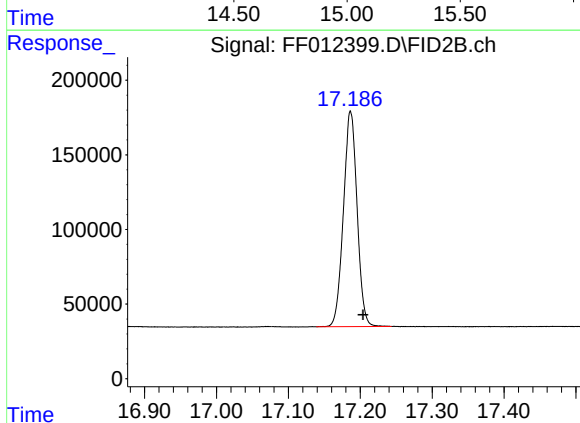

#12 N-OCTACOSANE

R.T.: 17.187 min
Delta R.T.: -0.018 min
Response: 1903962
Conc: 16.55 ug/ml