

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040820\
 Data File : FF006793.D
 Signal(s) : FID2B.ch
 Acq On : 08 Apr 2020 11:39
 Operator : DD\AJ
 Sample : L2117-01 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 09 00:53:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.577	338764	2.632 ug/ml
Target Compounds			
4) N-TETRADECANE	8.209	163795	1.145 ug/ml
7) N-EICOSANE	12.477	64662	0.435 ug/ml
8) N-DOCOSANE	13.679	124129	0.836 ug/ml
10) N-TETRACOSANE	14.771	715387	4.840 ug/ml
11) N-HEXACOSANE	15.796	72902	0.503 ug/ml
12) N-OCTACOSANE	16.743	185577	1.296 ug/ml
13) N-TRIACONTANE	17.627	388154	2.742 ug/ml
14) N-DOTRIACONTANE	18.454	473328	3.511 ug/ml
15) N-TETRATRIACONTANE	19.237	181734	1.609 ug/ml
16) N-HEXATRIACONTANE	19.976	246967	2.689 ug/ml
17) N-OCTATRIACONTANE	20.683	185446	2.686 ug/ml
18) N-TETRACONTANE	21.566	239520	3.461 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040820\
 Data File : FF006793.D
 Signal(s) : FID2B.ch
 Acq On : 08 Apr 2020 11:39
 Operator : DD\AJ
 Sample : L2117-01 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1


Integration File: autoint1.e
 Quant Time: Apr 09 00:53:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

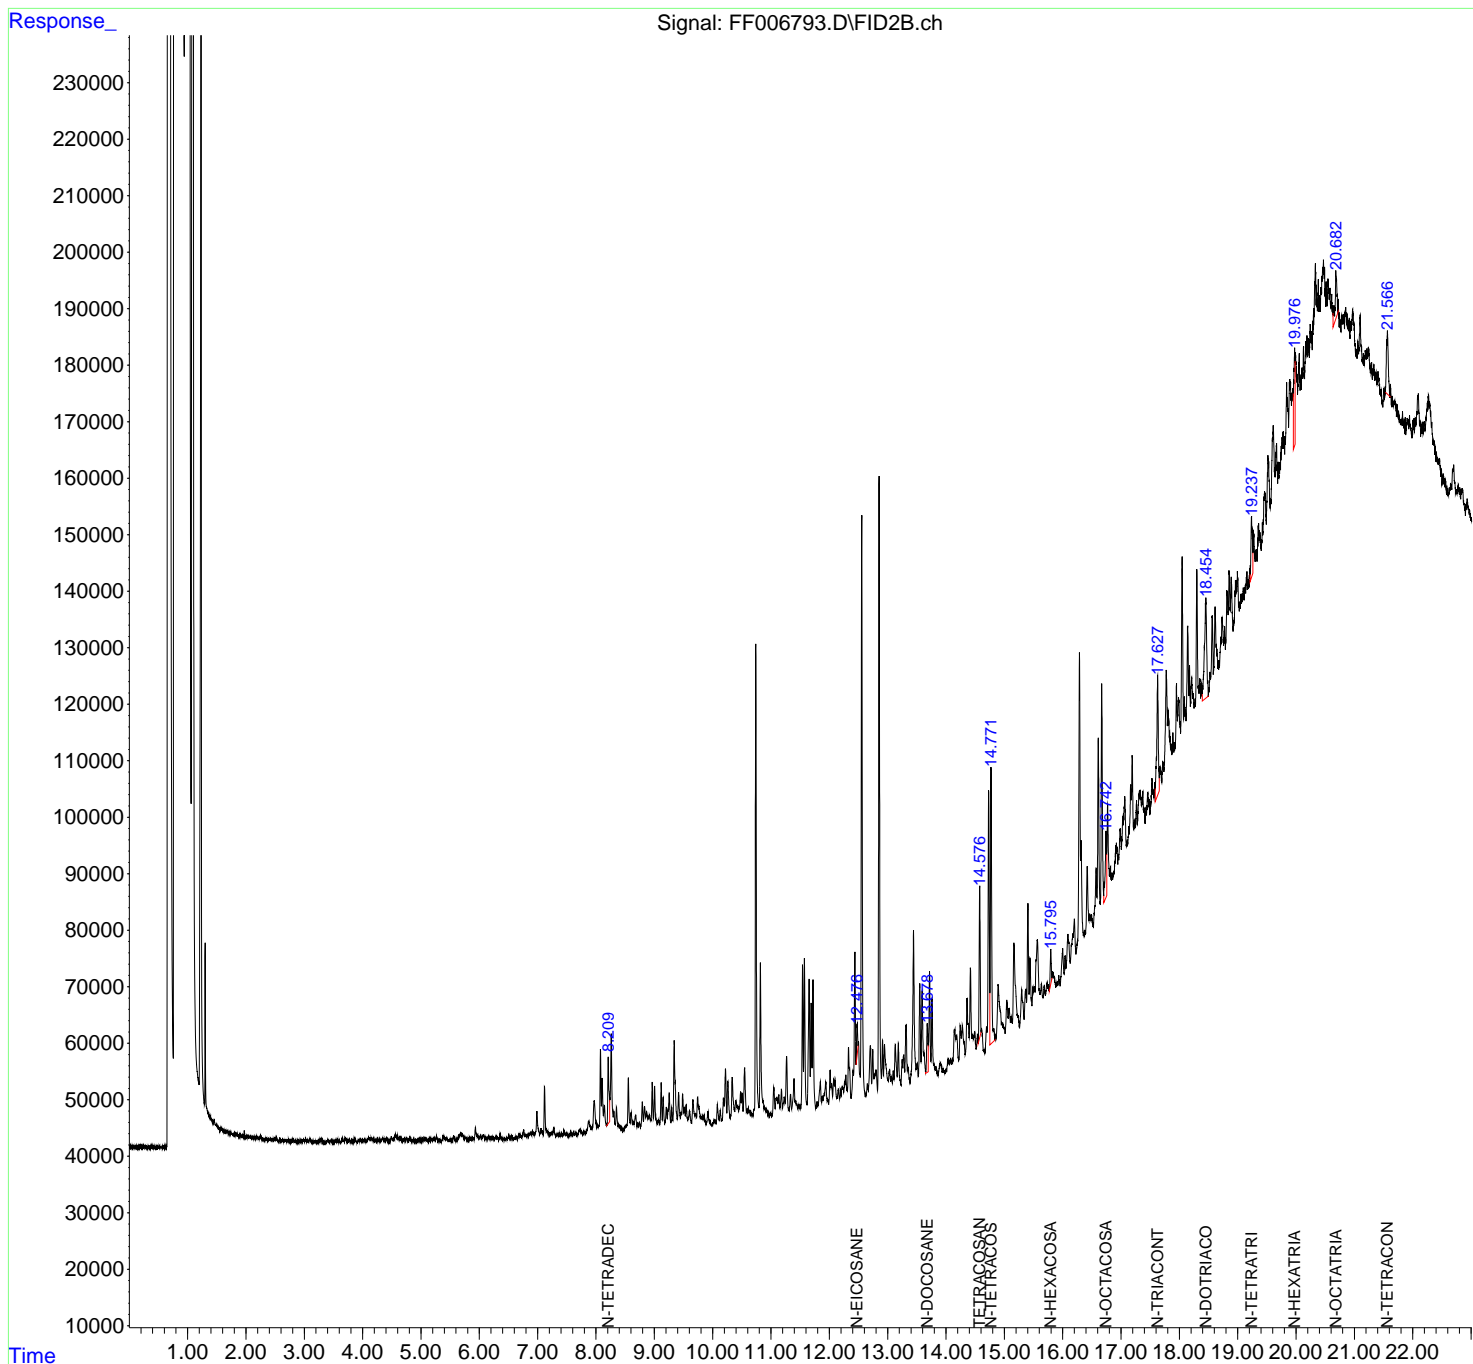


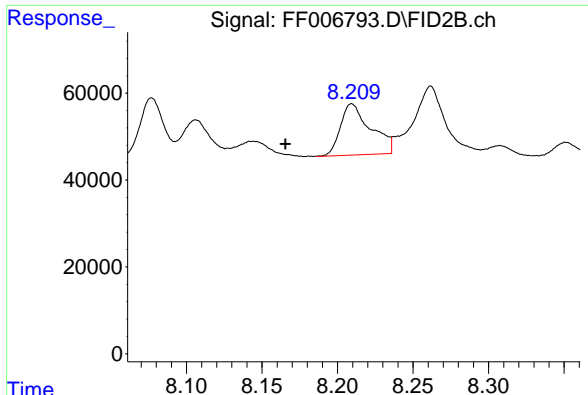


#4 N-TETRADECANE
R.T.: 8.209 min
Delta R.T.: 0.044 min
Response: 163795
Conc: 1.15 ug/ml

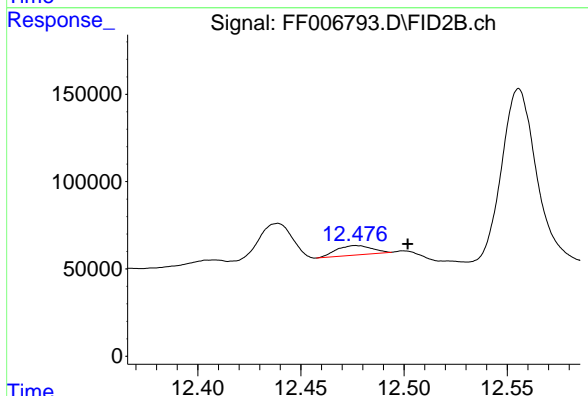


#7 N-EICOSANE
R.T.: 12.477 min
Delta R.T.: -0.025 min
Response: 64662
Conc: 0.44 ug/ml

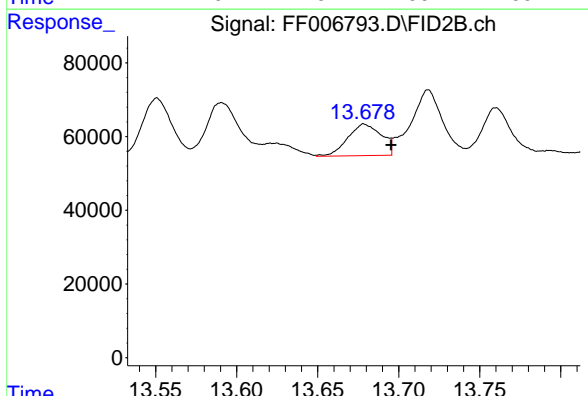

#8 N-DOCOSANE
R.T.: 13.679 min
Delta R.T.: -0.017 min
Response: 124129
Conc: 0.84 ug/ml

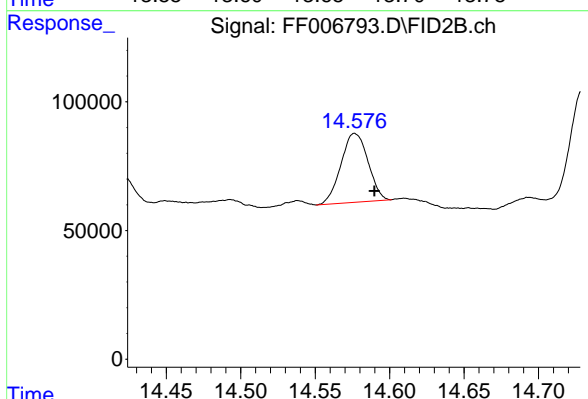


#9 TETRACOSANE-d50 (SURROGATE)
R.T.: 14.577 min
Delta R.T.: -0.013 min
Response: 338764
Conc: 2.63 ug/ml

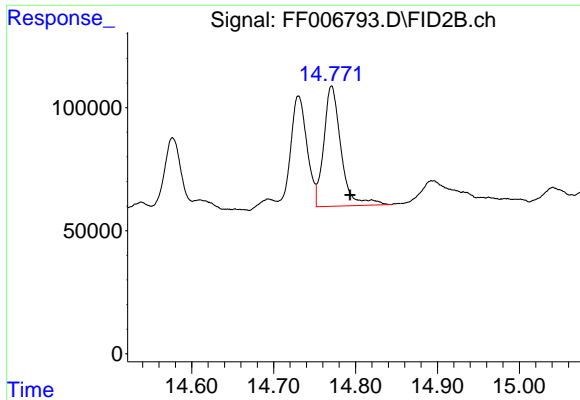


#10 N-TETRACOSANE

R.T.: 14.771 min
Delta R.T.: -0.023 min
Response: 715387
Conc: 4.84 ug/ml

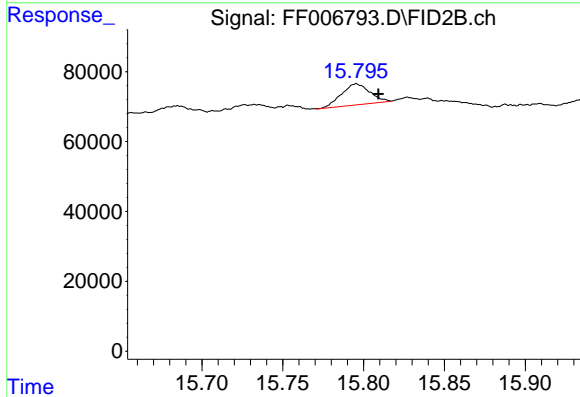


#11 N-HEXACOSANE

R.T.: 15.796 min
Delta R.T.: -0.014 min
Response: 72902
Conc: 0.50 ug/ml

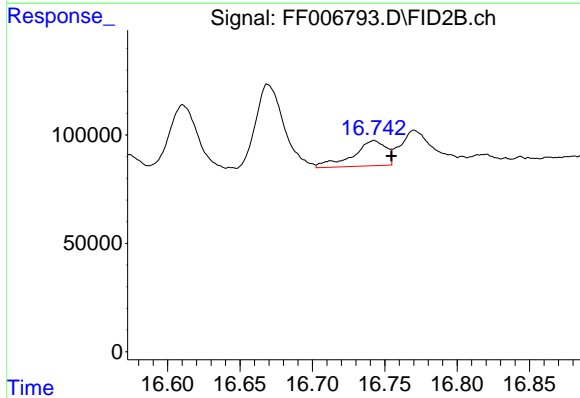


#12 N-OCTACOSANE

R.T.: 16.743 min
Delta R.T.: -0.012 min
Response: 185577
Conc: 1.30 ug/ml

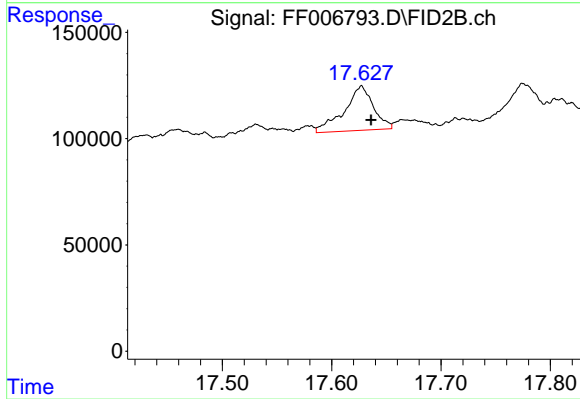


#13 N-TRIACONTANE

R.T.: 17.627 min
Delta R.T.: -0.009 min
Response: 388154
Conc: 2.74 ug/ml

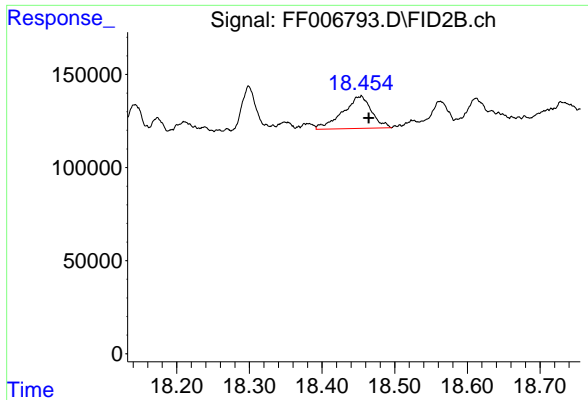


#14 N-DOTRIACONTANE

R.T.: 18.454 min
Delta R.T.: -0.010 min
Response: 473328
Conc: 3.51 ug/ml

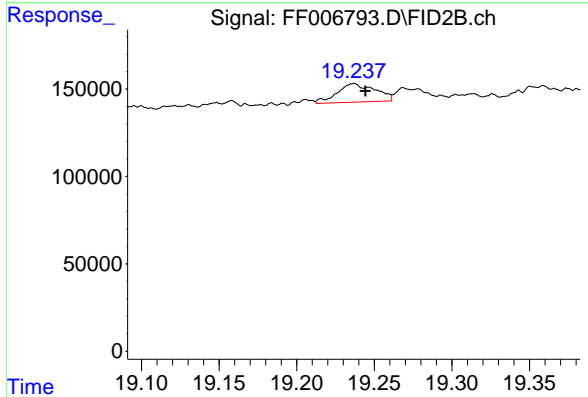


#15 N-TETRATRIACONTANE

R.T.: 19.237 min
Delta R.T.: -0.007 min
Response: 181734
Conc: 1.61 ug/ml

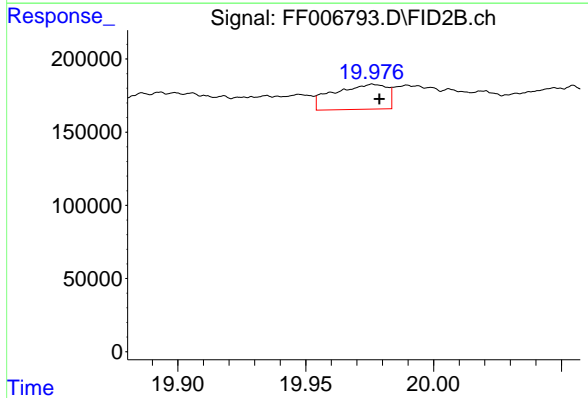


#16 N-HEXATRIACONTANE

R.T.: 19.976 min
Delta R.T.: -0.002 min
Response: 246967
Conc: 2.69 ug/ml

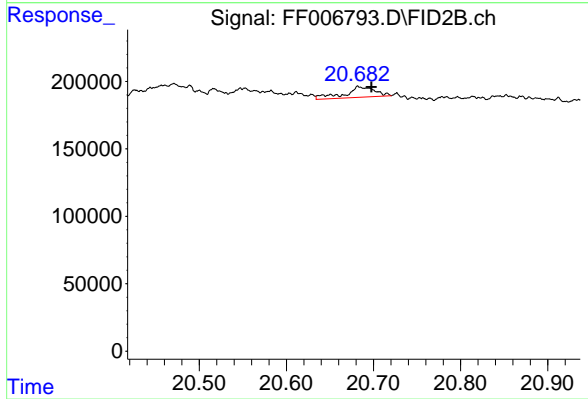

#17 N-OCTATRIACONTANE

R.T.: 20.683 min
Delta R.T.: -0.015 min
Response: 185446
Conc: 2.69 ug/ml

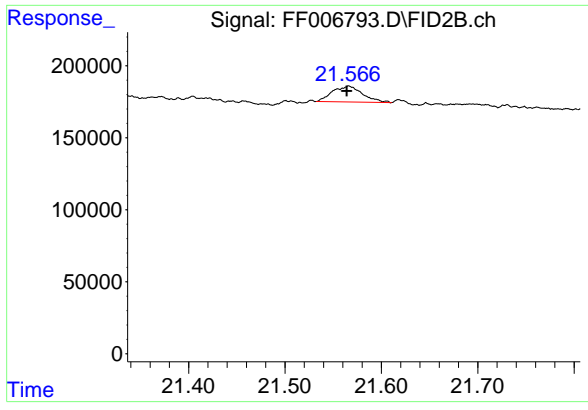

#18 N-TETRACONTANE

R.T.: 21.566 min
Delta R.T.: 0.002 min
Response: 239520
Conc: 3.46 ug/ml