

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040822\
 Data File : FF010297.D
 Signal(s) : FID2B.ch
 Acq On : 08 Apr 2022 08:55
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 08 23:26:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	2974761	24.887 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.694	172709	1.308 ug/ml
14) N-DOTRIACONTANE	18.526	258069	1.999 ug/ml
15) N-TETRATRIACONTANE	19.310	152895	1.314 ug/ml
16) N-HEXATRIACONTANE	20.050	104470	1.002 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040822\
Data File : FF010297.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2022 08:55
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 23:26:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

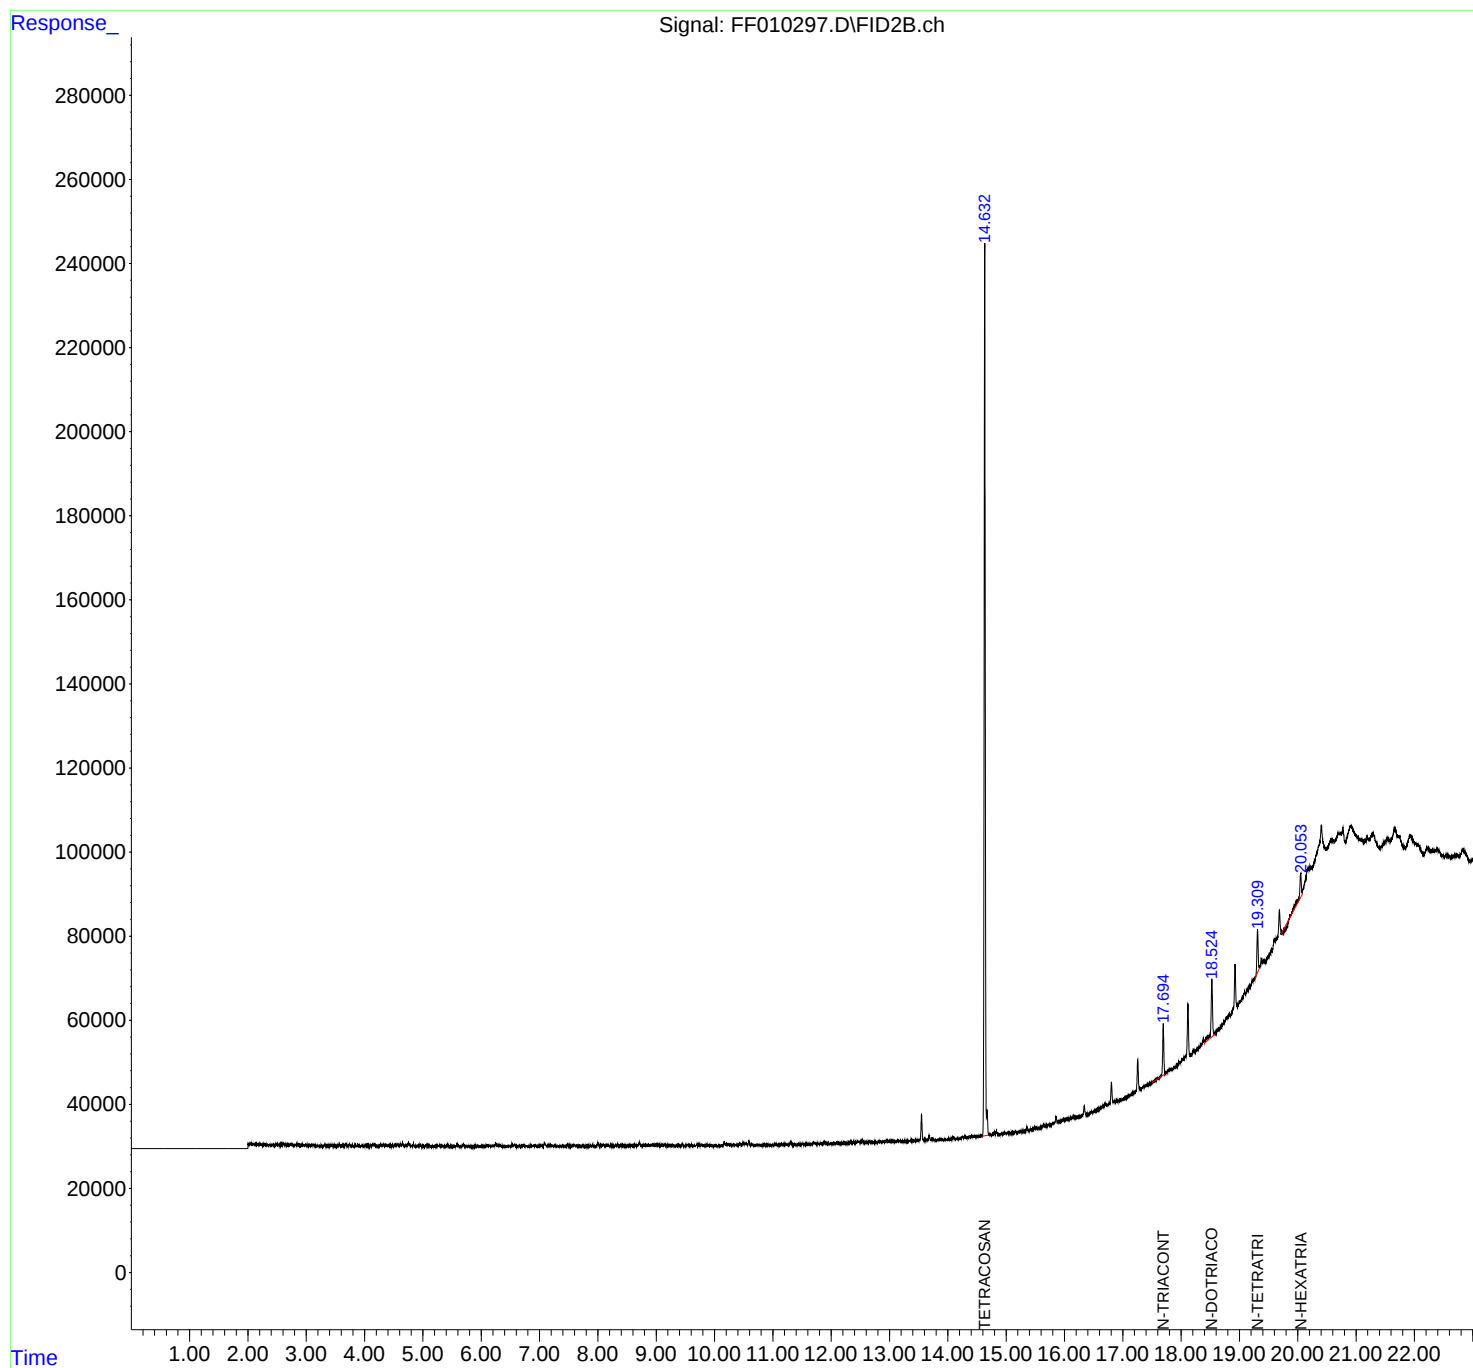


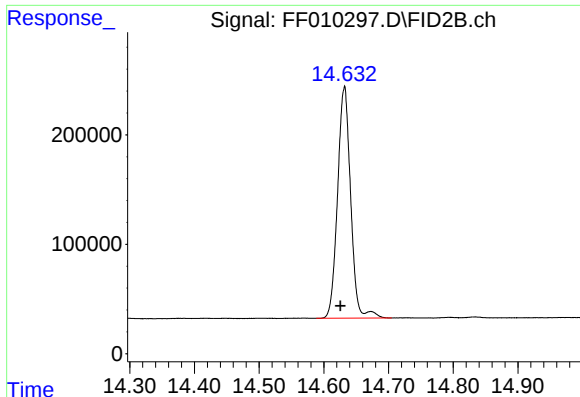

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.632 min
Delta R.T.: 0.006 min
Response: 2974761
Conc: 24.89 ug/ml

Instrument :
FID_F
ClientSampleId :

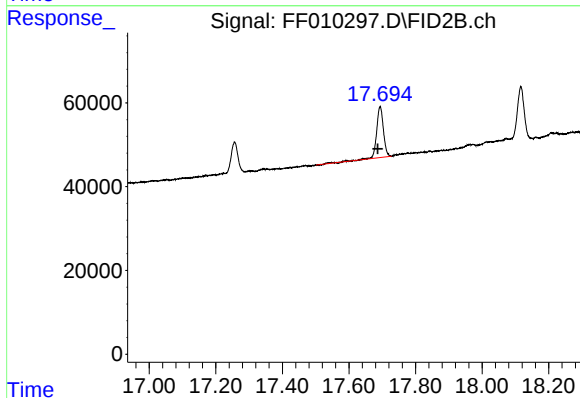


#13 N-TRIACONTANE

R.T.: 17.694 min
Delta R.T.: 0.007 min
Response: 172709
Conc: 1.31 ug/ml

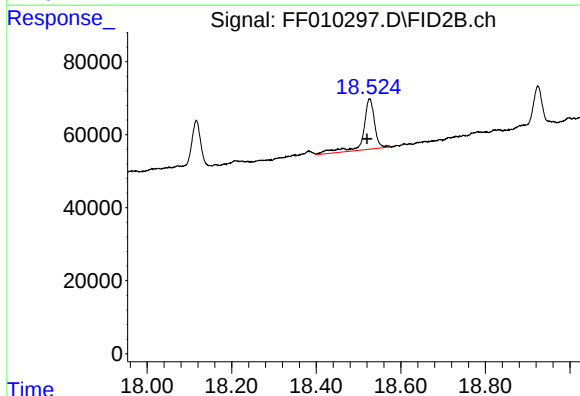


#14 N-DOTRIACONTANE

R.T.: 18.526 min
Delta R.T.: 0.006 min
Response: 258069
Conc: 2.00 ug/ml

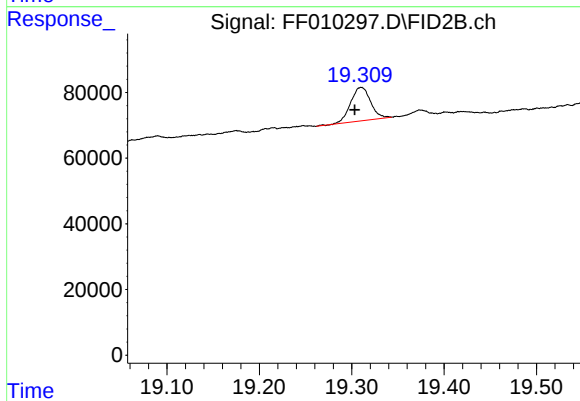

#15 N-TETRATRIACONTANE

R.T.: 19.310 min
Delta R.T.: 0.007 min
Response: 152895
Conc: 1.31 ug/ml

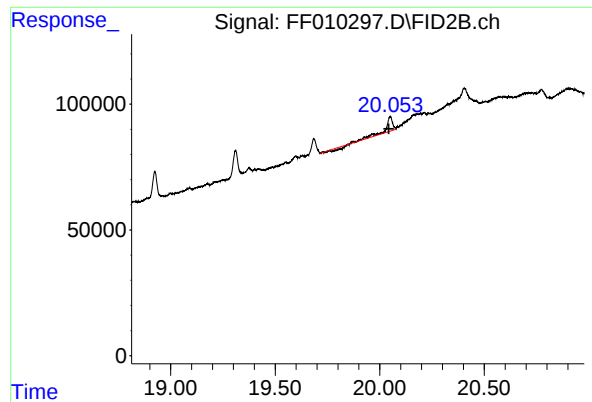

#16 N-HEXATRIACONTANE

R.T.: 20.050 min
Delta R.T.: 0.008 min
Response: 104470
Conc: 1.00 ug/ml

Instrument :
FID_F
ClientSampleId :