

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040822\
Data File : FF010299.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2022 09:56
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 23:27:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.384	3123807	23.461 ug/ml
12)	N-OCTACOSANE	16.808	3060063	23.088 ug/ml
13)	N-TRIACONTANE	17.694	85488	0.647 ug/ml
14)	N-DOTRIACONTANE	18.527	83103	0.644 ug/ml
16)	N-HEXATRIACONTANE	20.049	322561	3.093 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040822\
Data File : FF010299.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2022 09:56
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 23:27:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

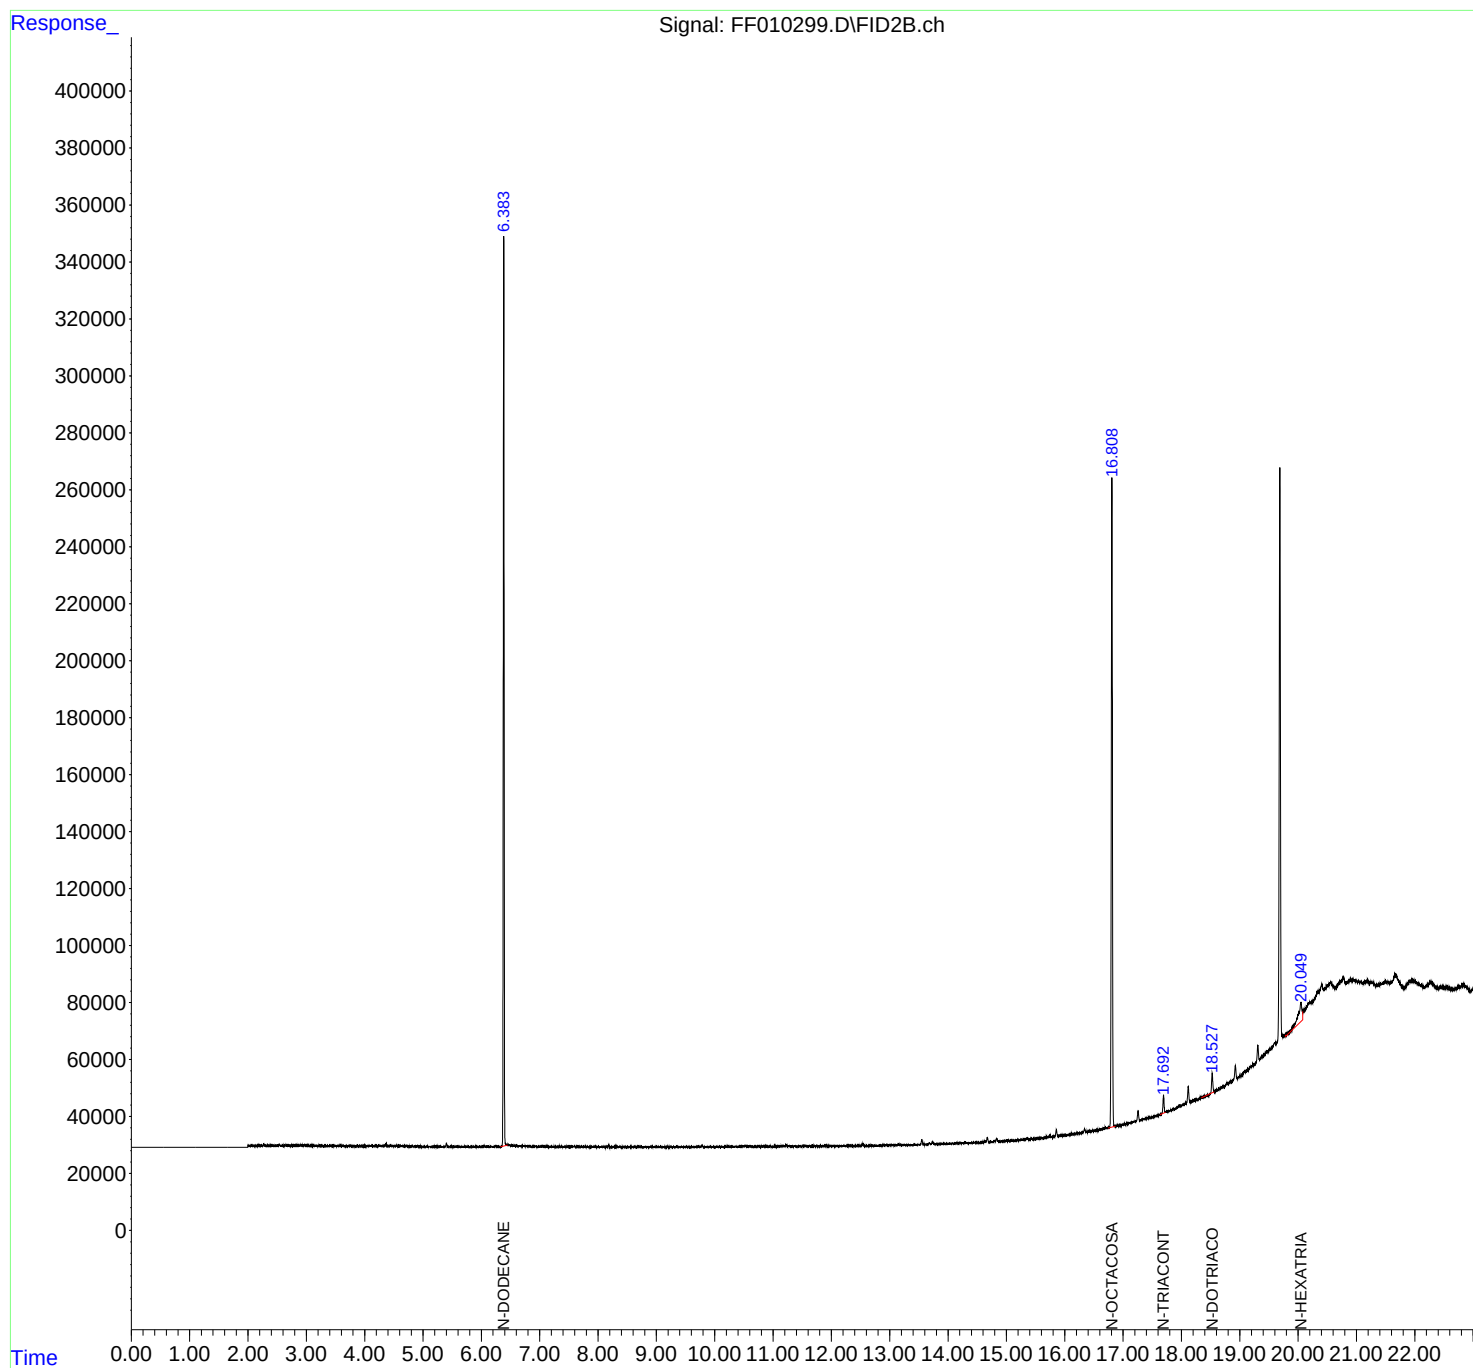


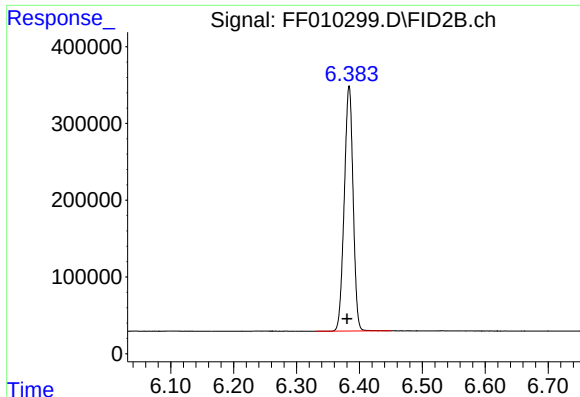

#3 N-DODECANE


R.T.: 6.384 min
Delta R.T.: 0.003 min
Response: 3123807
Conc: 23.46 ug/ml

Instrument :
FID_F
ClientSampleId :

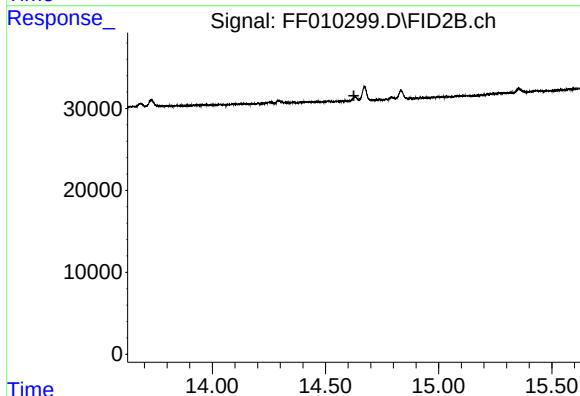


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.625 min
Response: 0
Conc: N.D.

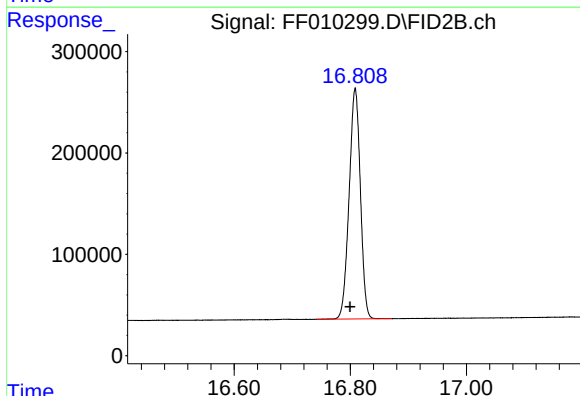


#12 N-OCTACOSANE

R.T.: 16.808 min
Delta R.T.: 0.009 min
Response: 3060063
Conc: 23.09 ug/ml

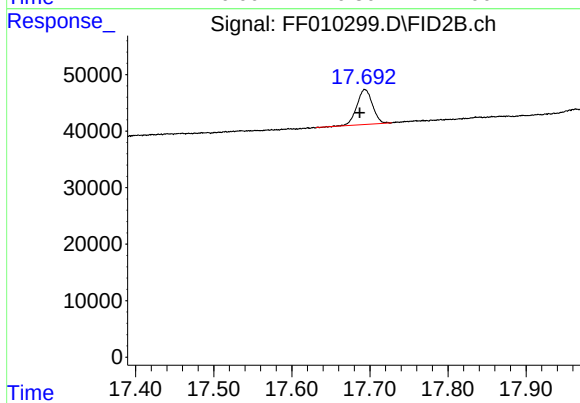

#13 N-TRIACONTANE


R.T.: 17.694 min
Delta R.T.: 0.007 min
Response: 85488
Conc: 0.65 ug/ml

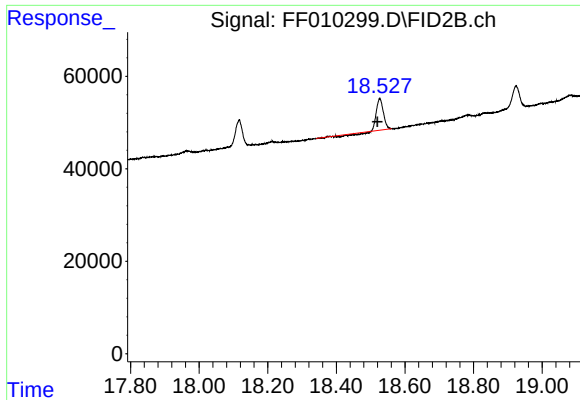

#14 N-DOTRIACONTANE

R.T.: 18.527 min
Delta R.T.: 0.006 min
Response: 83103
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

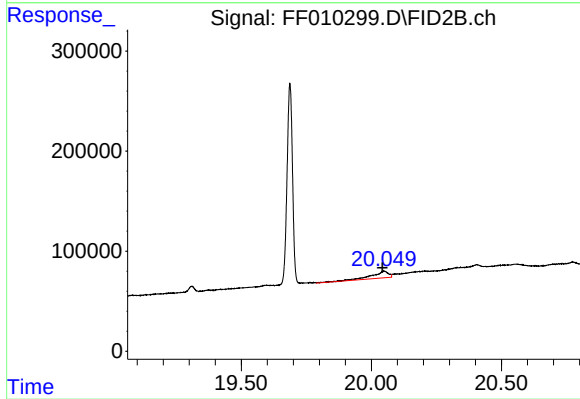

#16 N-HEXATRIACONTANE

R.T.: 20.049 min
Delta R.T.: 0.006 min
Response: 322561
Conc: 3.09 ug/ml