

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040822\
Data File : FF010301.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2022 11:05
Operator : AJ\MA
Sample : N2301-02 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 23:27:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.629	123114	1.030 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	20.050	94711	0.908 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040822\
Data File : FF010301.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2022 11:05
Operator : AJ\MA
Sample : N2301-02 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 23:27:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

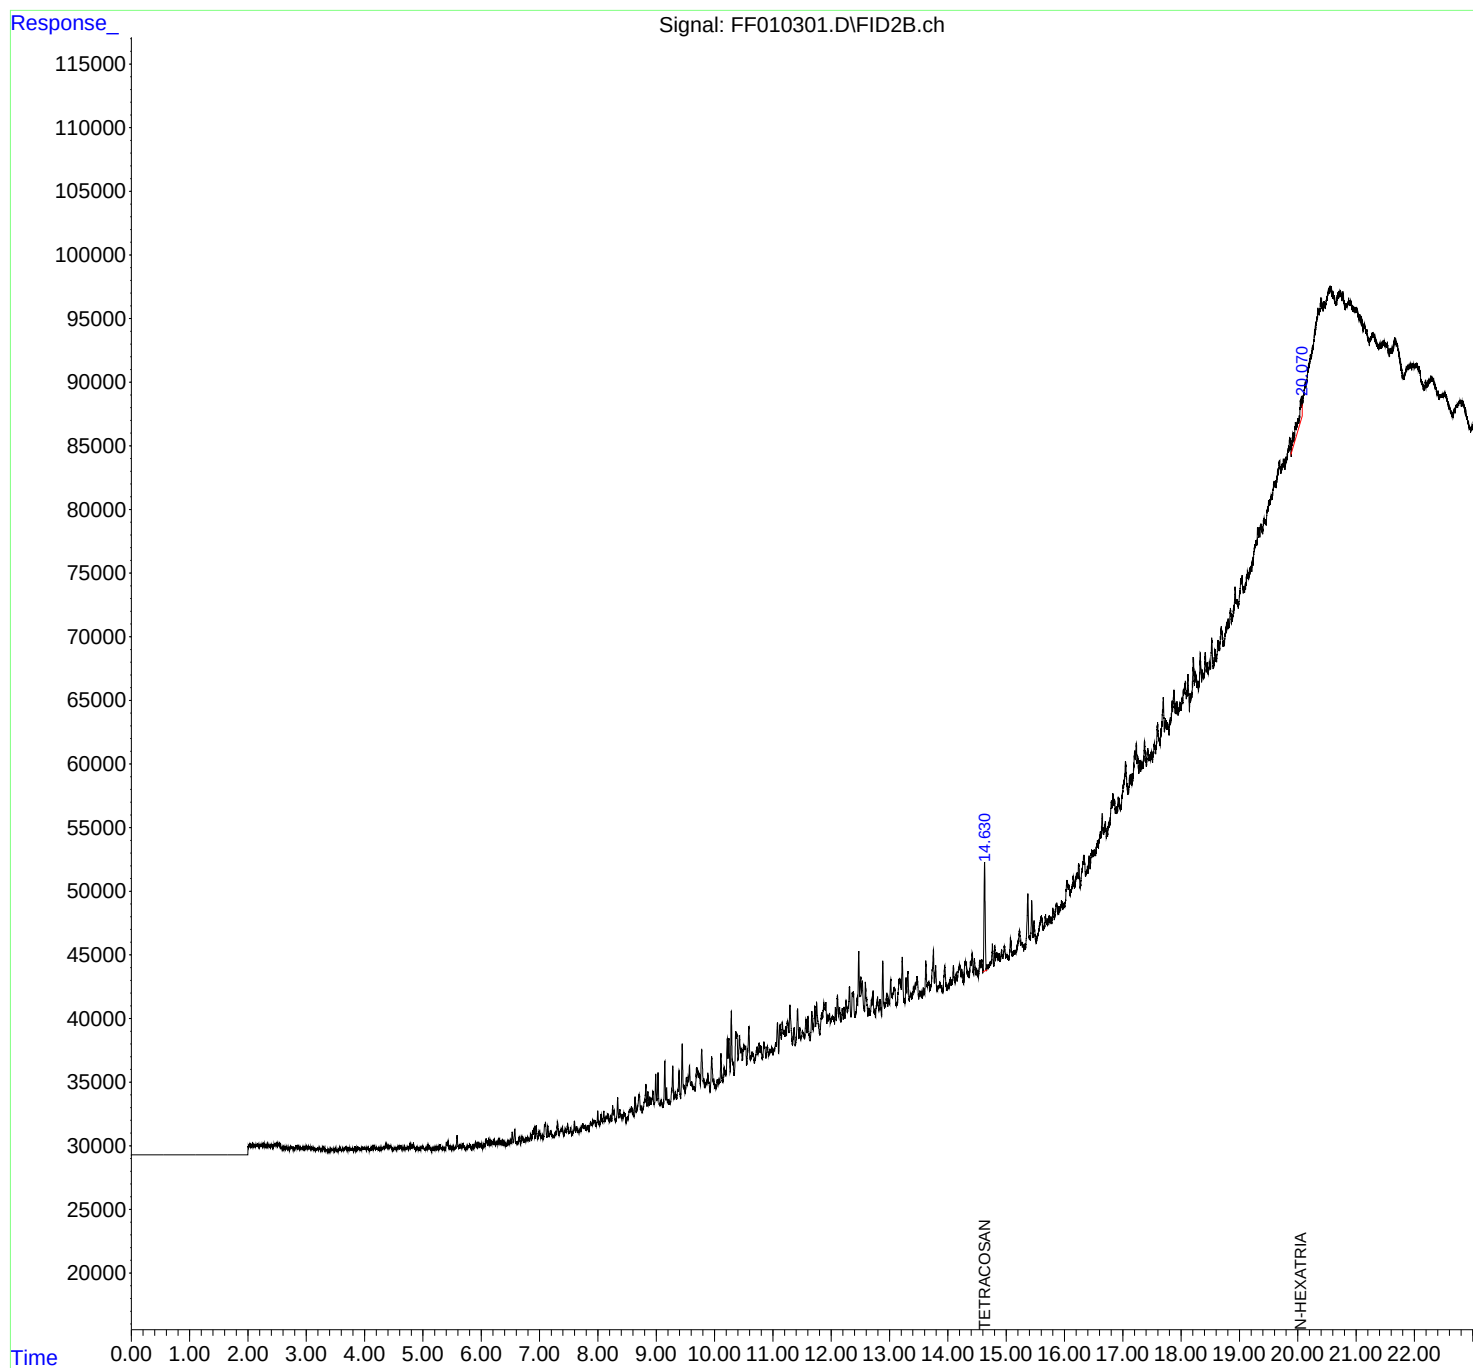


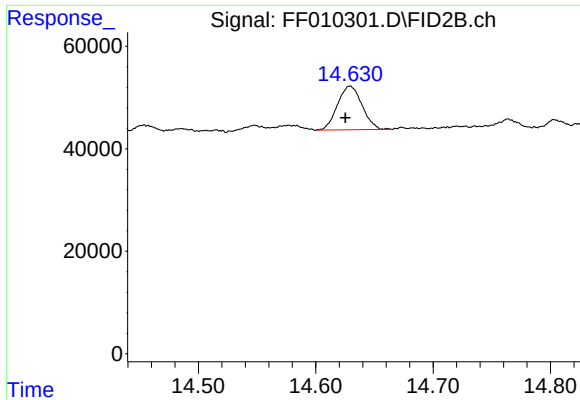

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.629 min
Delta R.T.: 0.004 min
Response: 123114
Conc: 1.03 ug/ml

Instrument :
FID_F
ClientSampleId :

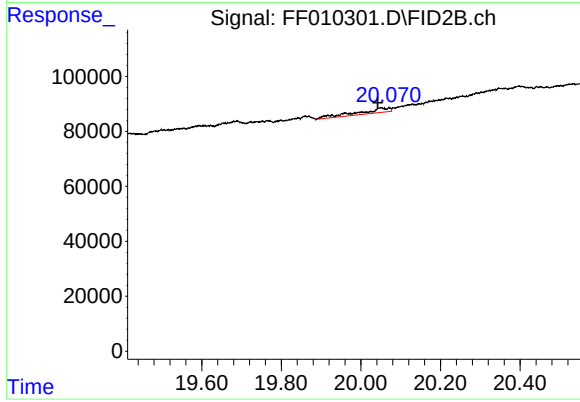

#16 N-HEXATRIACONTANE

R.T.: 20.050 min
Delta R.T.: 0.008 min
Response: 94711
Conc: 0.91 ug/ml