

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040822\
 Data File : FF010303.D
 Signal(s) : FID2B.ch
 Acq On : 08 Apr 2022 12:05
 Operator : AJ\MA
 Sample : N2301-05 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 08 23:27:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	152835	1.279 ug/ml
Target Compounds			
7) N-EICOSANE	12.531	95346	0.710 ug/ml
8) N-DOCOSANE	13.730	255264	1.908 ug/ml
10) N-TETRACOSANE	14.833	171043	1.277 ug/ml
11) N-HEXACOSANE	15.855	95398	0.719 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040822\
Data File : FF010303.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2022 12:05
Operator : AJ\MA
Sample : N2301-05 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 08 23:27:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

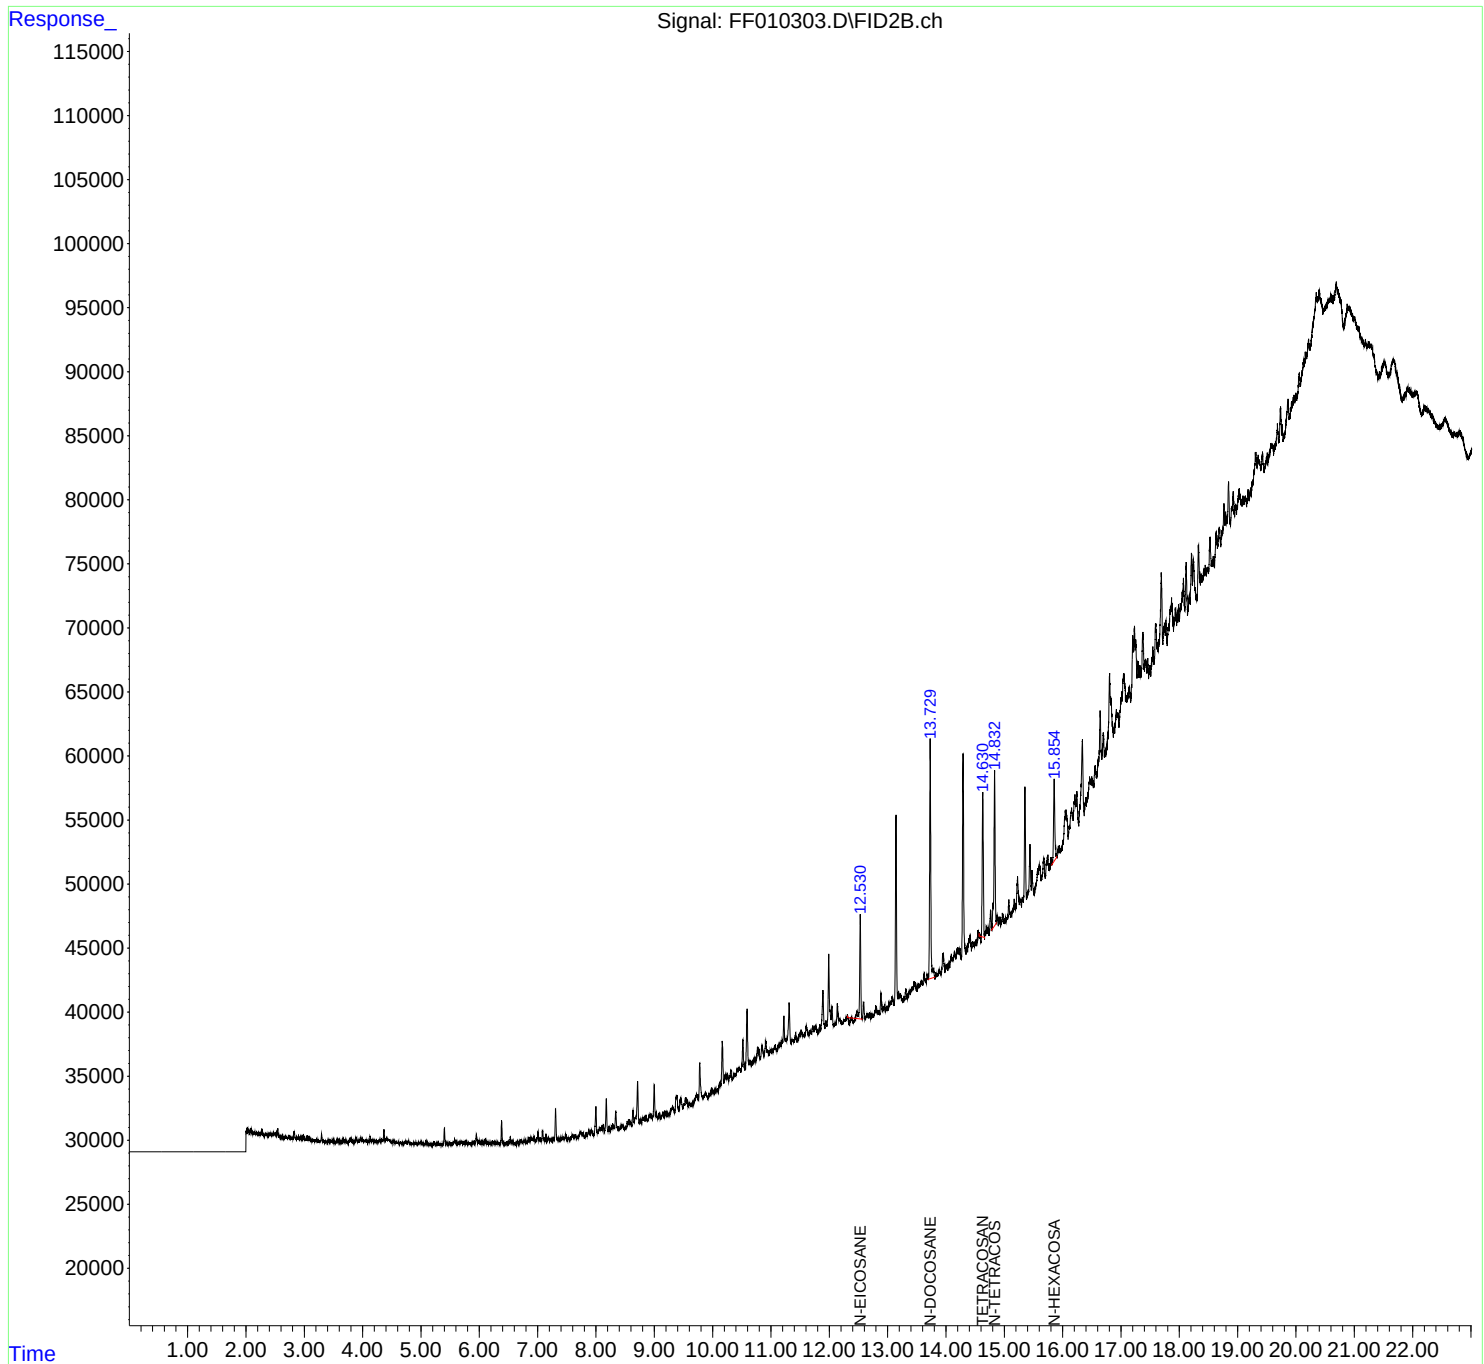


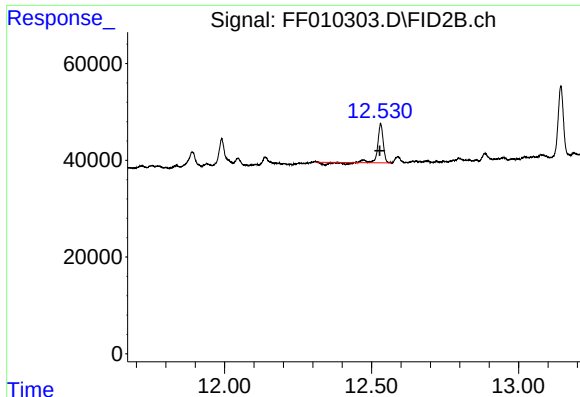

#7 N-EICOSANE


R.T.: 12.531 min
Delta R.T.: 0.004 min
Response: 95346
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :

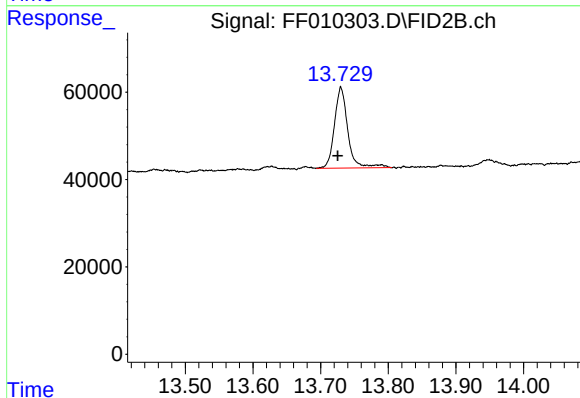


#8 N-DOCOSANE

R.T.: 13.730 min
Delta R.T.: 0.004 min
Response: 255264
Conc: 1.91 ug/ml

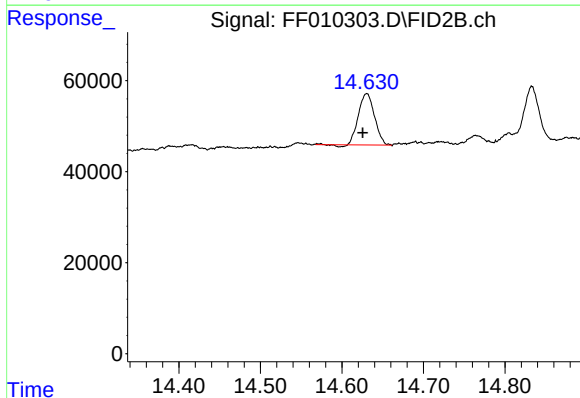


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.630 min
Delta R.T.: 0.005 min
Response: 152835
Conc: 1.28 ug/ml

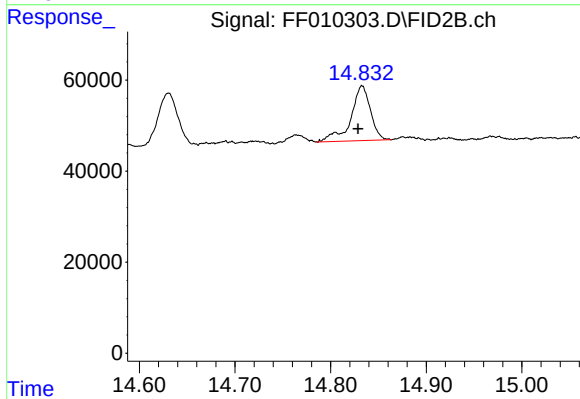

#10 N-TETRACOSANE

R.T.: 14.833 min
Delta R.T.: 0.004 min
Response: 171043
Conc: 1.28 ug/ml

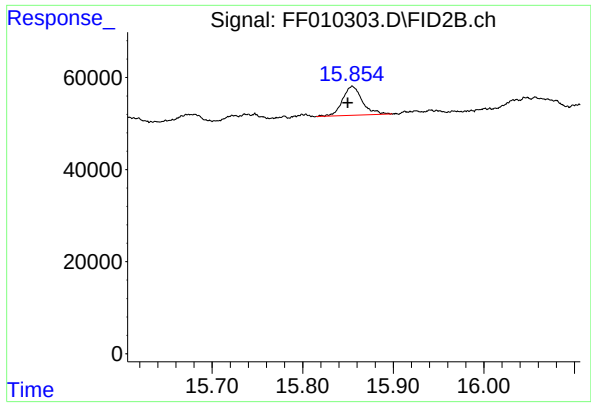

#11 N-HEXACOSANE

R.T.: 15.855 min
Delta R.T.: 0.005 min
Response: 95398
Conc: 0.72 ug/ml

Instrument :

FID_F

ClientSampleId :