

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040822\
 Data File : FF010304.D
 Signal(s) : FID2B.ch
 Acq On : 08 Apr 2022 12:36
 Operator : AJ\MA
 Sample : N2301-06 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WC-14A-1A-4-GR-6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/11/2022
 Supervised By :mohammad ahmed 04/12/2022

Integration File: autoint1.e
 Quant Time: Apr 08 23:27:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	118652	0.993 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040822\
Data File : FF010304.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2022 12:36
Operator : AJ\MA
Sample : N2301-06 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
WC-14A-1A-4-GR-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/12/2022

Integration File: autoint1.e
Quant Time: Apr 08 23:27:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

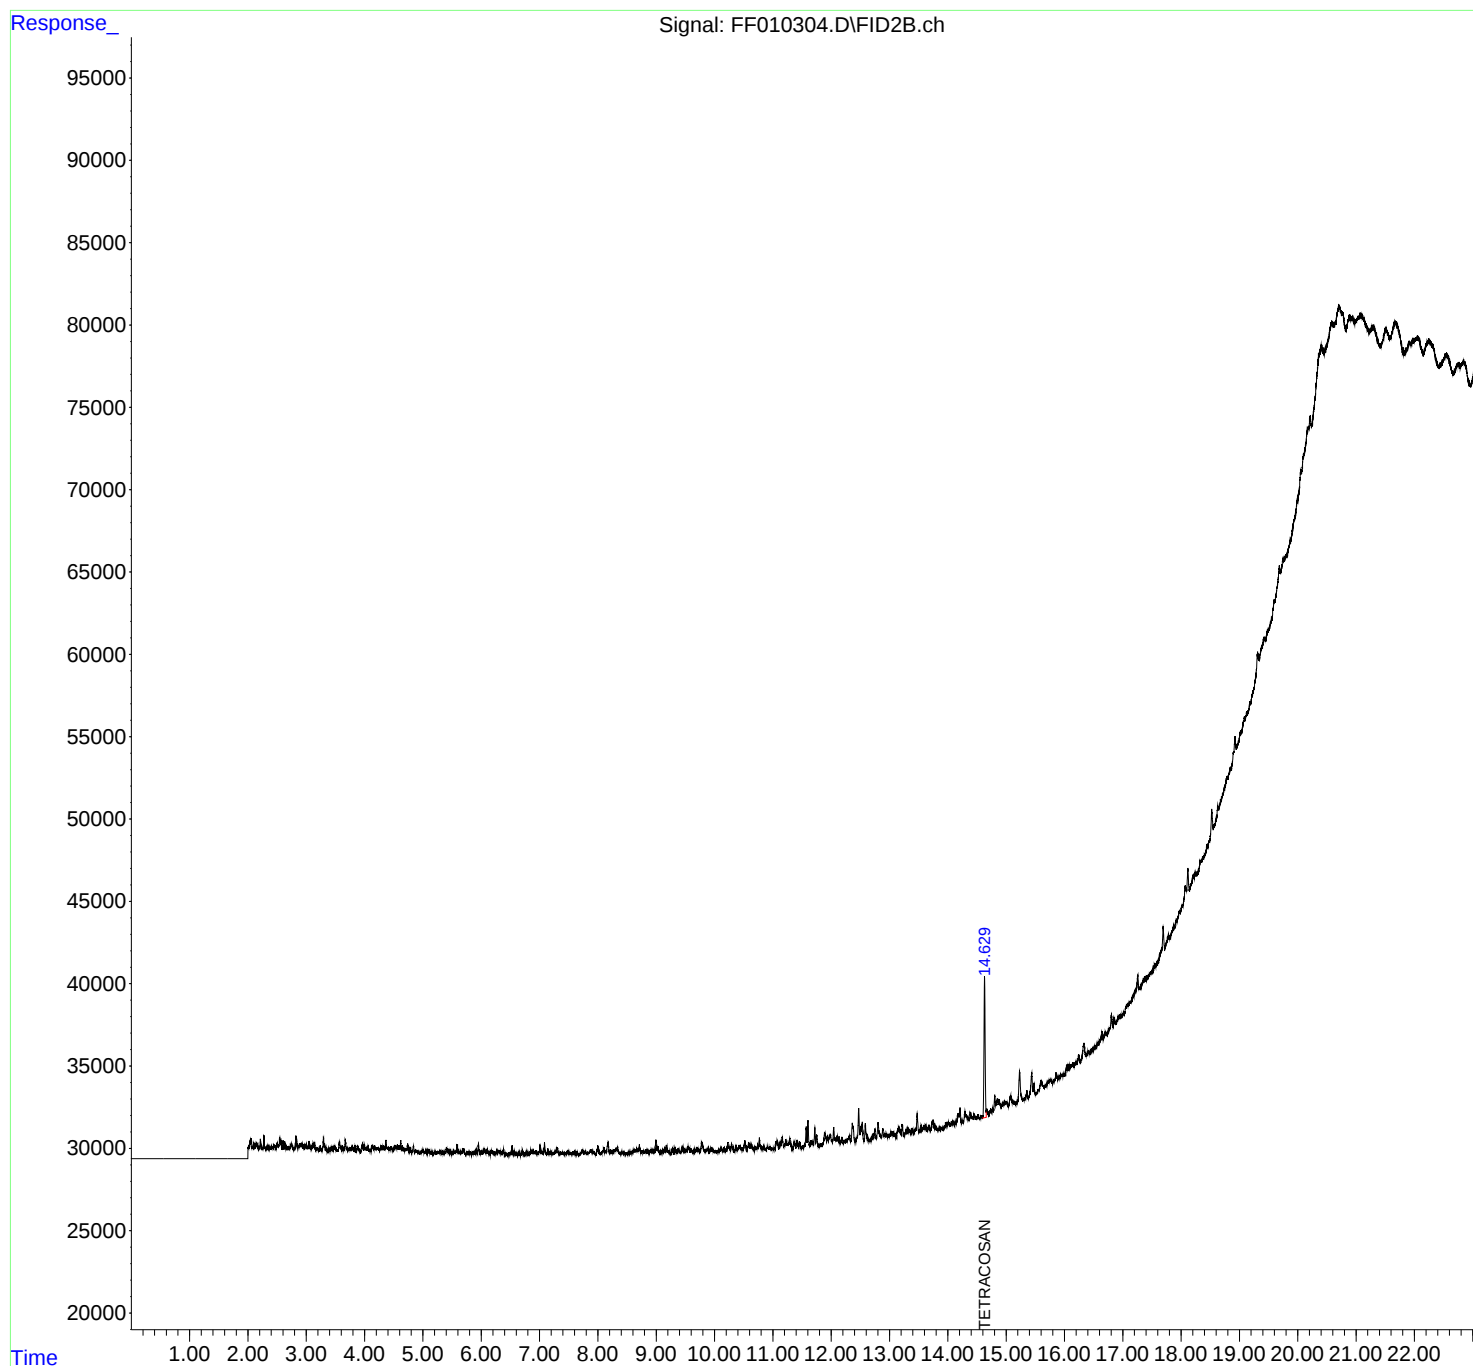

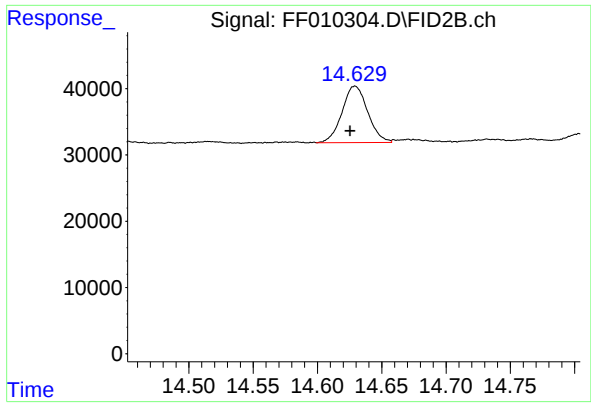

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.629 min
Delta R.T.: 0.003 min
Response: 118652
Conc: 0.99 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-14A-1A-4-GR-6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/11/2022
Supervised By :mohammad ahmed 04/12/2022