

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040823\
Data File : FF012426.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2023 05:44
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 03:35:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.741	2215947	17.875 ug/ml
12)	N-OCTACOSANE	17.185	2325732	20.219 ug/ml
14)	N-DOTRIACONTANE	18.903	59125	0.570 ug/ml
15)	N-TETRATRIACONTANE	19.684	47315	0.500 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040823\
Data File : FF012426.D
Signal(s) : FID2B.ch
Acq On : 08 Apr 2023 05:44
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 03:35:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

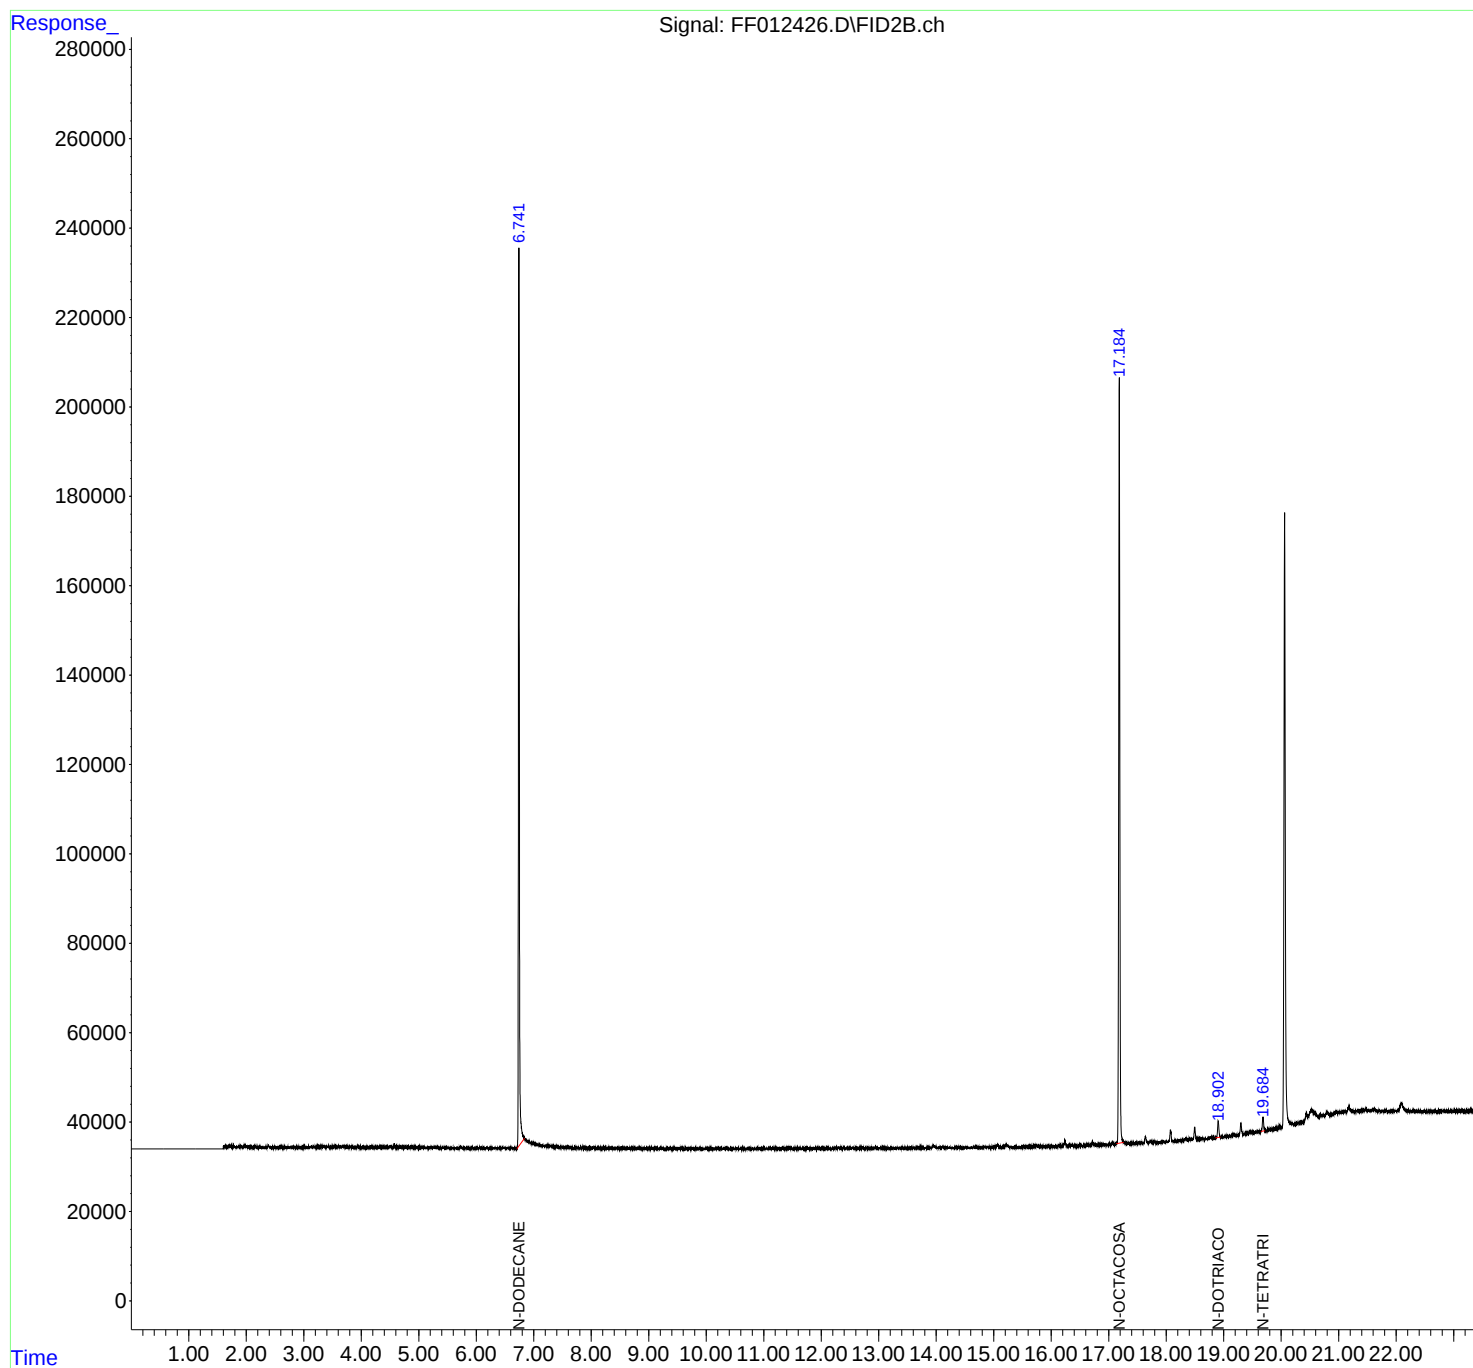


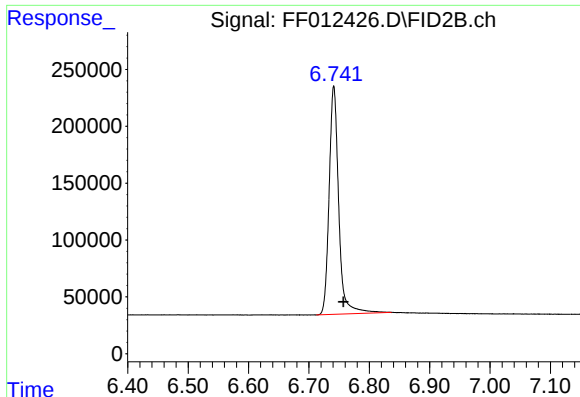

#3 N-DODECANE


R.T.: 6.741 min
Delta R.T.: -0.016 min
Response: 2215947
Conc: 17.88 ug/ml

Instrument :
FID_F
ClientSampleId :

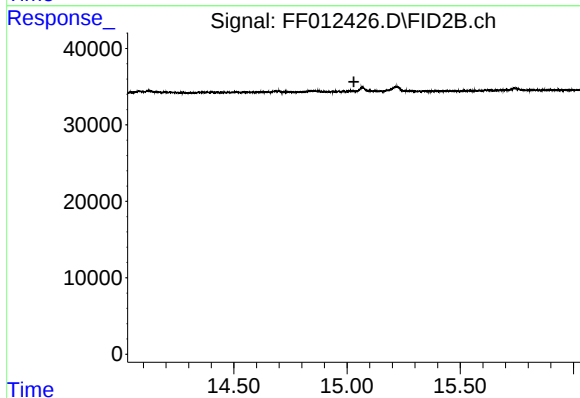


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.030 min
Response: 0
Conc: N.D.

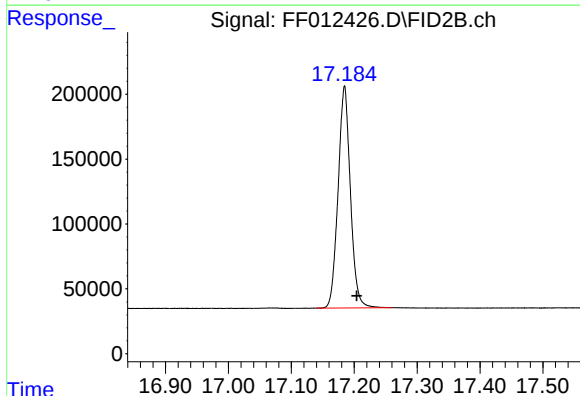


#12 N-OCTACOSANE

R.T.: 17.185 min
Delta R.T.: -0.019 min
Response: 2325732
Conc: 20.22 ug/ml

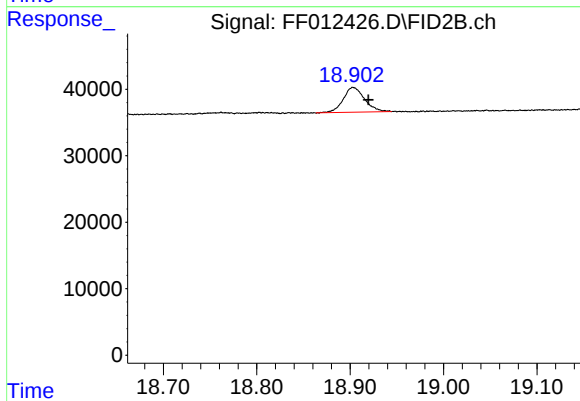

#14 N-DOTRIACONTANE

R.T.: 18.903 min
Delta R.T.: -0.016 min
Response: 59125
Conc: 0.57 ug/ml

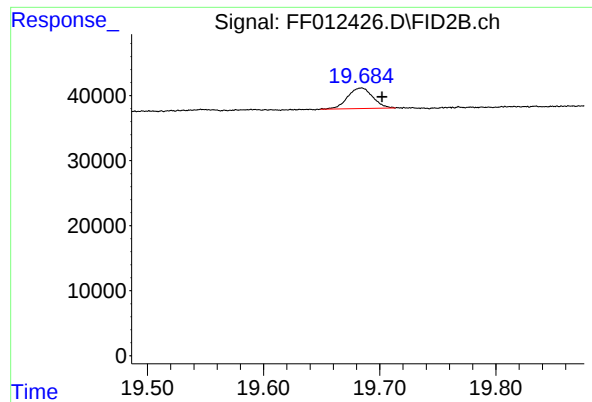

#15 N-TETRATRIACONTANE

R.T.: 19.684 min
Delta R.T.: -0.018 min
Response: 47315
Conc: 0.50 ug/ml

Instrument :

FID_F

ClientSampleId :