

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040919\
 Data File : FF004162.D
 Signal(s) : FID2B.ch
 Acq On : 09 Apr 2019 21:13
 Operator : AJ\SJ
 Sample : K2338-08MSD
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 10 01:12:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.538	1306920	10.053 ug/ml
Target Compounds			
2) N-DECANE	4.288	1489259	11.004 ug/ml
3) N-DODECANE	6.305	1548505	11.037 ug/ml
4) N-TETRADECANE	8.095	1564361	11.002 ug/ml
5) N-HEXADECANE	9.693	1596061	10.784 ug/ml
6) N-OCTADECANE	11.132	1618240	10.745 ug/ml
7) N-EICOSANE	12.440	1597365	10.629 ug/ml
8) N-DOCOSANE	13.637	1551762	10.367 ug/ml
10) N-TETRACOSANE	14.741	1657909	11.255 ug/mlm
11) N-HEXACOSANE	15.761	1576721	10.861 ug/ml
12) N-OCTACOSANE	16.711	1803034	12.539 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040919\
Data File : FF04162.D
Signal(s) : FID2B.ch
Acq On : 09 Apr 2019 21:13
Operator : AJ\SJ
Sample : K2338-08MSD
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 10 01:12:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

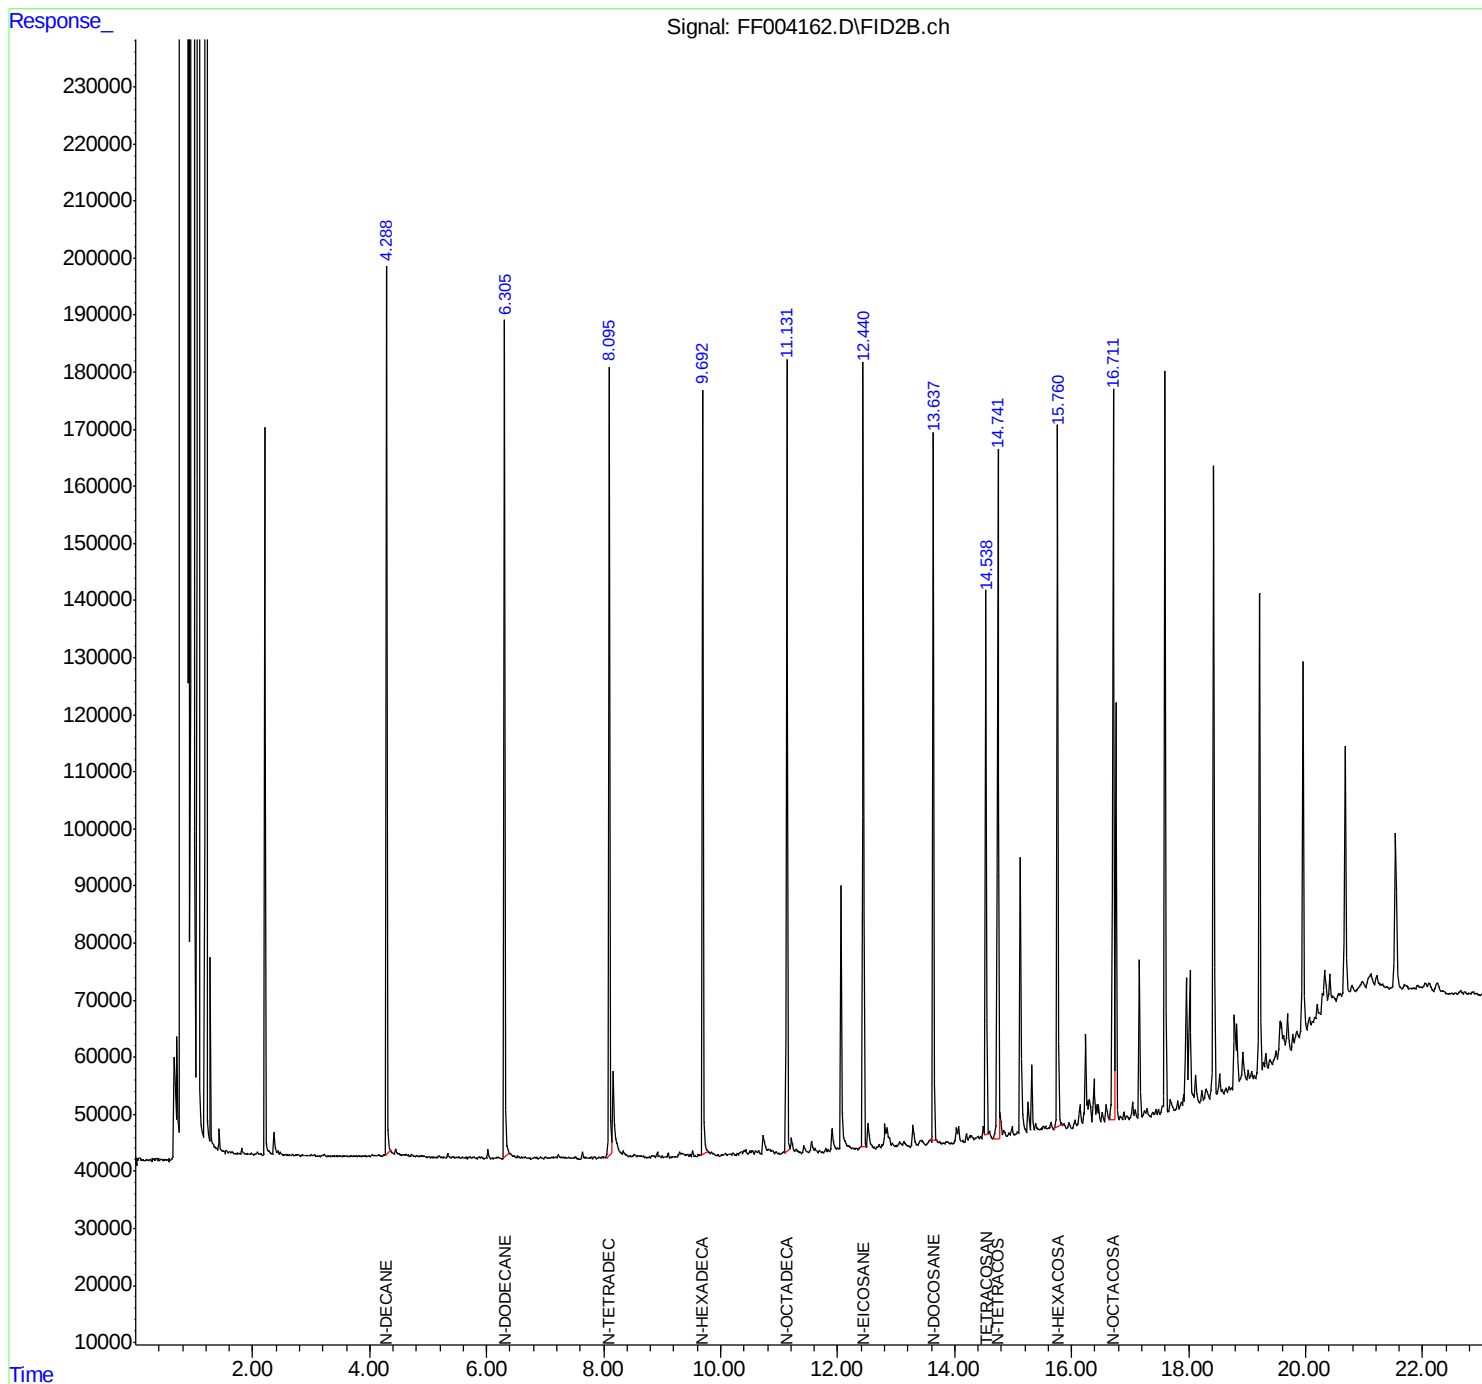

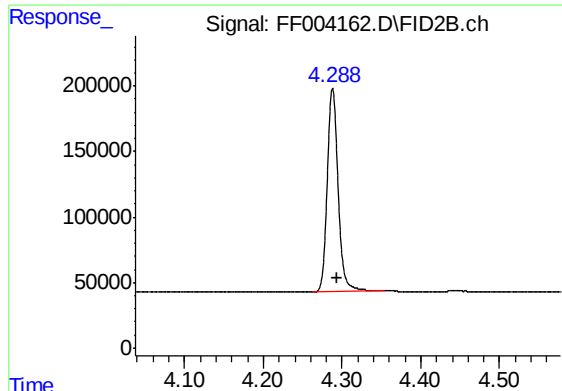


#2 N-DECANE

R.T.: 4.288 min
Delta R.T.: -0.006 min
Response: 1489259
Conc: 11.00 ug/ml

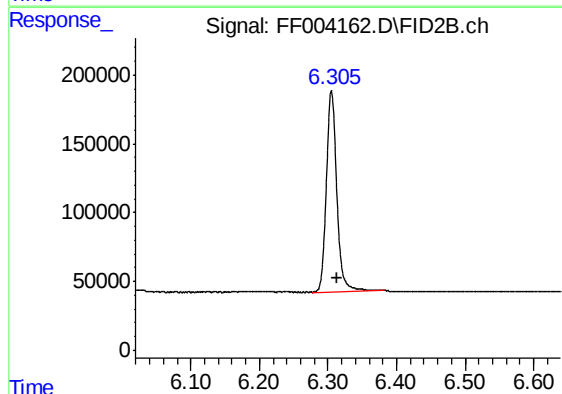


#3 N-DODECANE

R.T.: 6.305 min
Delta R.T.: -0.008 min
Response: 1548505
Conc: 11.04 ug/ml

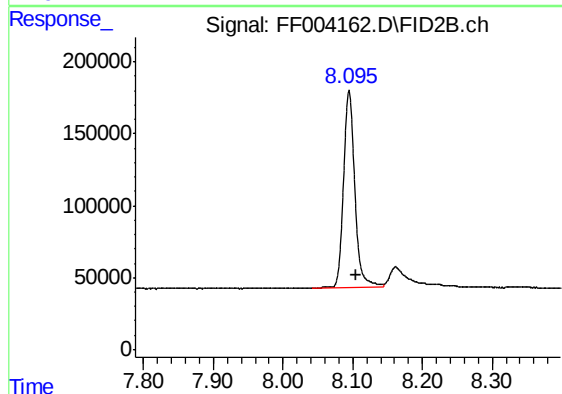


#4 N-TETRADECANE

R.T.: 8.095 min
Delta R.T.: -0.011 min
Response: 1564361
Conc: 11.00 ug/ml

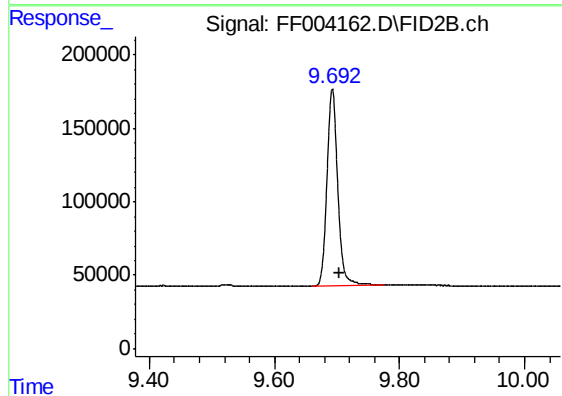


#5 N-HEXADECANE

R.T.: 9.693 min
Delta R.T.: -0.012 min
Response: 1596061
Conc: 10.78 ug/ml

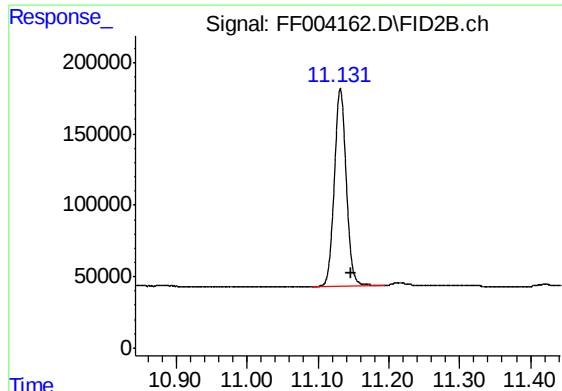


#6 N-OCTADECANE

R.T.: 11.132 min
Delta R.T.: -0.014 min
Response: 1618240
Conc: 10.75 ug/ml

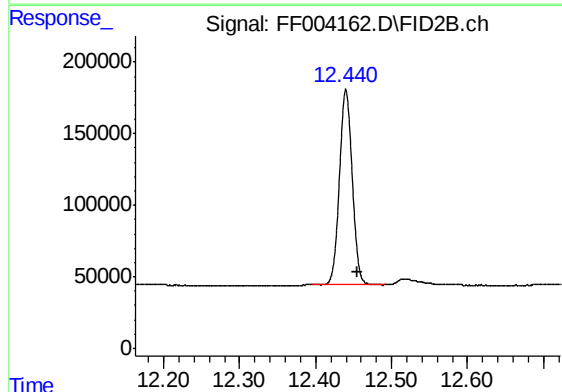


#7 N-EICOSANE

R.T.: 12.440 min
Delta R.T.: -0.016 min
Response: 1597365
Conc: 10.63 ug/ml

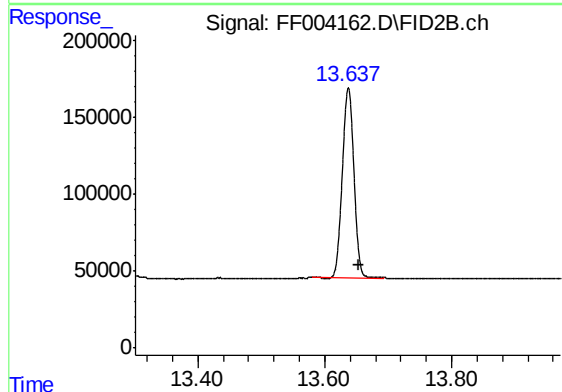


#8 N-DOCOSANE

R.T.: 13.637 min
Delta R.T.: -0.016 min
Response: 1551762
Conc: 10.37 ug/ml

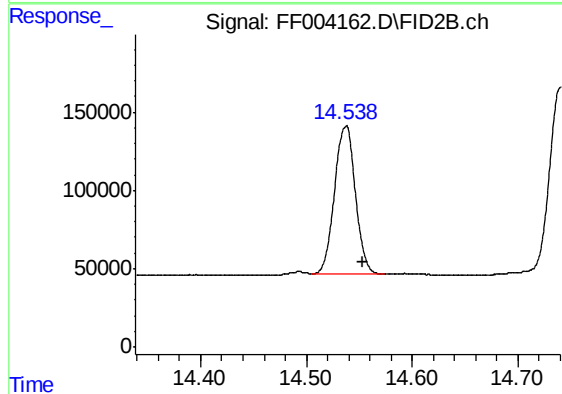


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.538 min
Delta R.T.: -0.016 min
Response: 1306920
Conc: 10.05 ug/ml

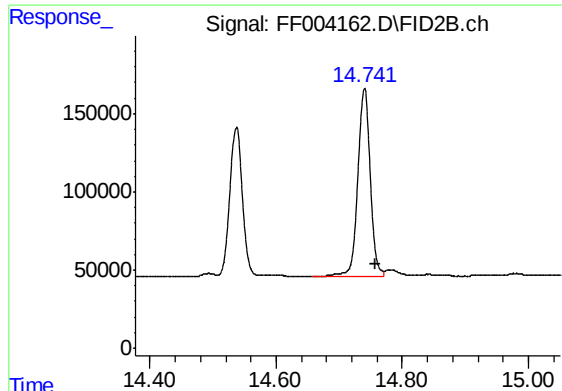


#10 N-TETRACOSANE

R.T.: 14.741 min
Delta R.T.: -0.017 min
Response: 1657909
Conc: 11.26 ug/ml m

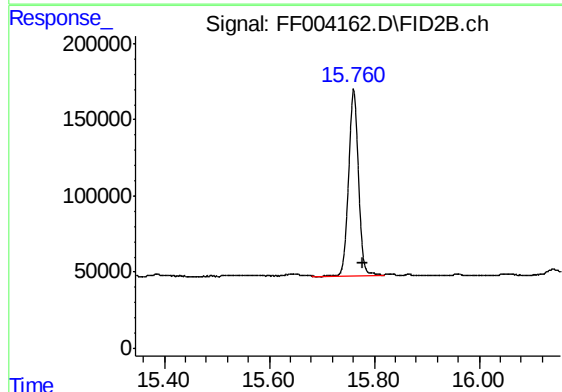

#11 N-HEXACOSANE

R.T.: 15.761 min
Delta R.T.: -0.017 min
Response: 1576721
Conc: 10.86 ug/ml

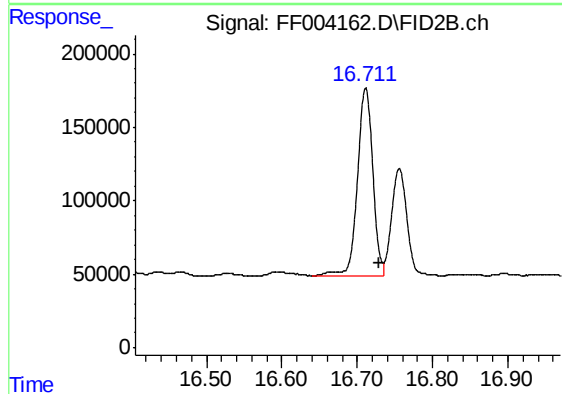

#12 N-OCTACOSANE

R.T.: 16.711 min
Delta R.T.: -0.019 min
Response: 1803034
Conc: 12.54 ug/ml