

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040922\
 Data File : FF010316.D
 Signal(s) : FID2B.ch
 Acq On : 09 Apr 2022 13:42
 Operator : AJ\MA
 Sample : N2336-02
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 11 01:23:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	1558734	13.041 ug/ml
Target Compounds			
5) N-HEXADECANE	9.710f	85593	0.645 ug/ml
6) N-OCTADECANE	11.234	100081	0.728 ug/ml
7) N-EICOSANE	12.585f	879719	6.548 ug/ml
8) N-DOCOSANE	13.749	149953	1.121 ug/ml
10) N-TETRACOSANE	14.804	514978	3.846 ug/ml
11) N-HEXACOSANE	15.881	102871	0.776 ug/ml
12) N-OCTACOSANE	16.834	710613	5.361 ug/ml
13) N-TRIACONTANE	17.699	1346223	10.196 ug/ml
14) N-DOTRIACONTANE	18.528	526939	4.082 ug/ml
15) N-TETRATRIACONTANE	19.356f	324486	2.788 ug/ml
16) N-HEXATRIACONTANE	20.035	779623	7.475 ug/ml
18) N-TETRACONTANE	21.678	1480965	16.906 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040922\
Data File : FF010316.D
Signal(s) : FID2B.ch
Acq On : 09 Apr 2022 13:42
Operator : AJ\MA
Sample : N2336-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 11 01:23:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

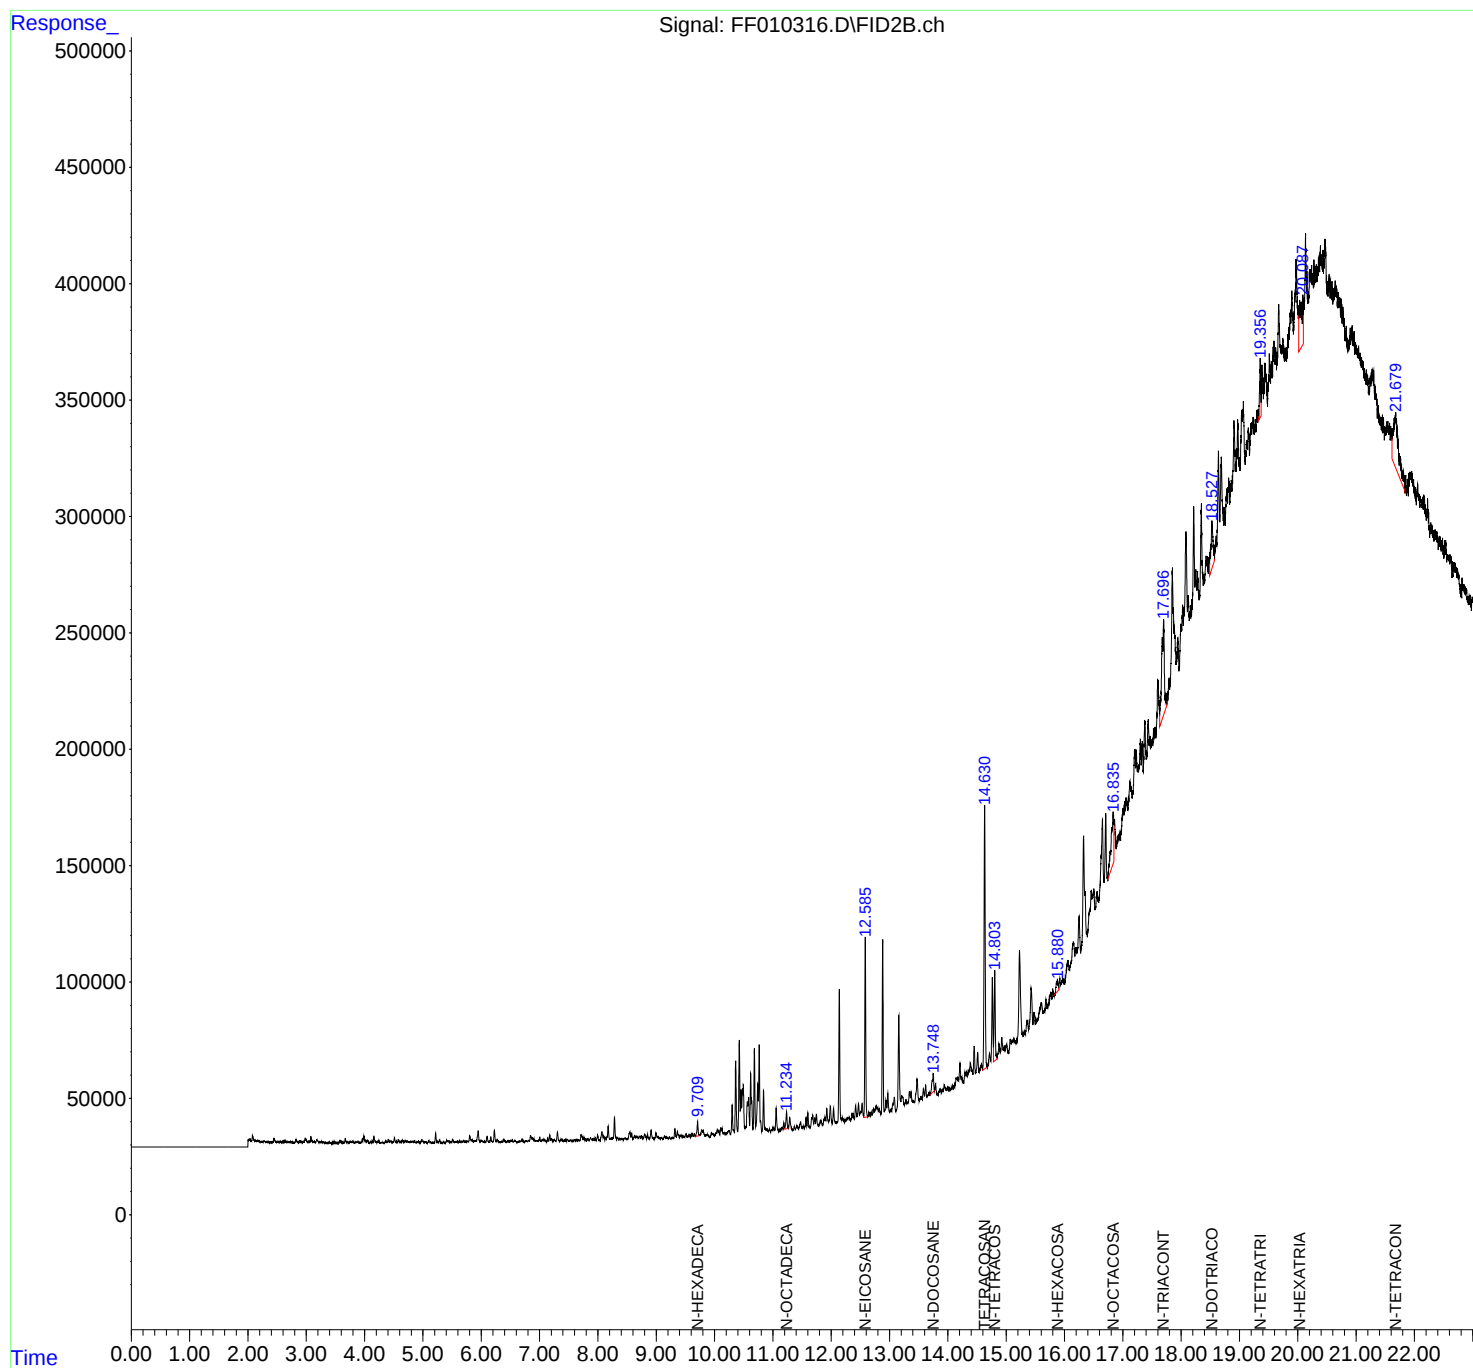


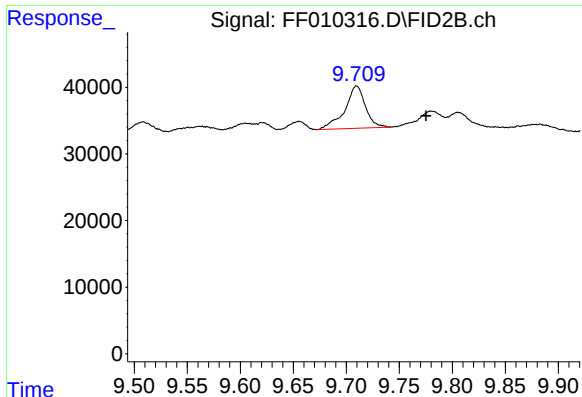

#5 N-HEXADECANE


R.T.: 9.710 min
Delta R.T.: -0.065 min
Response: 85593
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

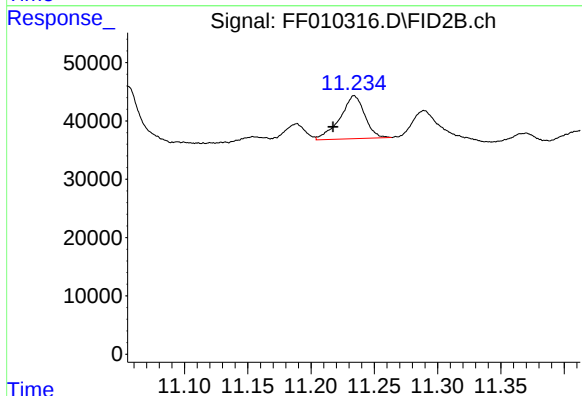


#6 N-OCTADECANE

R.T.: 11.234 min
Delta R.T.: 0.017 min
Response: 100081
Conc: 0.73 ug/ml

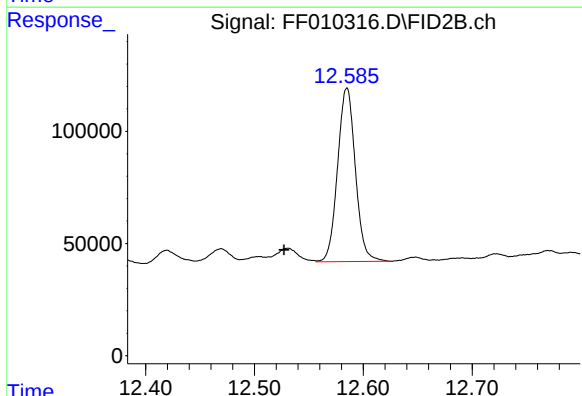


#7 N-EICOSANE

R.T.: 12.585 min
Delta R.T.: 0.058 min
Response: 879719
Conc: 6.55 ug/ml

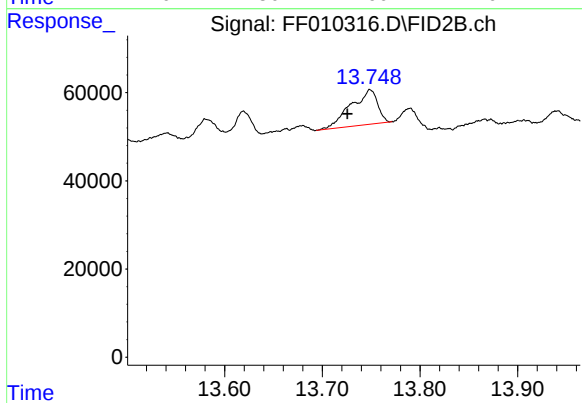

#8 N-DOCOSANE


R.T.: 13.749 min
Delta R.T.: 0.023 min
Response: 149953
Conc: 1.12 ug/ml

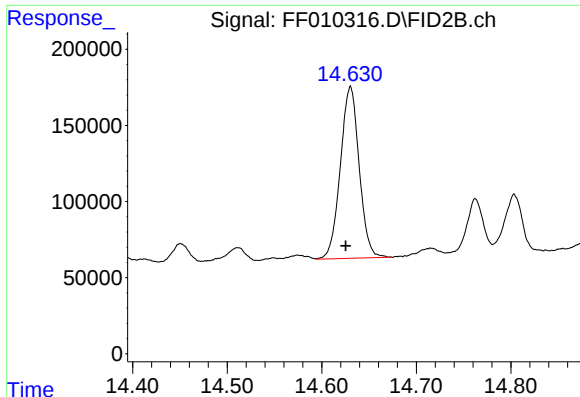

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.630 min
Delta R.T.: 0.005 min
Response: 1558734
Conc: 13.04 ug/ml

Instrument :
FID_F
ClientSampleId :

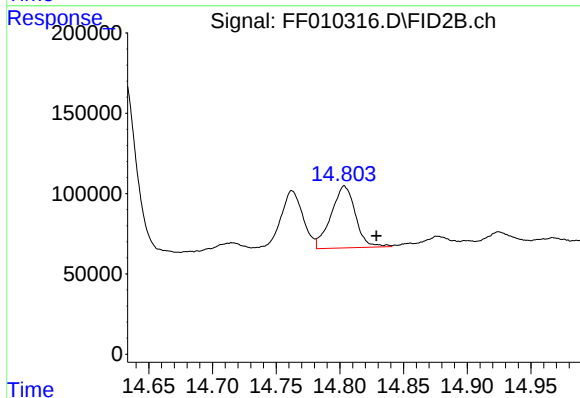


#10 N-TETRACOSANE

R.T.: 14.804 min
Delta R.T.: -0.025 min
Response: 514978
Conc: 3.85 ug/ml

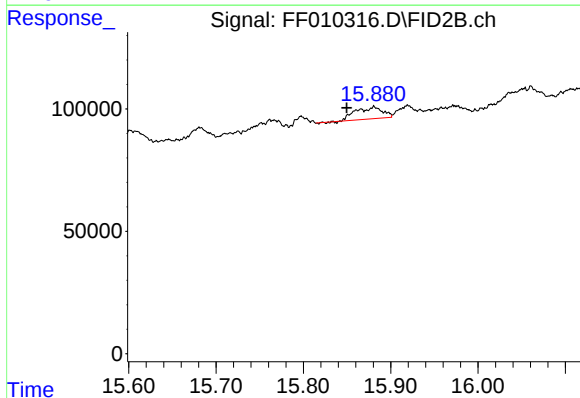


#11 N-HEXACOSANE

R.T.: 15.881 min
Delta R.T.: 0.031 min
Response: 102871
Conc: 0.78 ug/ml

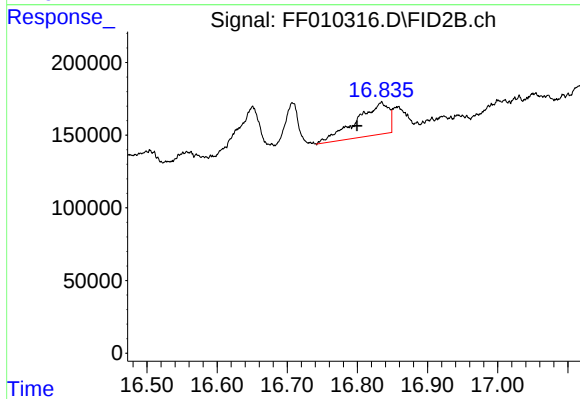

#12 N-OCTACOSANE


R.T.: 16.834 min
Delta R.T.: 0.035 min
Response: 710613
Conc: 5.36 ug/ml

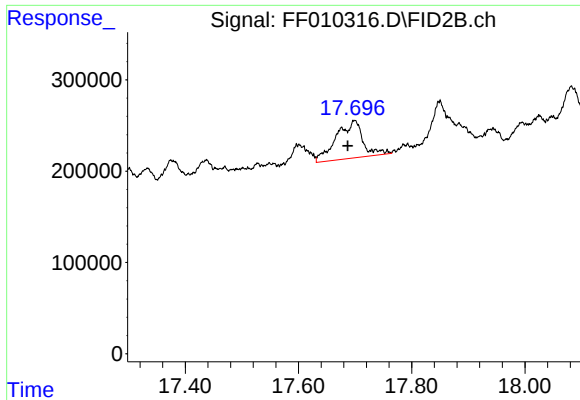

#13 N-TRIACONTANE


R.T.: 17.699 min
Delta R.T.: 0.012 min
Response: 1346223
Conc: 10.20 ug/ml

Instrument :
FID_F
ClientSampleId :

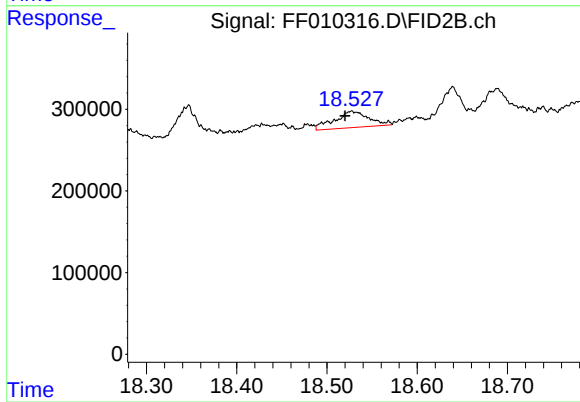


#14 N-DOTRIACONTANE

R.T.: 18.528 min
Delta R.T.: 0.007 min
Response: 526939
Conc: 4.08 ug/ml

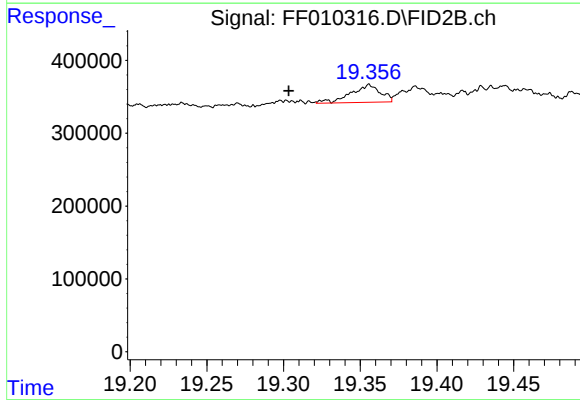


#15 N-TETRATRIACONTANE

R.T.: 19.356 min
Delta R.T.: 0.052 min
Response: 324486
Conc: 2.79 ug/ml

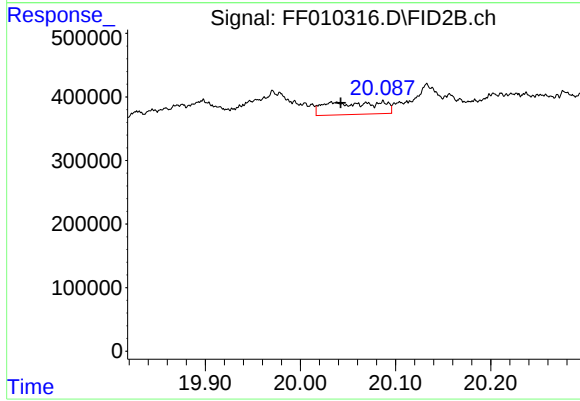

#16 N-HEXATRIACONTANE

R.T.: 20.035 min
Delta R.T.: -0.007 min
Response: 779623
Conc: 7.47 ug/ml

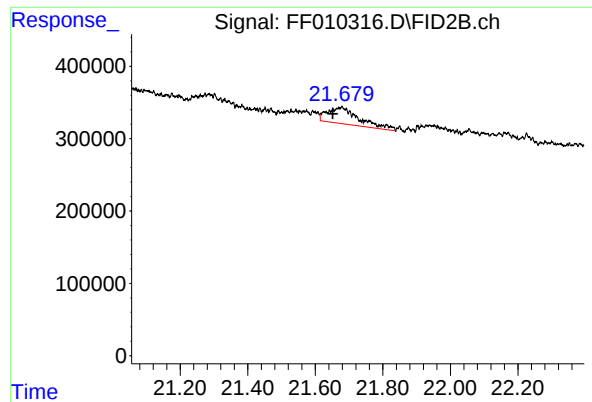

#18 N-TETRACONTANE

R.T.: 21.678 min
Delta R.T.: 0.027 min
Response: 1480965
Conc: 16.91 ug/ml

Instrument :

FID_F

ClientSampleId :