

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040922\
Data File : FF010317.D
Signal(s) : FID2B.ch
Acq On : 09 Apr 2022 14:42
Operator : AJ\MA
Sample : N2301-06
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-14A-1A-4-6R-6

Integration File: autoint1.e
Quant Time: Apr 11 01:24:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	1495969	12.516 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF040922\
Data File : FF010317.D
Signal(s) : FID2B.ch
Acq On : 09 Apr 2022 14:42
Operator : AJ\MA
Sample : N2301-06
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-14A-1A-4-6R-6

Integration File: autoint1.e
Quant Time: Apr 11 01:24:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

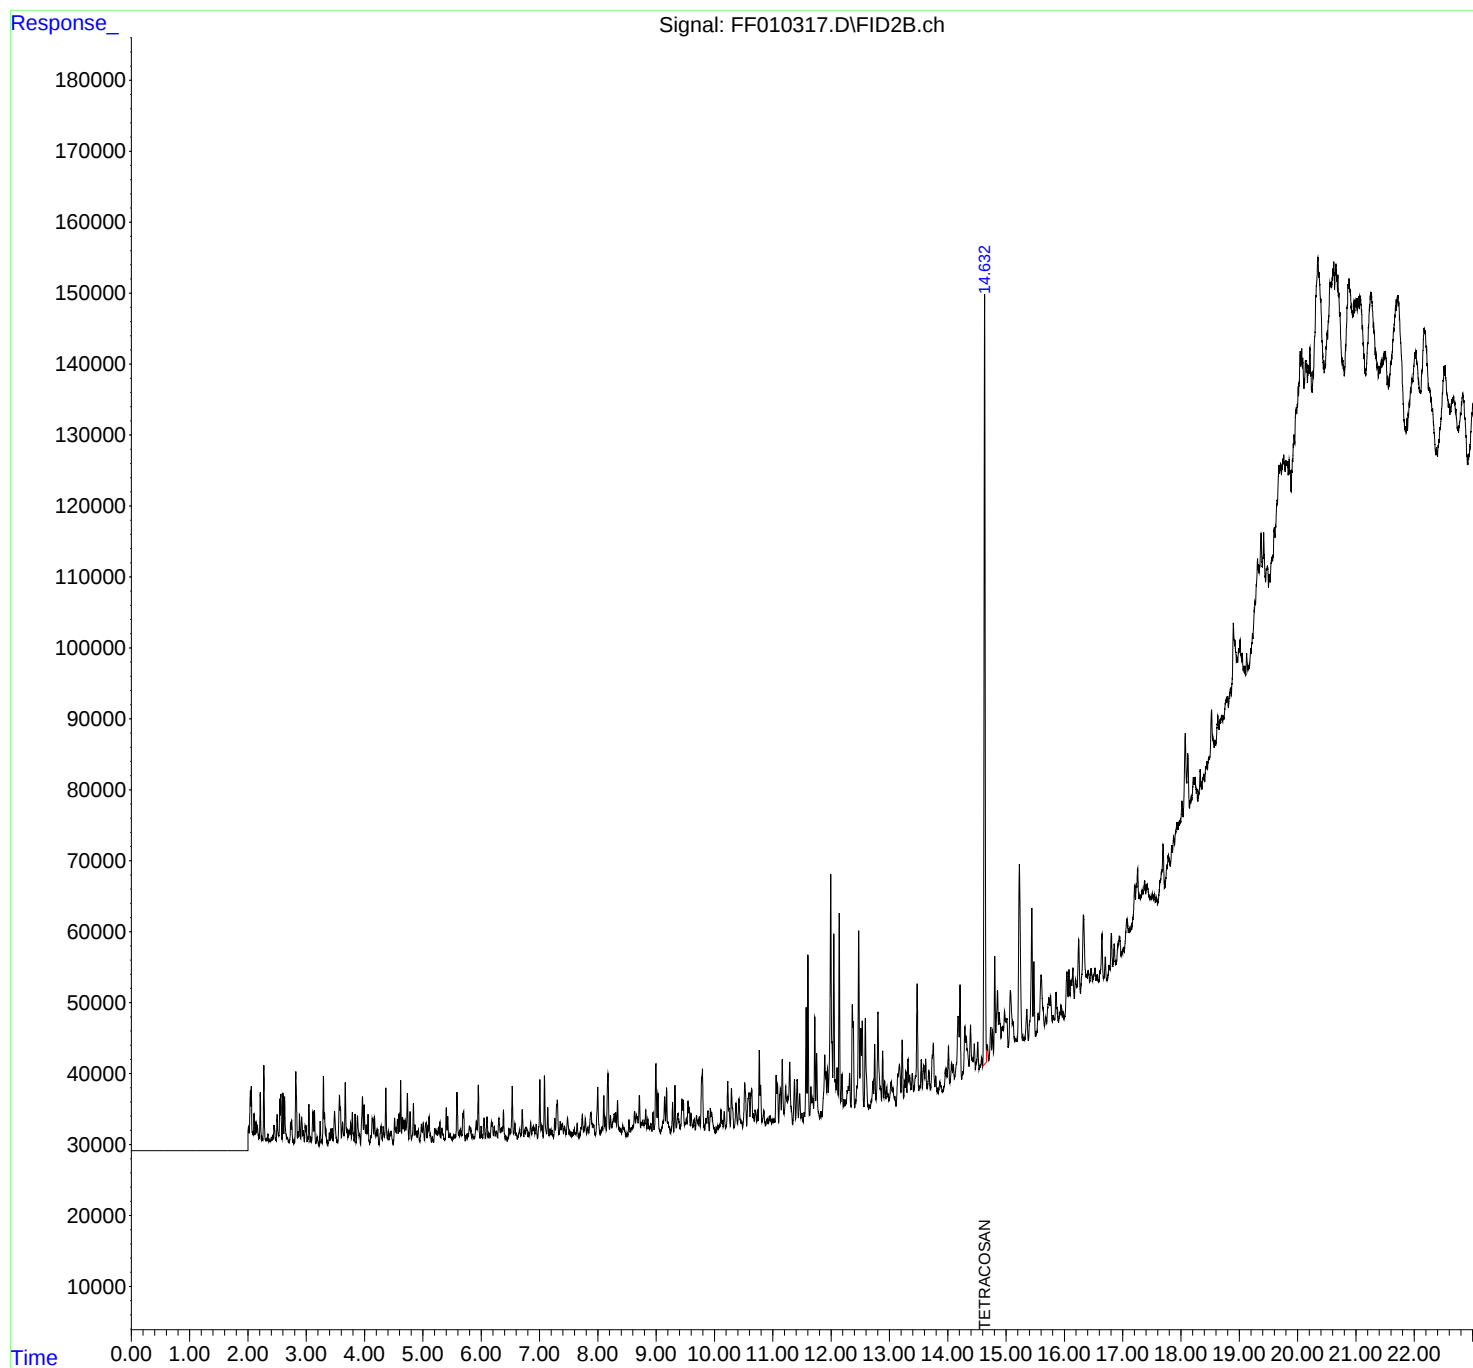

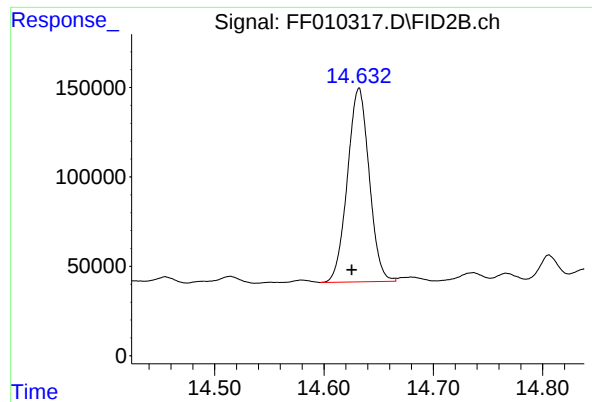

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.632 min
Delta R.T.: 0.006 min
Response: 1495969
Conc: 12.52 ug/ml

Instrument :

FID_F

ClientSampleId :

WC-14A-1A-4-6R-6