

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041019\
 Data File : FF004179.D
 Signal(s) : FID2B.ch
 Acq On : 10 Apr 2019 16:16
 Operator : AJ\SJ
 Sample : IDOC-1
 Misc : IDOC-DRO-1-FOR SS
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 11 02:13:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.538	1019093	7.839 ug/ml
Target Compounds			
2) N-DECANE	4.288	1083107	8.003 ug/ml
3) N-DODECANE	6.305	1128815	8.046 ug/ml
4) N-TETRADECANE	8.095	1097124	7.716 ug/ml
5) N-HEXADECANE	9.693	1173573	7.929 ug/ml
6) N-OCTADECANE	11.133	1208153	8.022 ug/ml
7) N-EICOSANE	12.440	1198830	7.977 ug/ml
8) N-DOCOSANE	13.638	1183314	7.906 ug/ml
10) N-TETRACOSANE	14.741	1181003	8.018 ug/mlm
11) N-HEXACOSANE	15.762	1195897	8.238 ug/ml
12) N-OCTACOSANE	16.712	1330981	9.256 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041019\
Data File : FF04179.D
Signal(s) : FID2B.ch
Acq On : 10 Apr 2019 16:16
Operator : AJ\SJ
Sample : IDOC-1
Misc : IDOC-DRO-1-FOR SS
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 11 02:13:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

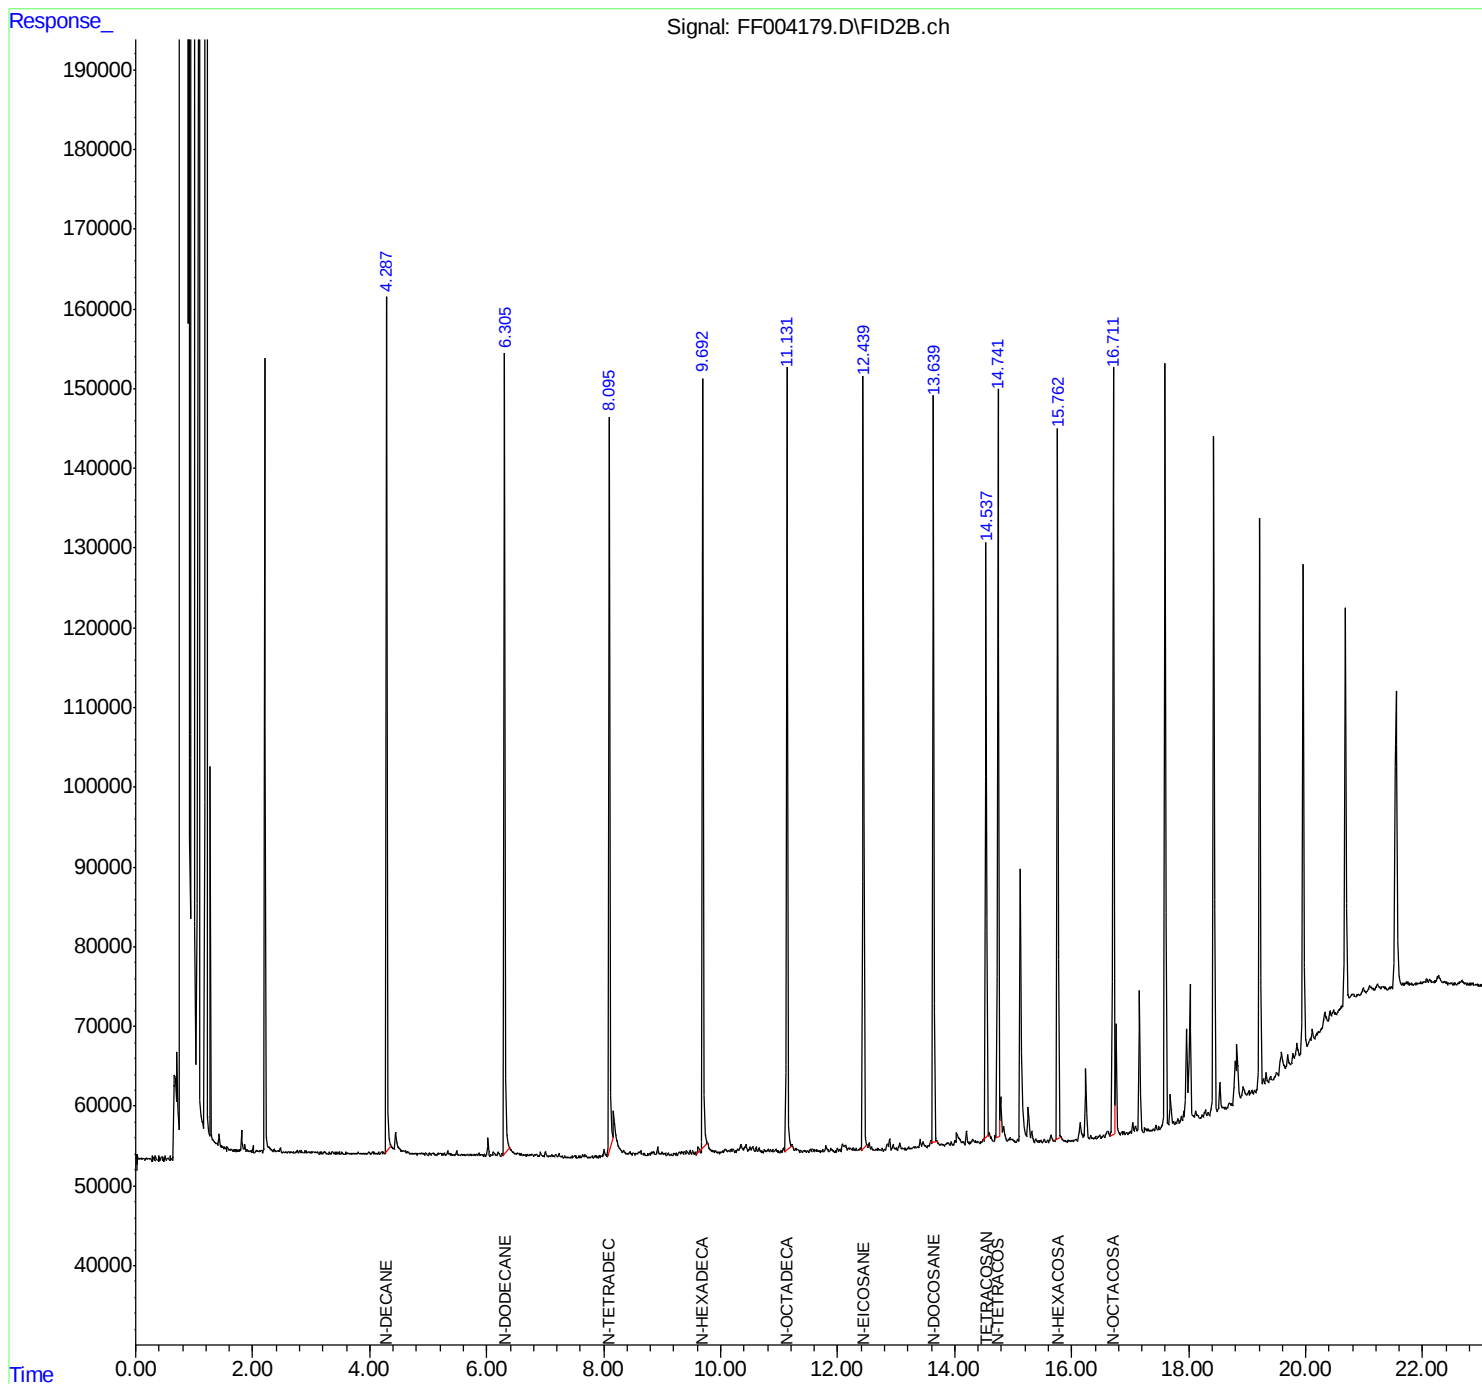

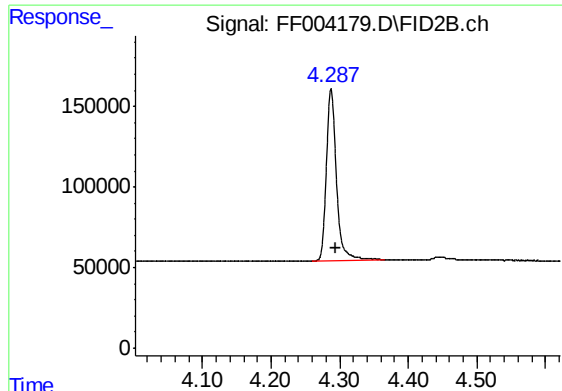


#2 N-DECANE

R.T.: 4.288 min
Delta R.T.: -0.006 min
Response: 1083107
Conc: 8.00 ug/ml

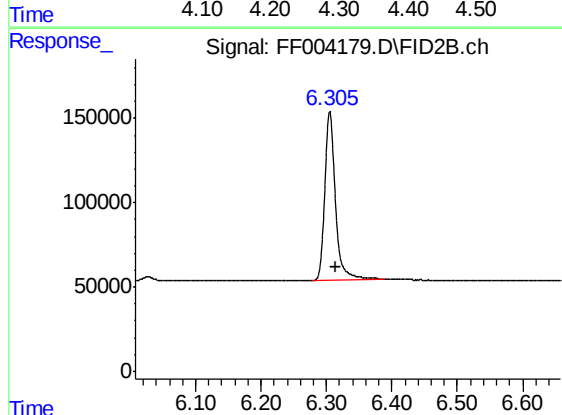


#3 N-DODECANE

R.T.: 6.305 min
Delta R.T.: -0.008 min
Response: 1128815
Conc: 8.05 ug/ml

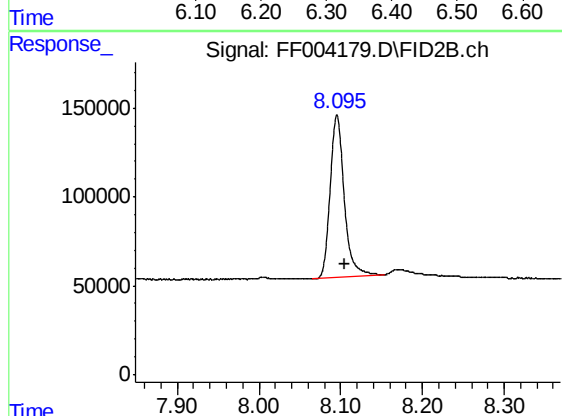


#4 N-TETRADECANE

R.T.: 8.095 min
Delta R.T.: -0.010 min
Response: 1097124
Conc: 7.72 ug/ml

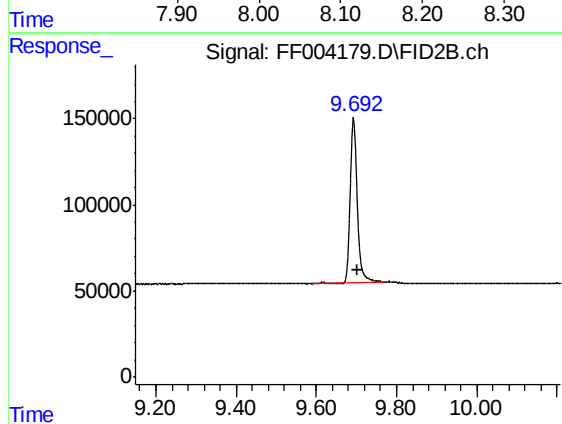


#5 N-HEXADECANE

R.T.: 9.693 min
Delta R.T.: -0.012 min
Response: 1173573
Conc: 7.93 ug/ml

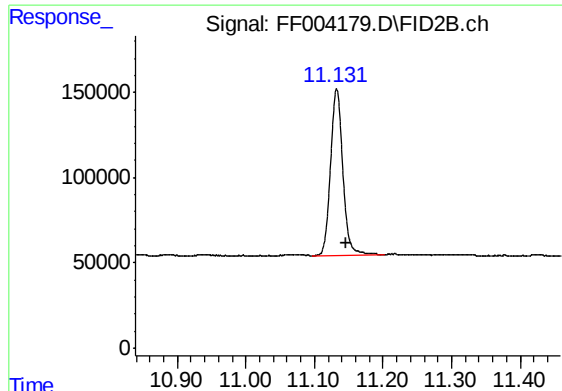


#6 N-OCTADECANE

R.T.: 11.133 min
Delta R.T.: -0.014 min
Response: 1208153
Conc: 8.02 ug/ml

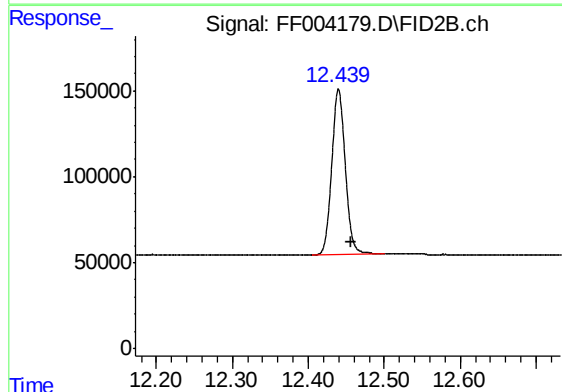


#7 N-EICOSANE

R.T.: 12.440 min
Delta R.T.: -0.016 min
Response: 1198830
Conc: 7.98 ug/ml

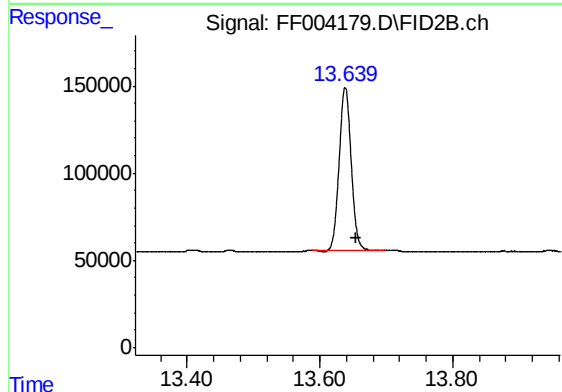


#8 N-DOCOSANE

R.T.: 13.638 min
Delta R.T.: -0.016 min
Response: 1183314
Conc: 7.91 ug/ml

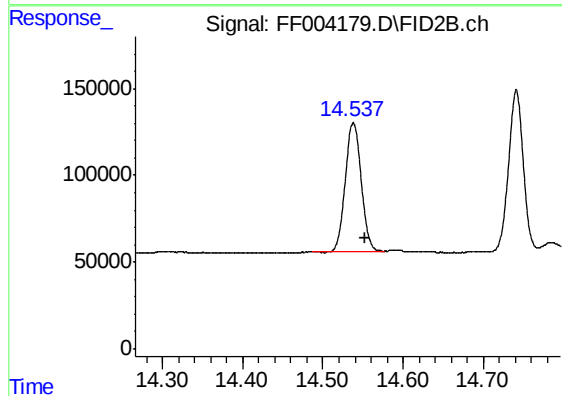


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.538 min
Delta R.T.: -0.016 min
Response: 1019093
Conc: 7.84 ug/ml

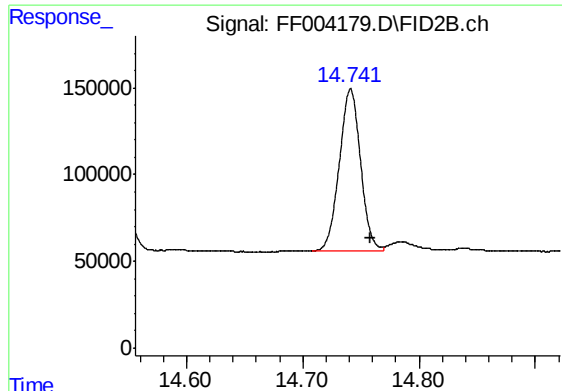


#10 N-TETRACOSANE

R.T.: 14.741 min
Delta R.T.: -0.017 min
Response: 1181003
Conc: 8.02 ug/ml m

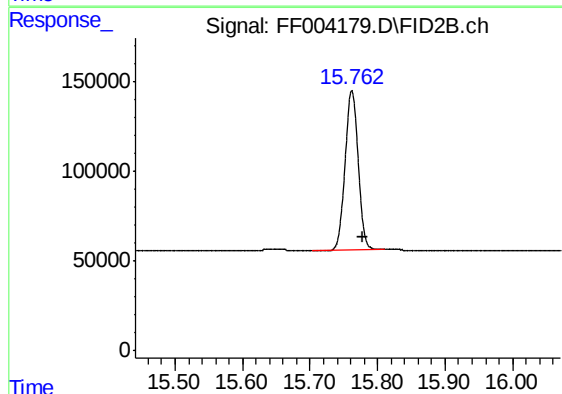

#11 N-HEXACOSANE

R.T.: 15.762 min
Delta R.T.: -0.016 min
Response: 1195897
Conc: 8.24 ug/ml

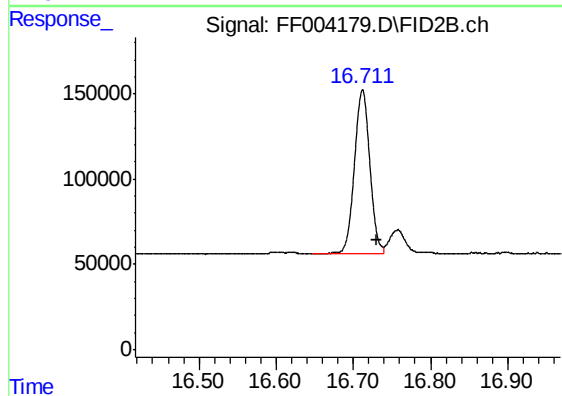

#12 N-OCTACOSANE

R.T.: 16.712 min
Delta R.T.: -0.018 min
Response: 1330981
Conc: 9.26 ug/ml