

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041019\
 Data File : FF004180.D
 Signal(s) : FID2B.ch
 Acq On : 10 Apr 2019 16:48
 Operator : AJ\SJ
 Sample : IDOC-2
 Misc : IDOC-DRO-2-FOR SS
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 11 02:14:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.538	1639528	12.612 ug/ml
Target Compounds			
2) N-DECANE	4.289	1421397	10.503 ug/ml
3) N-DODECANE	6.305	1513814	10.790 ug/ml
4) N-TETRADECANE	8.095	1609180	11.317 ug/ml
5) N-HEXADECANE	9.693	1702733	11.505 ug/ml
6) N-OCTADECANE	11.132	1741288	11.563 ug/ml
7) N-EICOSANE	12.441	1744837	11.611 ug/ml
8) N-DOCOSANE	13.638	1752604	11.709 ug/ml
10) N-TETRACOSANE	14.741	1703826	11.567 ug/ml
11) N-HEXACOSANE	15.763	1761849	12.136 ug/ml
12) N-OCTACOSANE	16.713	1857296	12.917 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041019\
Data File : FF004180.D
Signal(s) : FID2B.ch
Acq On : 10 Apr 2019 16:48
Operator : AJ\SJ
Sample : IDOC-2
Misc : IDOC-DRO-2-FOR SS
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 11 02:14:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

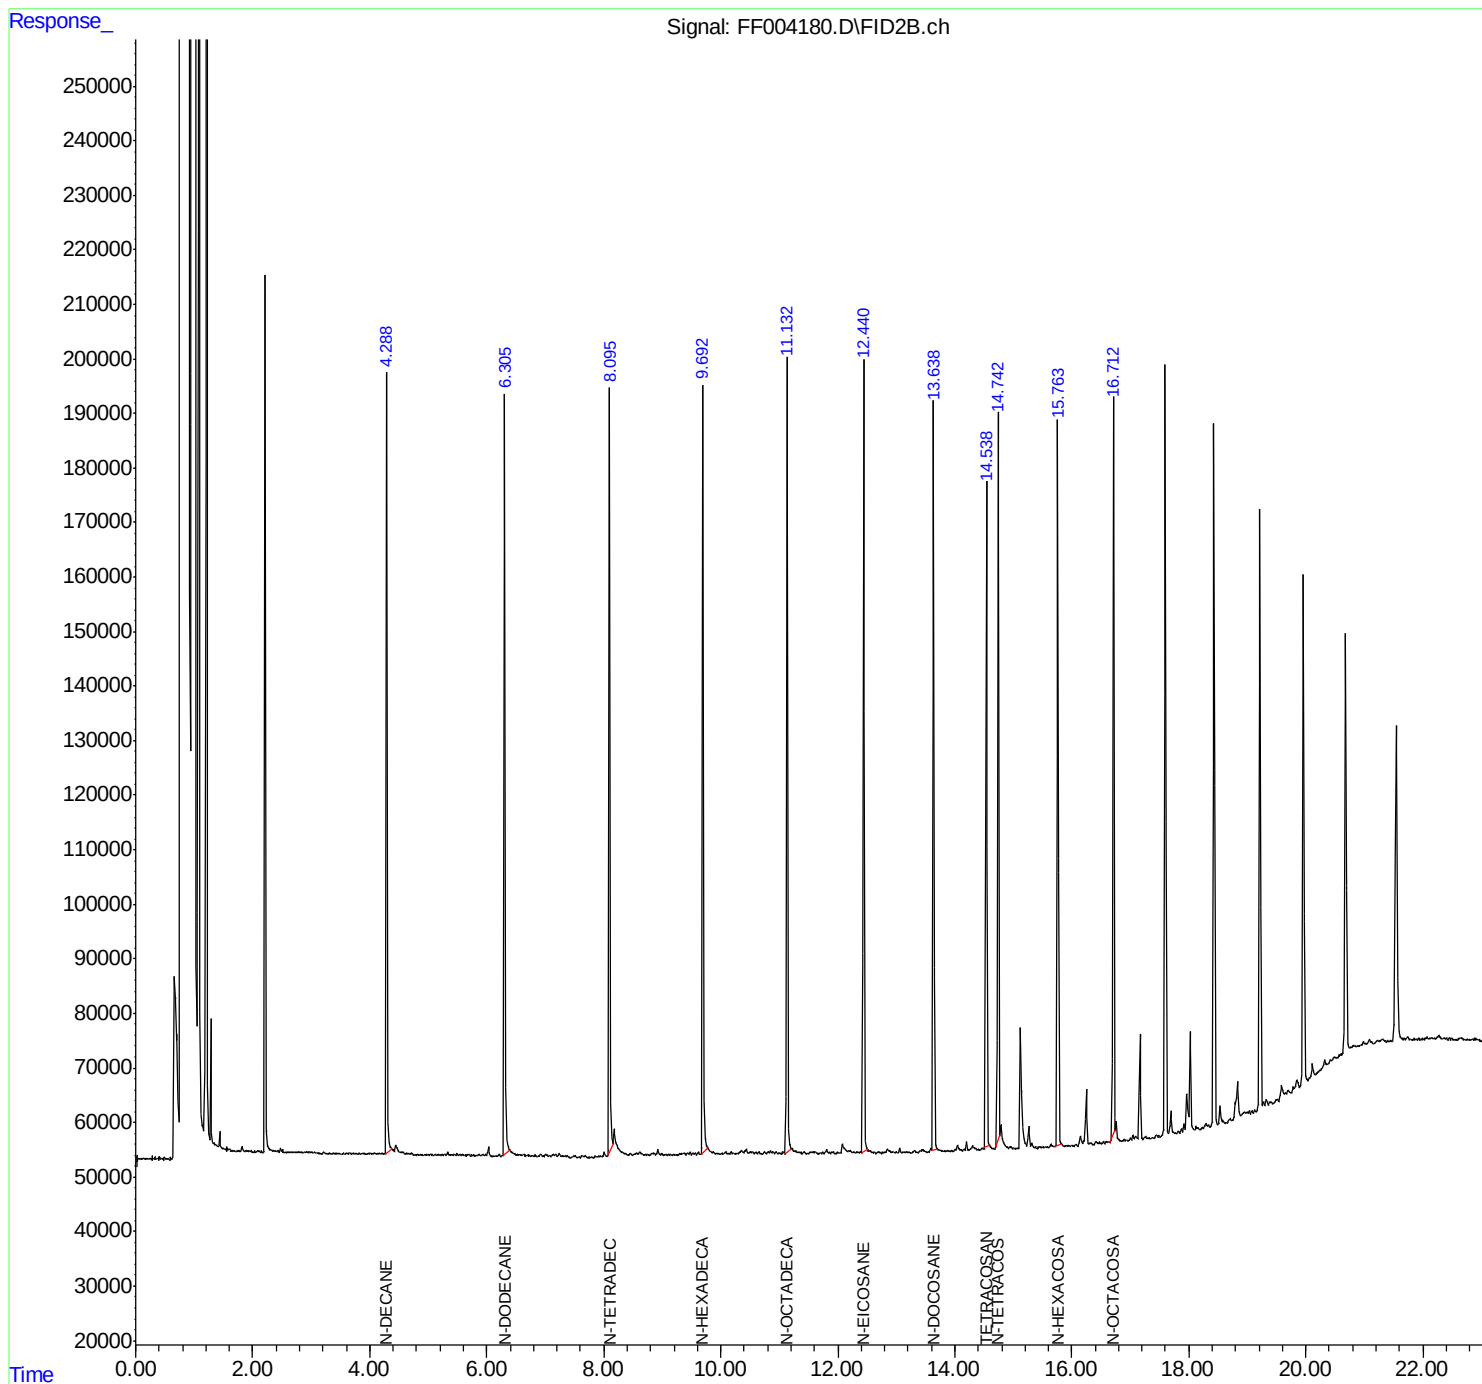

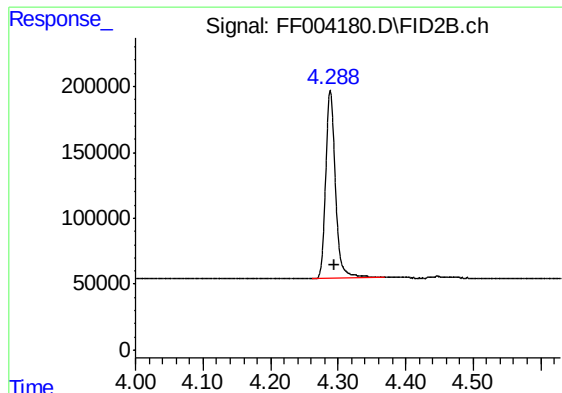


#2 N-DECANE

R.T.: 4.289 min
Delta R.T.: -0.005 min
Response: 1421397
Conc: 10.50 ug/ml

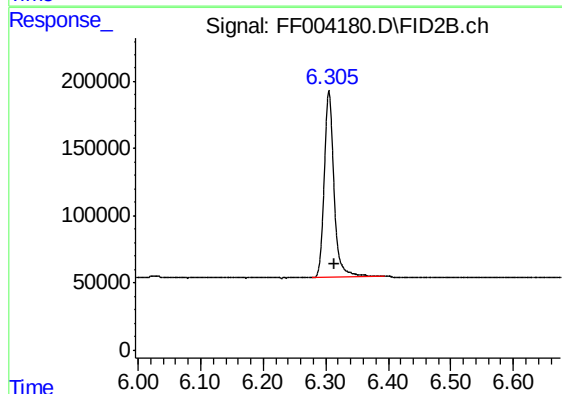


#3 N-DODECANE

R.T.: 6.305 min
Delta R.T.: -0.008 min
Response: 1513814
Conc: 10.79 ug/ml

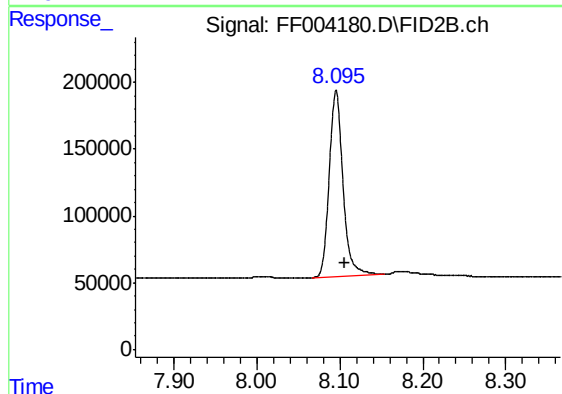


#4 N-TETRADECANE

R.T.: 8.095 min
Delta R.T.: -0.010 min
Response: 1609180
Conc: 11.32 ug/ml

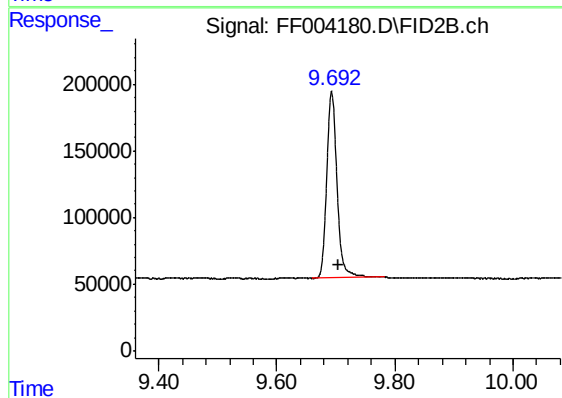


#5 N-HEXADECANE

R.T.: 9.693 min
Delta R.T.: -0.011 min
Response: 1702733
Conc: 11.50 ug/ml

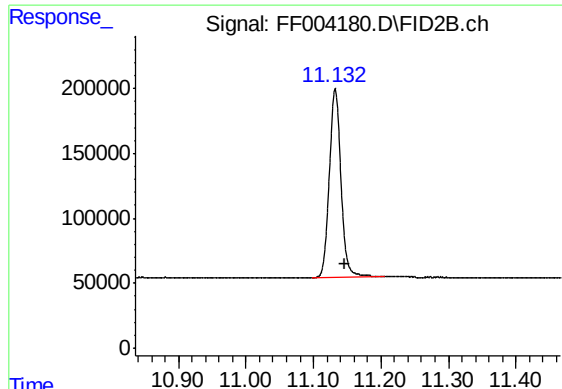


#6 N-OCTADECANE

R.T.: 11.132 min
Delta R.T.: -0.014 min
Response: 1741288
Conc: 11.56 ug/ml

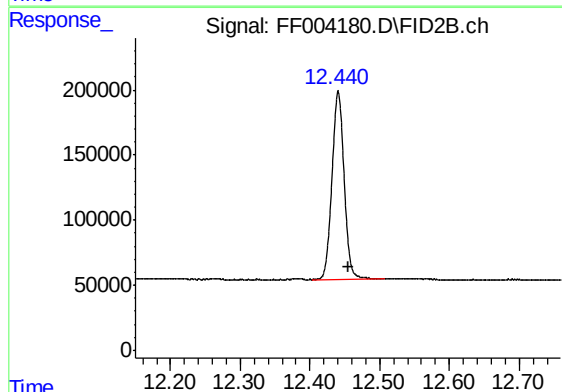


#7 N-EICOSANE

R.T.: 12.441 min
Delta R.T.: -0.015 min
Response: 1744837
Conc: 11.61 ug/ml

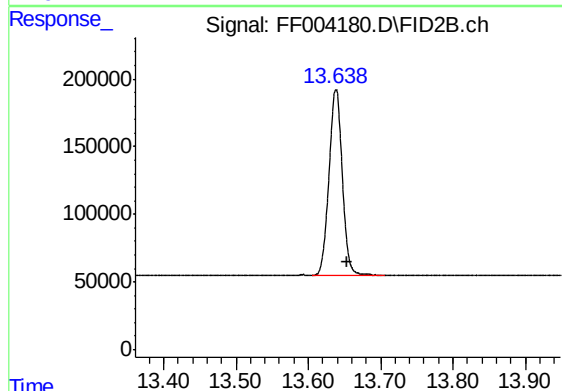


#8 N-DOCOSANE

R.T.: 13.638 min
Delta R.T.: -0.015 min
Response: 1752604
Conc: 11.71 ug/ml

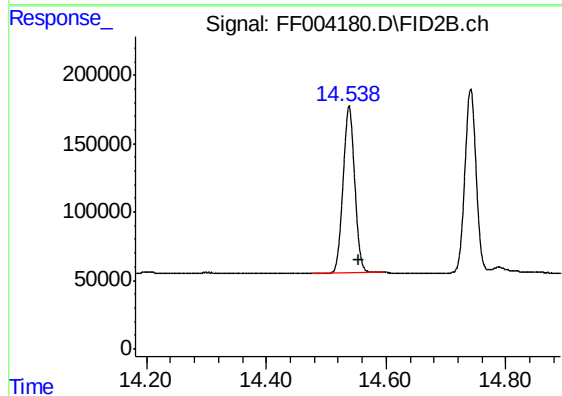


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.538 min
Delta R.T.: -0.015 min
Response: 1639528
Conc: 12.61 ug/ml

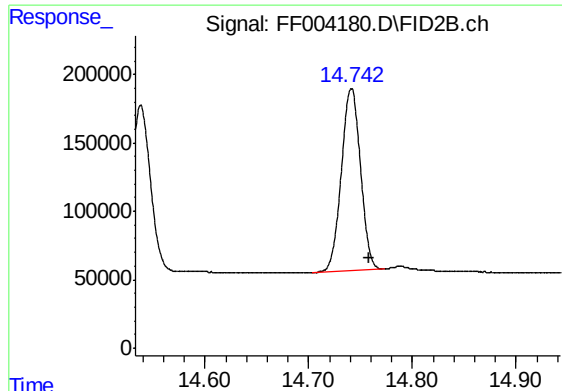


#10 N-TETRACOSANE

R.T.: 14.741 min
Delta R.T.: -0.016 min
Response: 1703826
Conc: 11.57 ug/ml

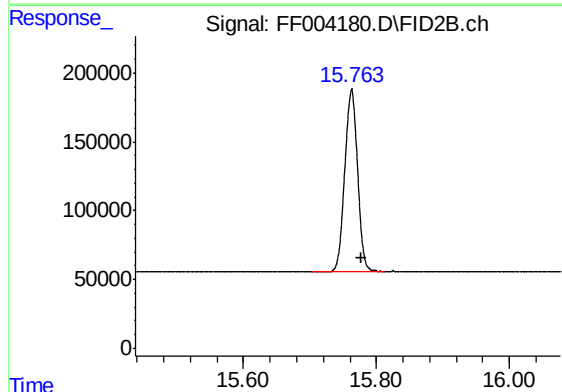

#11 N-HEXACOSANE

R.T.: 15.763 min
Delta R.T.: -0.015 min
Response: 1761849
Conc: 12.14 ug/ml

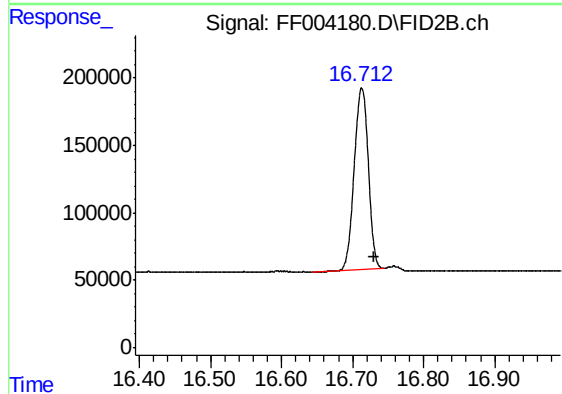

#12 N-OCTACOSANE

R.T.: 16.713 min
Delta R.T.: -0.017 min
Response: 1857296
Conc: 12.92 ug/ml