

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041023\
 Data File : FF012436.D
 Signal(s) : FID2B.ch
 Acq On : 10 Apr 2023 09:24
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 10 12:00:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.740	2370384	19.121 ug/ml
12)	N-OCTACOSANE	17.184	2425802	21.088 ug/ml
13)	N-TRIACONTANE	18.076	58930	0.536 ug/ml
14)	N-DOTRIACONTANE	18.903	81546	0.786 ug/ml
15)	N-TETRATRIACONTANE	19.682	68415	0.723 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041023\
Data File : FF012436.D
Signal(s) : FID2B.ch
Acq On : 10 Apr 2023 09:24
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 12:00:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

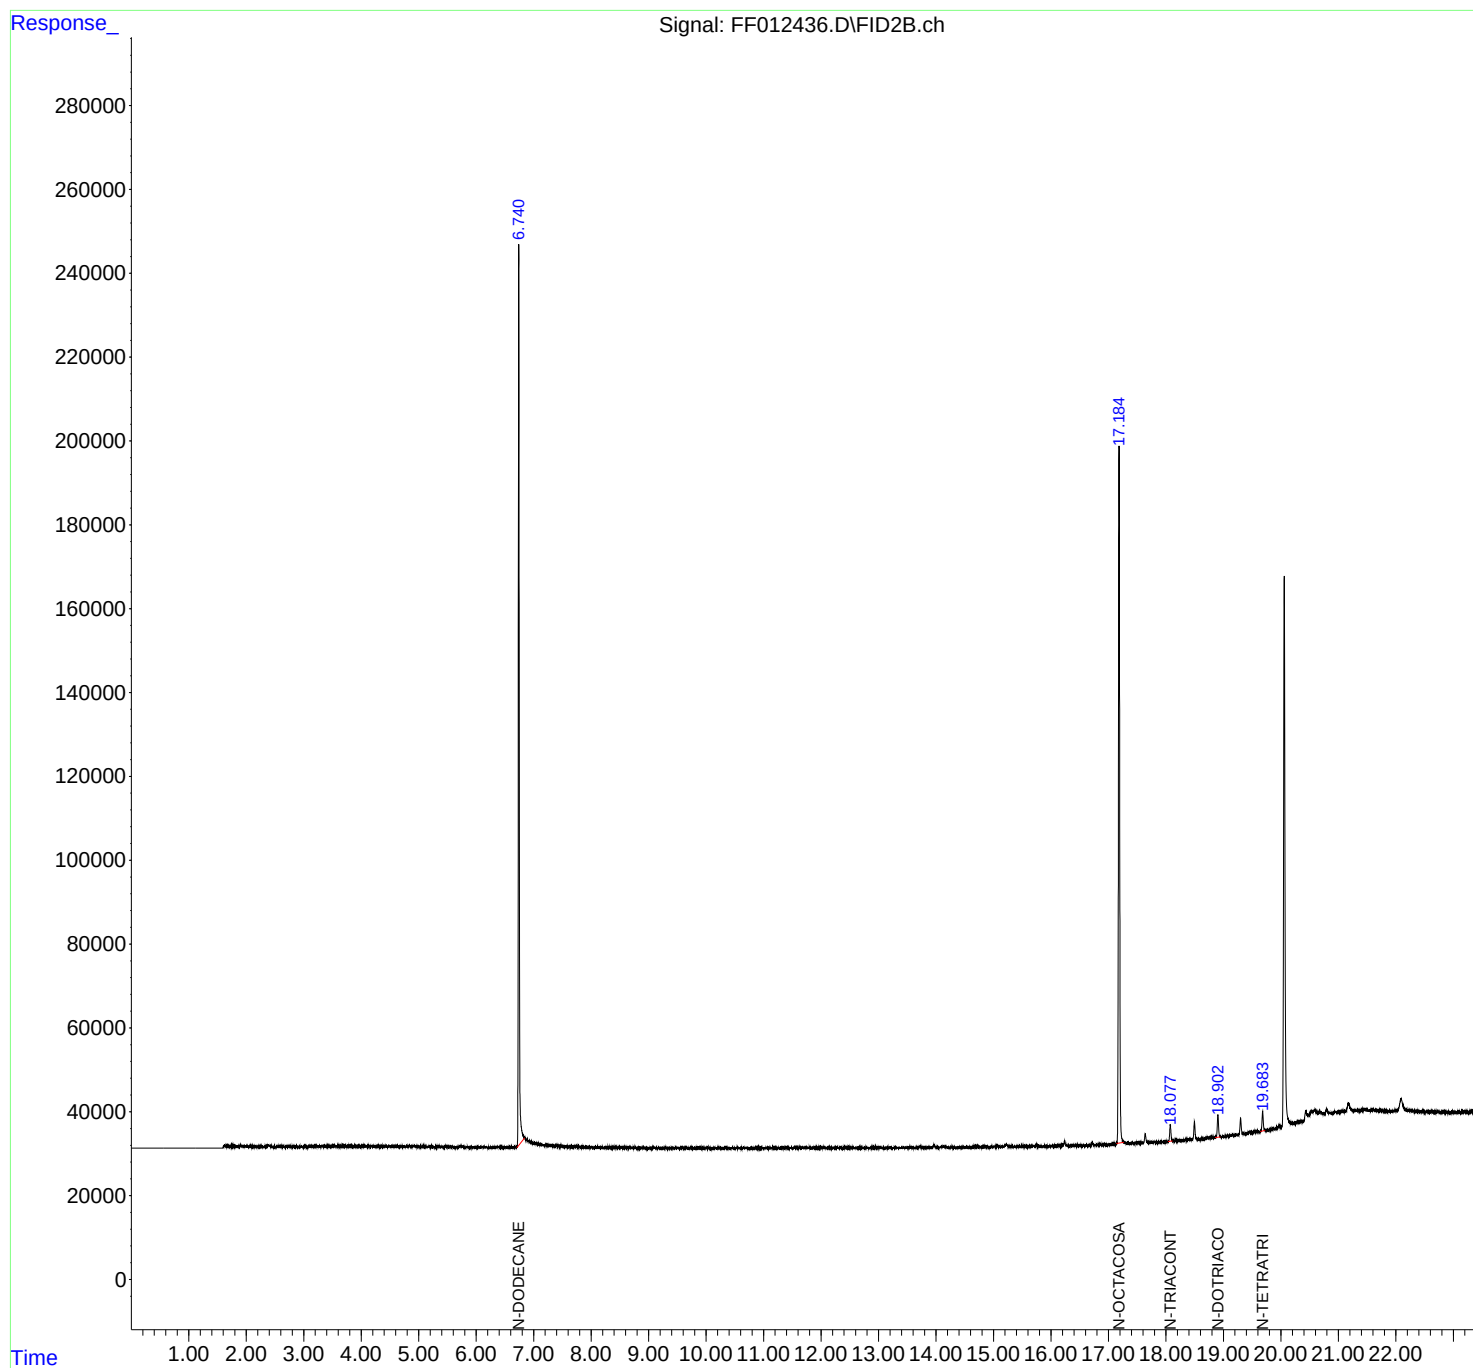

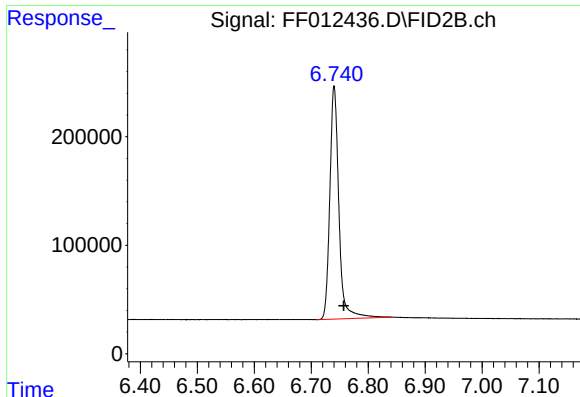


#3 N-DODECANE

R.T.: 6.740 min
Delta R.T.: -0.017 min
Response: 2370384
Conc: 19.12 ug/ml

Instrument :


FID_F

ClientSampleId :

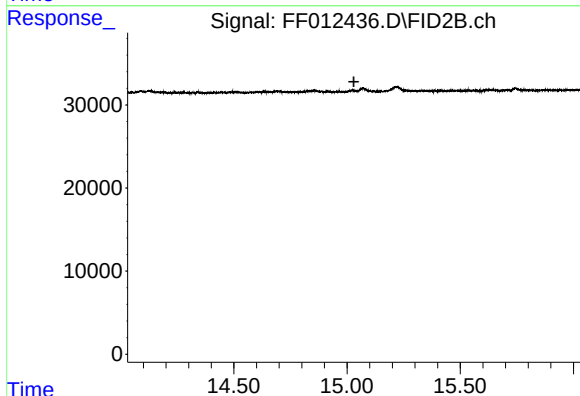


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.030 min
Response: 0
Conc: N.D.

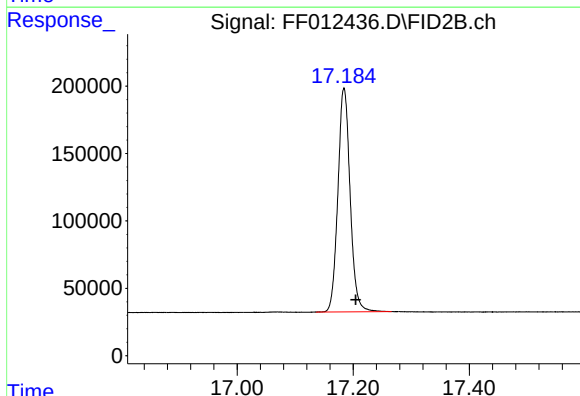


#12 N-OCTACOSANE

R.T.: 17.184 min
Delta R.T.: -0.020 min
Response: 2425802
Conc: 21.09 ug/ml

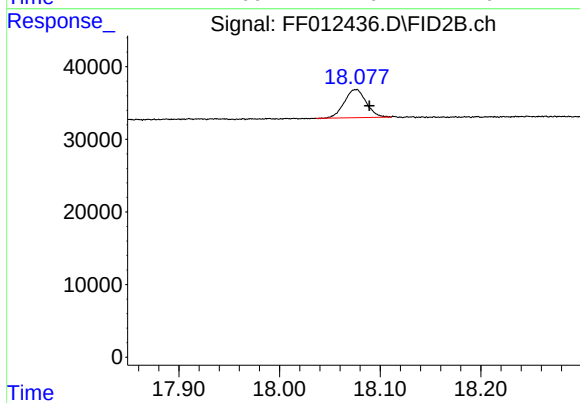

#13 N-TRIACONTANE


R.T.: 18.076 min
Delta R.T.: -0.013 min
Response: 58930
Conc: 0.54 ug/ml

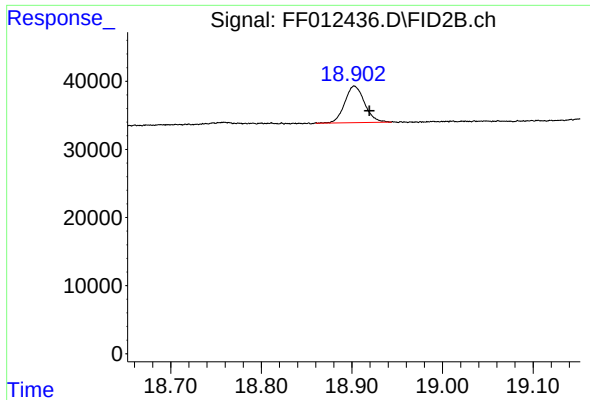

#14 N-DOTRIACONTANE

R.T.: 18.903 min
Delta R.T.: -0.017 min
Response: 81546
Conc: 0.79 ug/ml

Instrument :
FID_F
ClientSampleId :

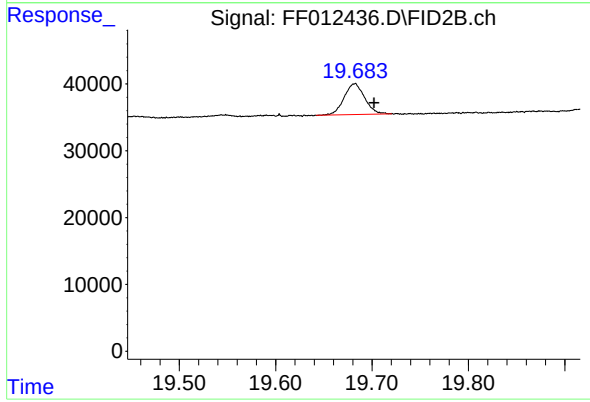

#15 N-TETRATRIACONTANE

R.T.: 19.682 min
Delta R.T.: -0.020 min
Response: 68415
Conc: 0.72 ug/ml