

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041023\
 Data File : FF012437.D
 Signal(s) : FID2B.ch
 Acq On : 10 Apr 2023 09:53
 Operator : YP\AJ
 Sample : PB151967BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 10 12:00:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.014	2070440	18.500 ug/ml
Target Compounds			
12) N-OCTACOSANE	17.193	55099	0.479 ug/ml
13) N-TRIACONTANE	18.077	90631	0.824 ug/ml
14) N-DOTRIACONTANE	18.909	113118	1.090 ug/ml
15) N-TETRATRIACONTANE	19.693	70663	0.747 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041023\
Data File : FF012437.D
Signal(s) : FID2B.ch
Acq On : 10 Apr 2023 09:53
Operator : YP\AJ
Sample : PB151967BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 12:00:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

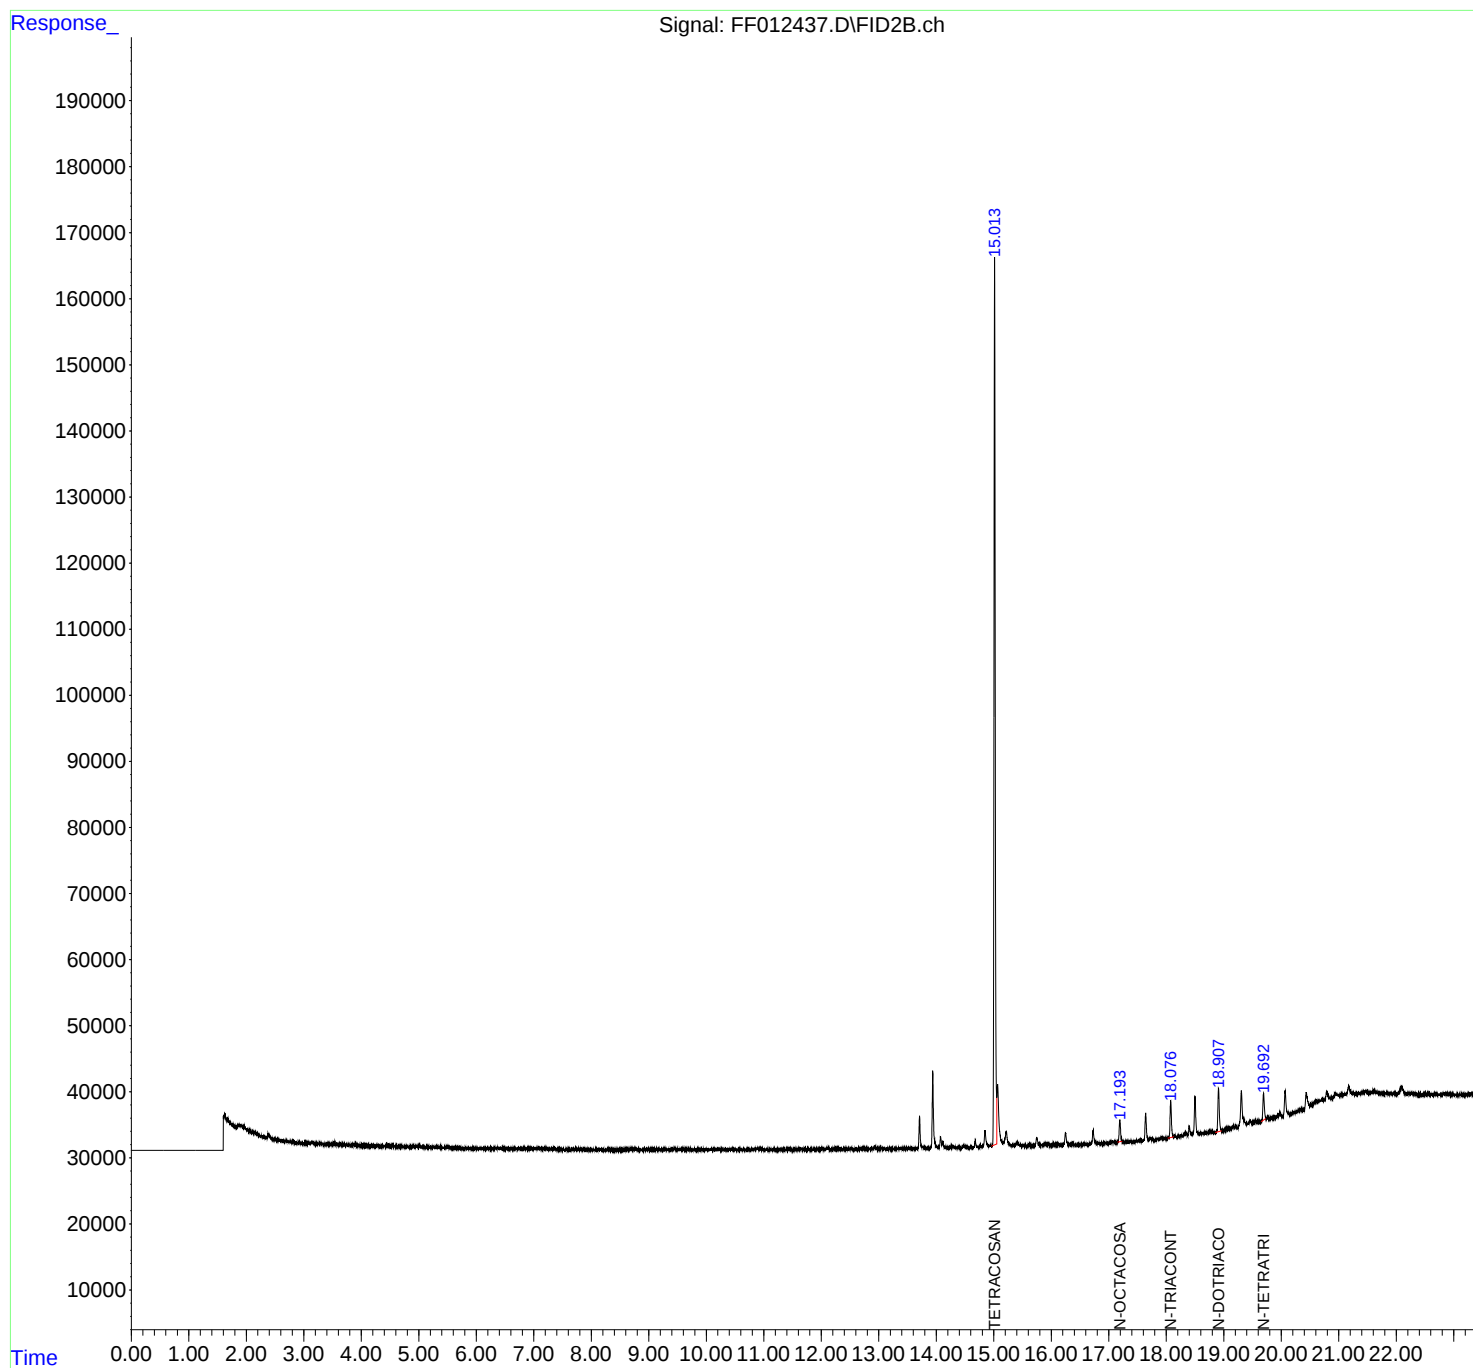


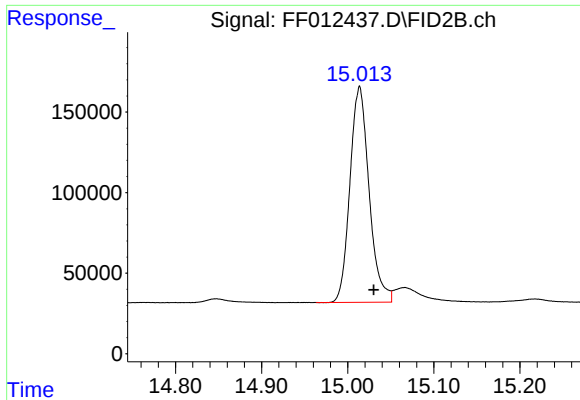

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.014 min
Delta R.T.: -0.016 min
Response: 2070440
Conc: 18.50 ug/ml

Instrument :
FID_F
ClientSampleId :

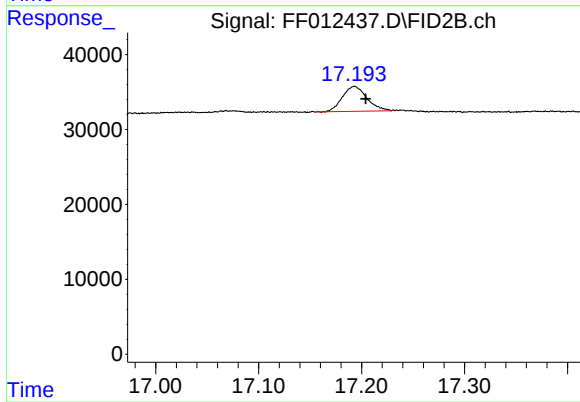


#12 N-OCTACOSANE

R.T.: 17.193 min
Delta R.T.: -0.011 min
Response: 55099
Conc: 0.48 ug/ml

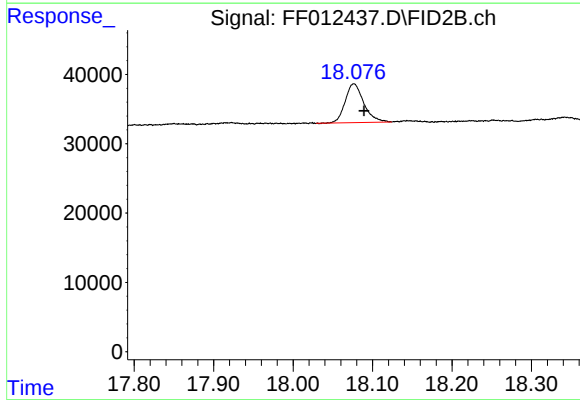


#13 N-TRIACONTANE

R.T.: 18.077 min
Delta R.T.: -0.013 min
Response: 90631
Conc: 0.82 ug/ml

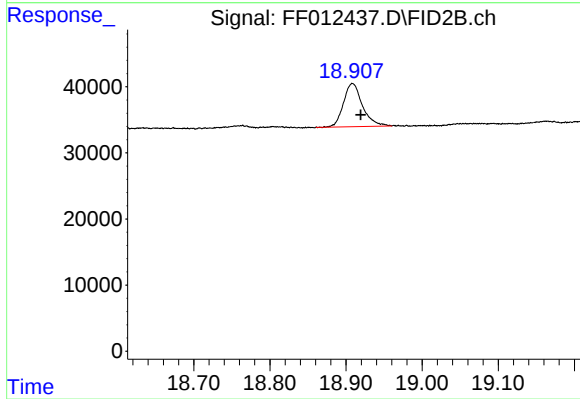

#14 N-DOTRIACONTANE

R.T.: 18.909 min
Delta R.T.: -0.011 min
Response: 113118
Conc: 1.09 ug/ml

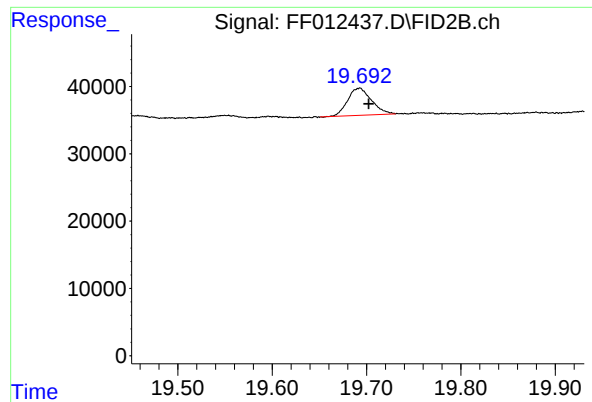

#15 N-TETRATRIACONTANE

R.T.: 19.693 min
Delta R.T.: -0.009 min
Response: 70663
Conc: 0.75 ug/ml

Instrument :

FID_F

ClientSampleId :