

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041122\
 Data File : FF010324.D
 Signal(s) : FID2B.ch
 Acq On : 11 Apr 2022 12:45
 Operator : AJ\MA
 Sample : N2335-02 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 12 01:09:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.633	987844	8.265 ug/ml
Target Compounds			
4) N-TETRADECANE	8.131	250464	1.889 ug/ml
5) N-HEXADECANE	9.790	943176	7.104 ug/ml
6) N-OCTADECANE	11.201	171601	1.248 ug/ml
7) N-EICOSANE	12.518	410045	3.052 ug/ml
8) N-DOCOSANE	13.757	1195292	8.933 ug/ml
10) N-TETRACOSANE	14.814	1916369	14.311 ug/ml
11) N-HEXACOSANE	15.801	97824	0.738 ug/ml
12) N-OCTACOSANE	16.810	352529	2.660 ug/ml
13) N-TRIACONTANE	17.696	448602	3.398 ug/ml
14) N-DOTRIACONTANE	18.526	175062	1.356 ug/ml
15) N-TETRATRIACONTANE	19.311	124763	1.072 ug/ml
16) N-HEXATRIACONTANE	20.050	208674	2.001 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041122\
Data File : FF010324.D
Signal(s) : FID2B.ch
Acq On : 11 Apr 2022 12:45
Operator : AJ\MA
Sample : N2335-02 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 01:09:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

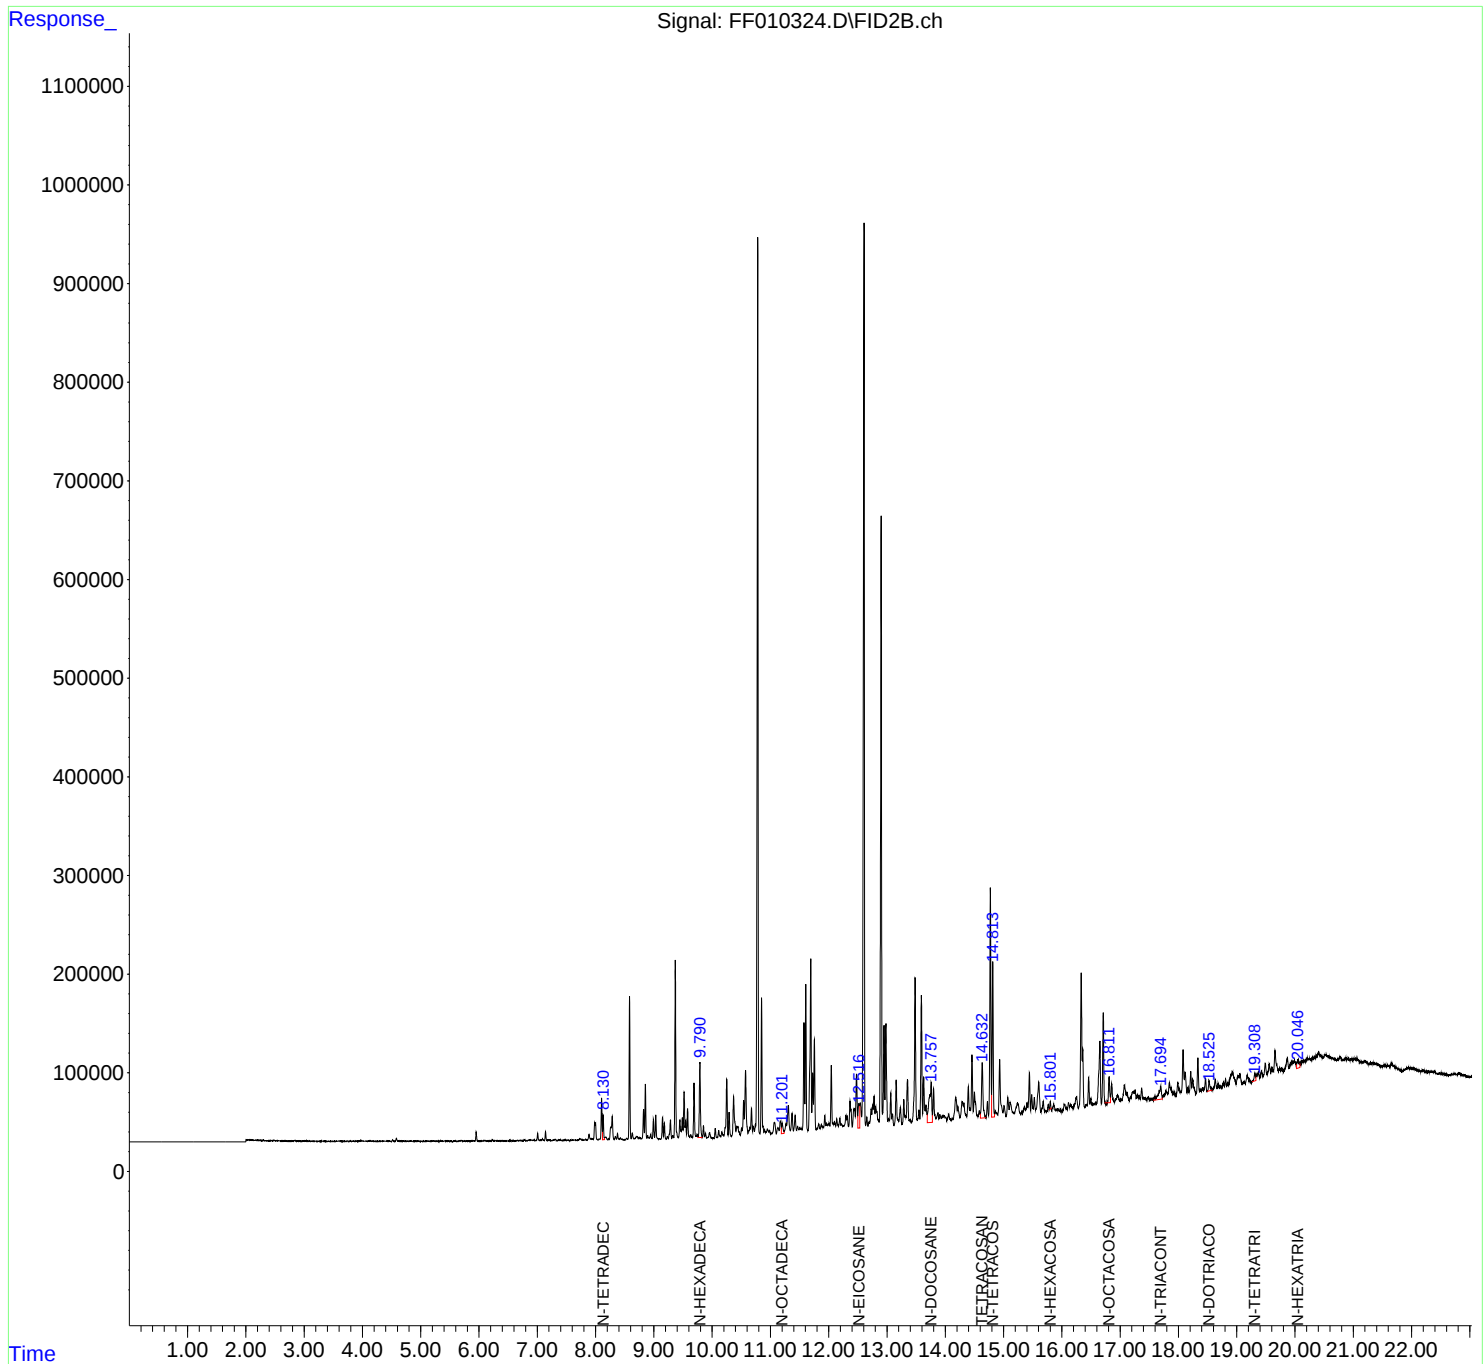


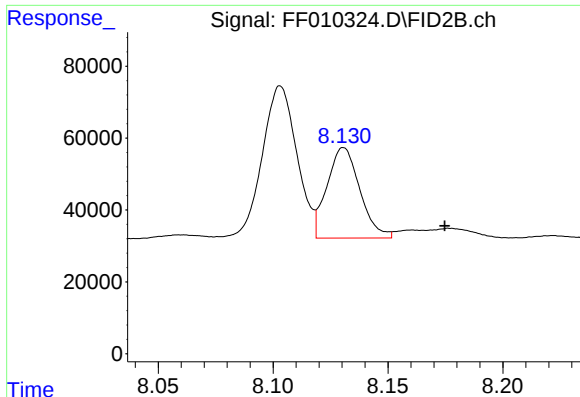

#4 N-TETRADECANE


R.T.: 8.131 min
Delta R.T.: -0.044 min
Response: 250464
Conc: 1.89 ug/ml

Instrument :
FID_F
ClientSampleId :

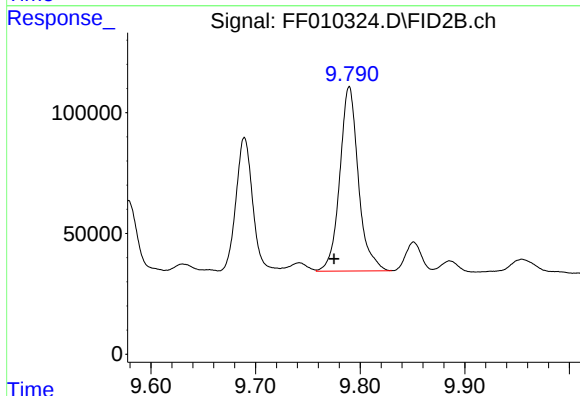


#5 N-HEXADECANE

R.T.: 9.790 min
Delta R.T.: 0.014 min
Response: 943176
Conc: 7.10 ug/ml

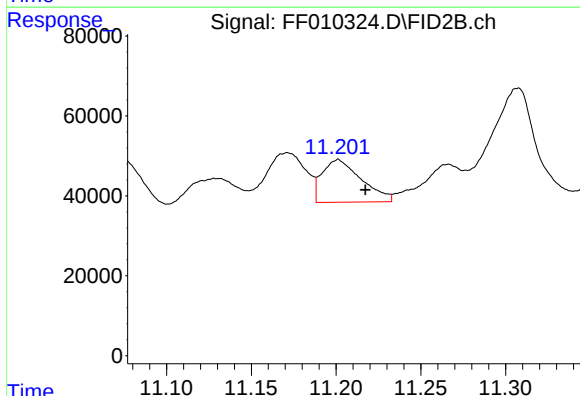


#6 N-OCTADECANE

R.T.: 11.201 min
Delta R.T.: -0.016 min
Response: 171601
Conc: 1.25 ug/ml

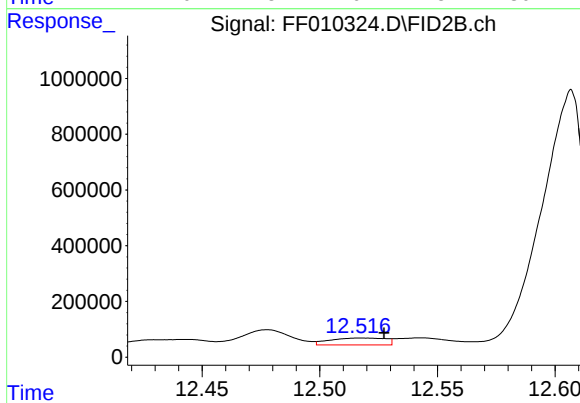

#7 N-EICOSANE


R.T.: 12.518 min
Delta R.T.: -0.009 min
Response: 410045
Conc: 3.05 ug/ml

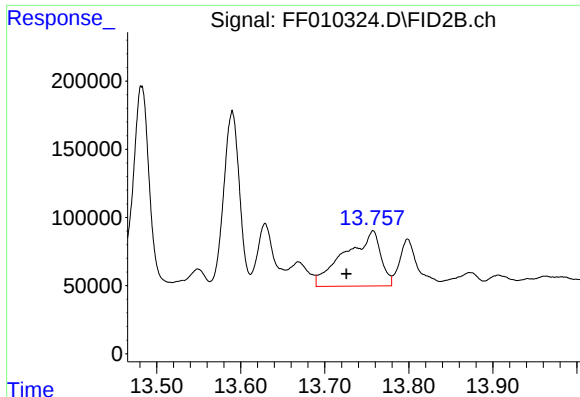

#8 N-DOCOSANE


R.T.: 13.757 min
Delta R.T.: 0.032 min
Response: 1195292
Conc: 8.93 ug/ml

Instrument :
FID_F
ClientSampleId :

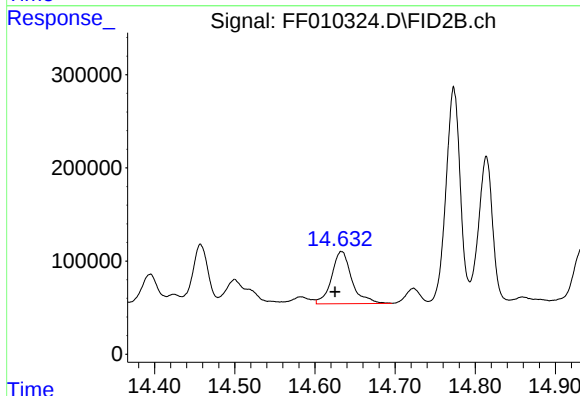


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.633 min
Delta R.T.: 0.008 min
Response: 987844
Conc: 8.26 ug/ml

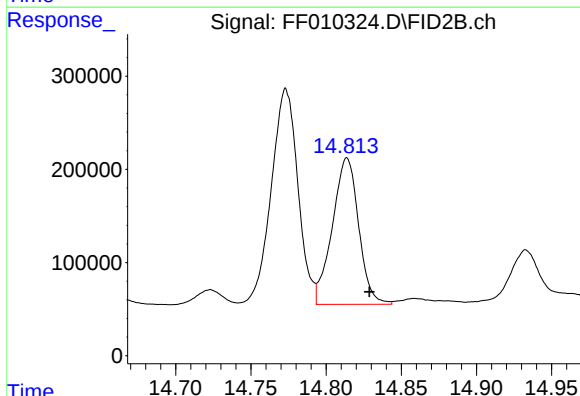


#10 N-TETRACOSANE

R.T.: 14.814 min
Delta R.T.: -0.015 min
Response: 1916369
Conc: 14.31 ug/ml

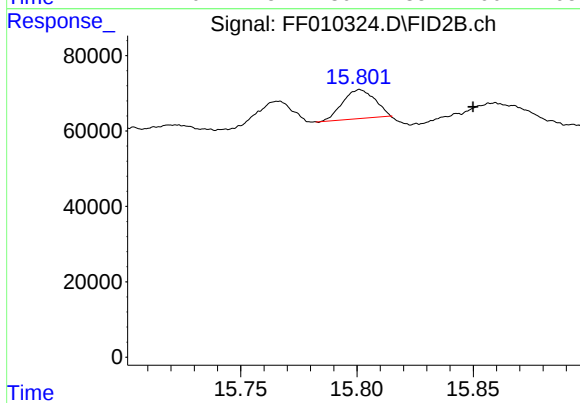

#11 N-HEXACOSANE


R.T.: 15.801 min
Delta R.T.: -0.048 min
Response: 97824
Conc: 0.74 ug/ml

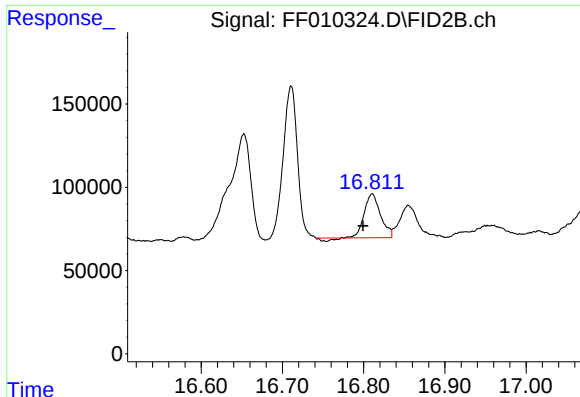

#12 N-OCTACOSANE


R.T.: 16.810 min
Delta R.T.: 0.011 min
Response: 352529
Conc: 2.66 ug/ml

Instrument :
FID_F
ClientSampleId :

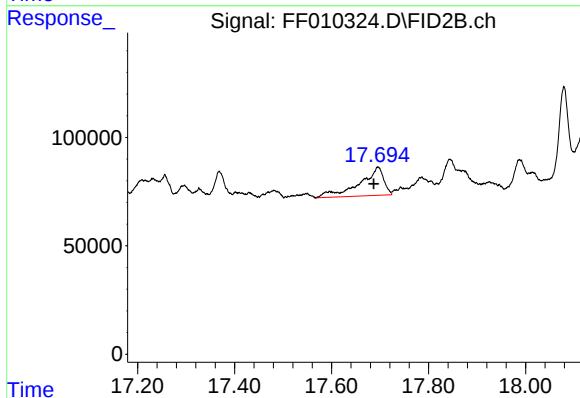


#13 N-TRIACONTANE

R.T.: 17.696 min
Delta R.T.: 0.009 min
Response: 448602
Conc: 3.40 ug/ml

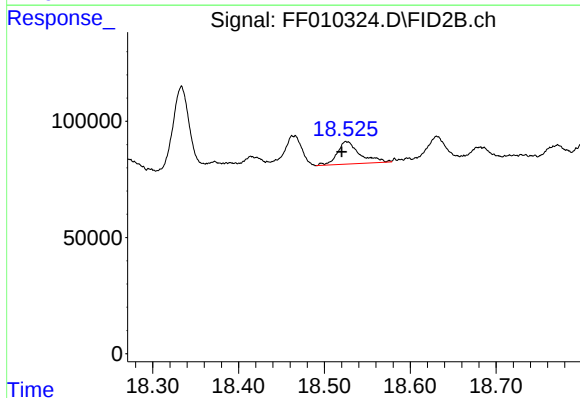


#14 N-DOTRIACONTANE

R.T.: 18.526 min
Delta R.T.: 0.006 min
Response: 175062
Conc: 1.36 ug/ml

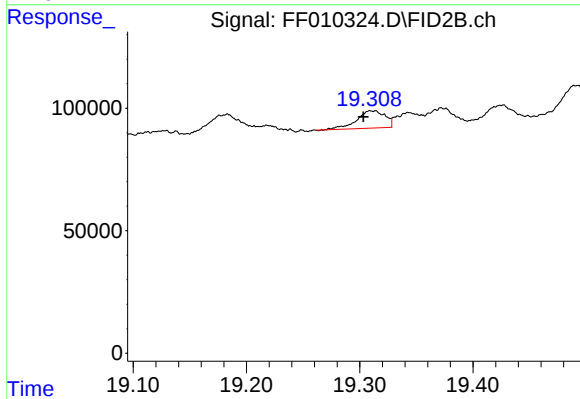

#15 N-TETRATRIACONTANE

R.T.: 19.311 min
Delta R.T.: 0.008 min
Response: 124763
Conc: 1.07 ug/ml

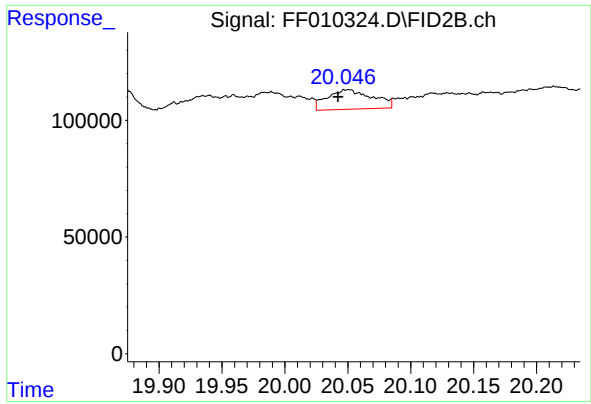

#16 N-HEXATRIACONTANE

R.T.: 20.050 min
Delta R.T.: 0.007 min
Response: 208674
Conc: 2.00 ug/ml

Instrument :
FID_F
ClientSampleId :