

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041122\
 Data File : FF010325.D
 Signal(s) : FID2B.ch
 Acq On : 11 Apr 2022 14:03
 Operator : AJ\MA
 Sample : N2336-02 5X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 12 01:10:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.628	361231	3.022 ug/ml
Target Compounds			
7) N-EICOSANE	12.585f	189676	1.412 ug/ml
10) N-TETRACOSANE	14.803	110506	0.825 ug/ml
13) N-TRIACONTANE	17.694	303829	2.301 ug/ml
15) N-TETRATRIACONTANE	19.235f	15164	0.130 ug/ml
16) N-HEXATRIACONTANE	20.044	59596	0.571 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041122\
Data File : FF010325.D
Signal(s) : FID2B.ch
Acq On : 11 Apr 2022 14:03
Operator : AJ\MA
Sample : N2336-02 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 01:10:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

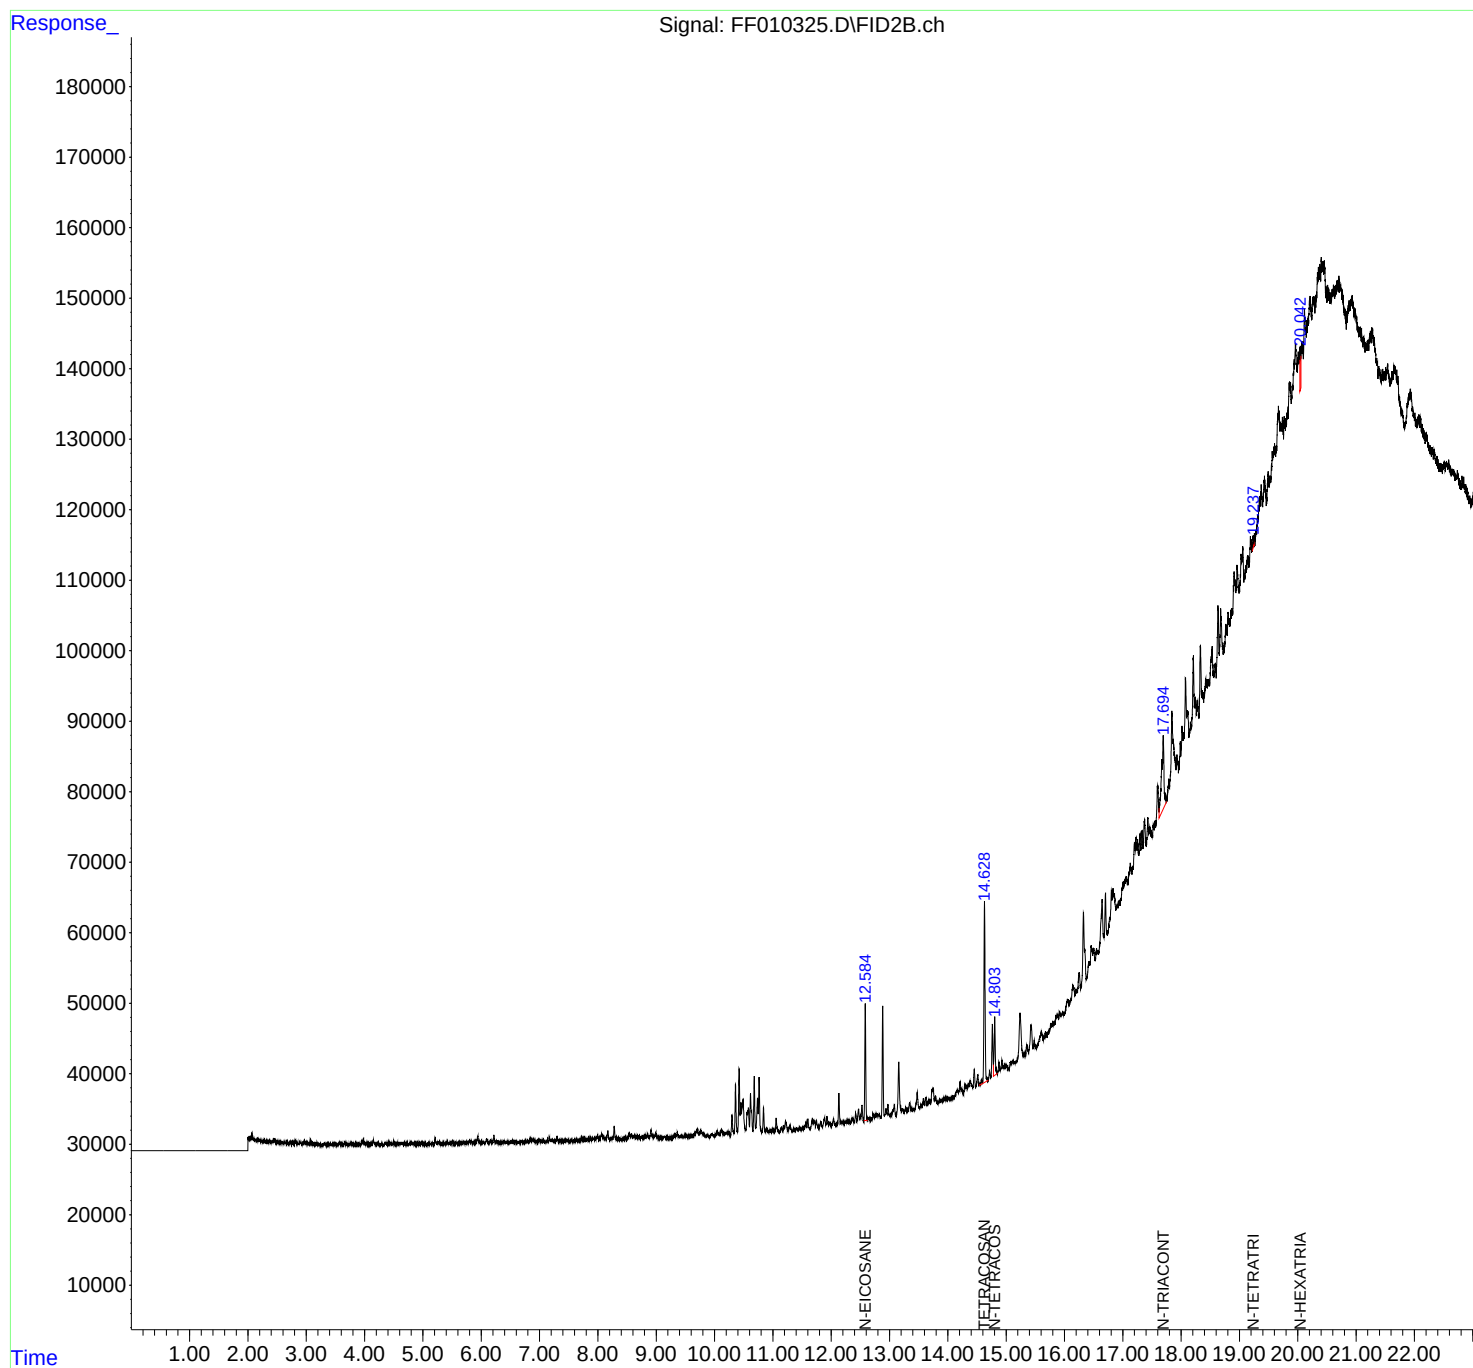


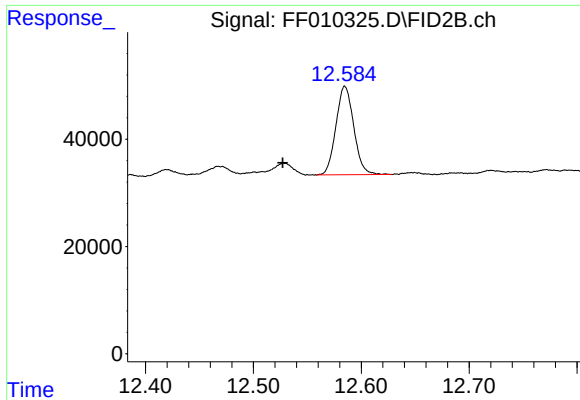

#7 N-EICOSANE


R.T.: 12.585 min
Delta R.T.: 0.058 min
Response: 189676
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :

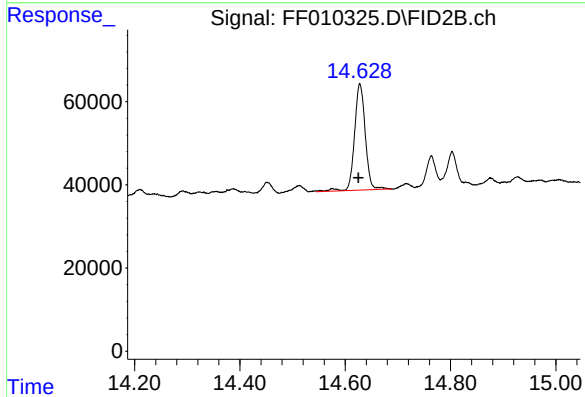


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.628 min
Delta R.T.: 0.003 min
Response: 361231
Conc: 3.02 ug/ml

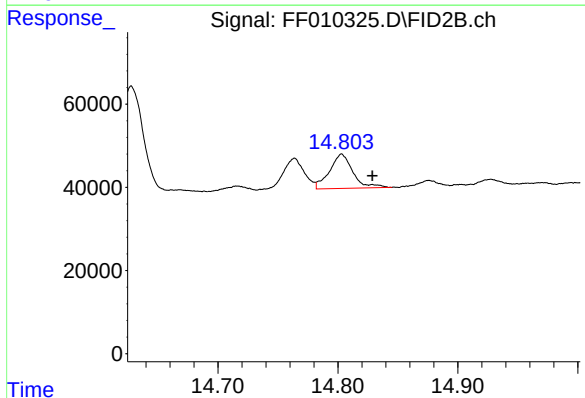


#10 N-TETRACOSANE

R.T.: 14.803 min
Delta R.T.: -0.026 min
Response: 110506
Conc: 0.83 ug/ml

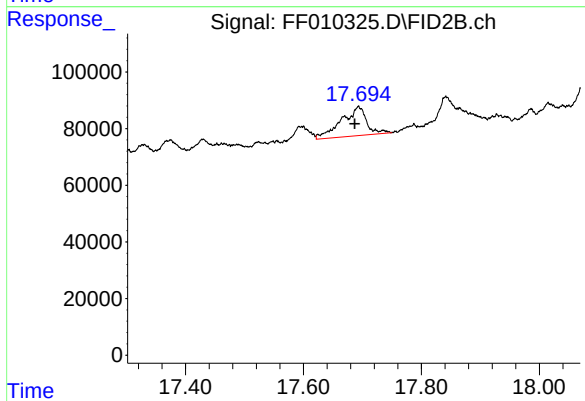

#13 N-TRIACONTANE


R.T.: 17.694 min
Delta R.T.: 0.007 min
Response: 303829
Conc: 2.30 ug/ml

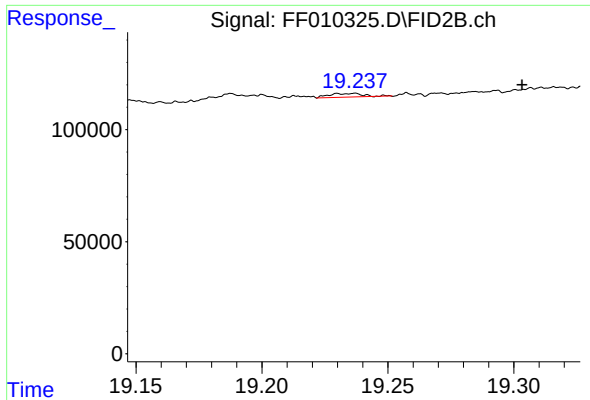

#15 N-TETRATRIACONTANE

R.T.: 19.235 min
Delta R.T.: -0.069 min
Response: 15164
Conc: 0.13 ug/ml

Instrument :
FID_F
ClientSampleId :

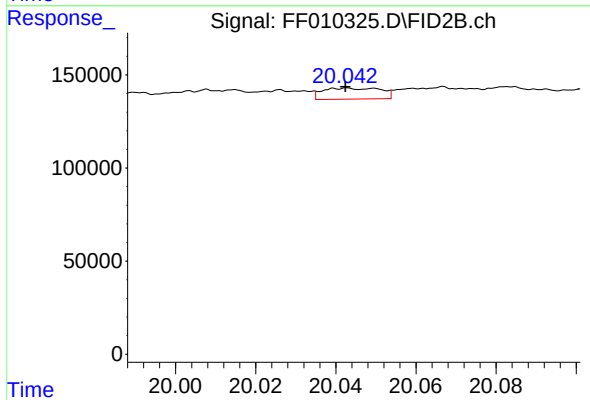

#16 N-HEXATRIACONTANE

R.T.: 20.044 min
Delta R.T.: 0.002 min
Response: 59596
Conc: 0.57 ug/ml