

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041123\
Data File : FF012442.D
Signal(s) : FID2B.ch
Acq On : 11 Apr 2023 07:46
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 02:22:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.870f	39875	0.300 ug/ml
8) N-DOCOSANE	14.103	94818	0.746 ug/ml
10) N-TETRACOSANE	15.190	512734	4.111 ug/ml
11) N-HEXACOSANE	16.231	53206	0.444 ug/ml
14) N-DOTRIACONTANE	18.910	137290	1.323 ug/ml
16) N-HEXATRIACONTANE	20.460	99188	1.132 ug/ml
17) N-OCTATRIACONTANE	21.152	65779	0.794 ug/ml
18) N-TETRACONTANE	22.058	308718	3.779 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041123\
Data File : FF012442.D
Signal(s) : FID2B.ch
Acq On : 11 Apr 2023 07:46
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 02:22:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

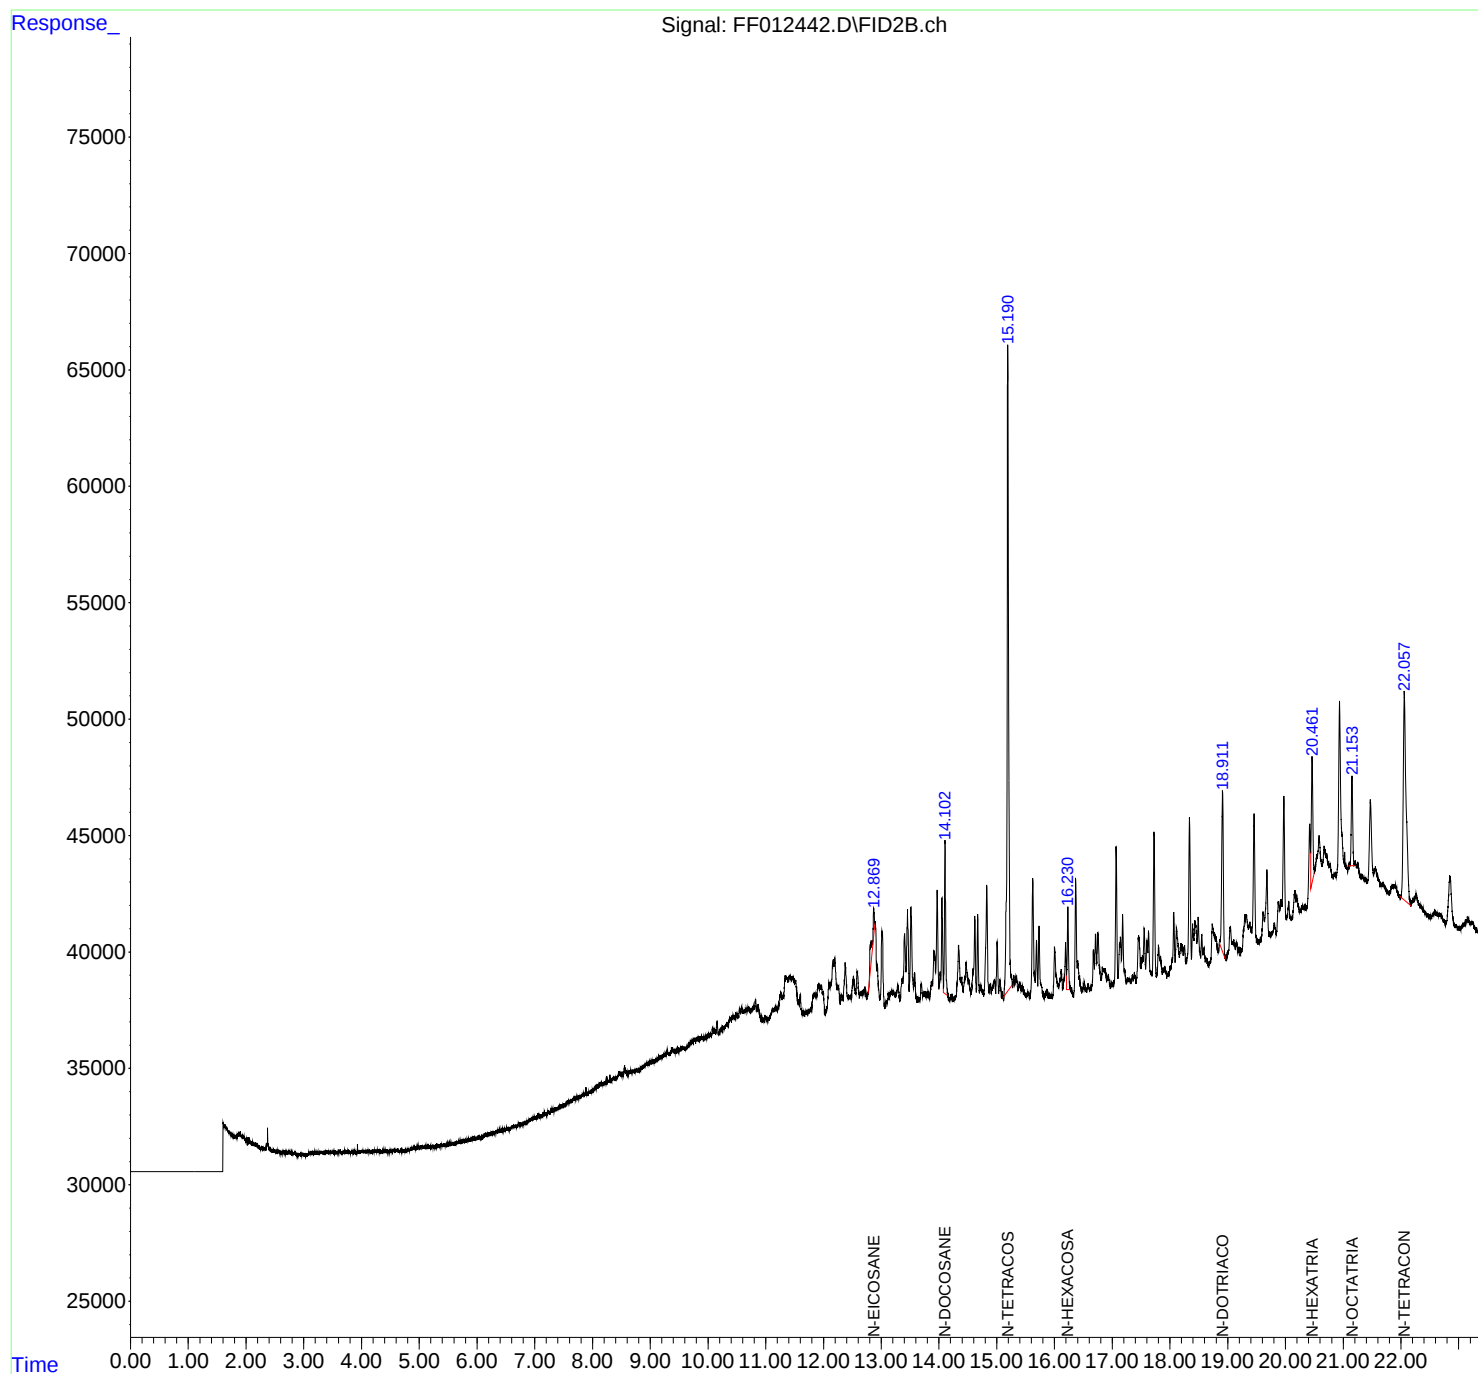


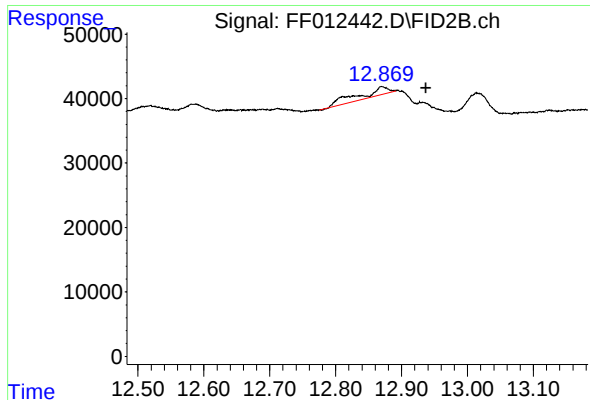

#7 N-EICOSANE


R.T.: 12.870 min
Delta R.T.: -0.067 min
Response: 39875
Conc: 0.30 ug/ml

Instrument :
FID_F
ClientSampleId :

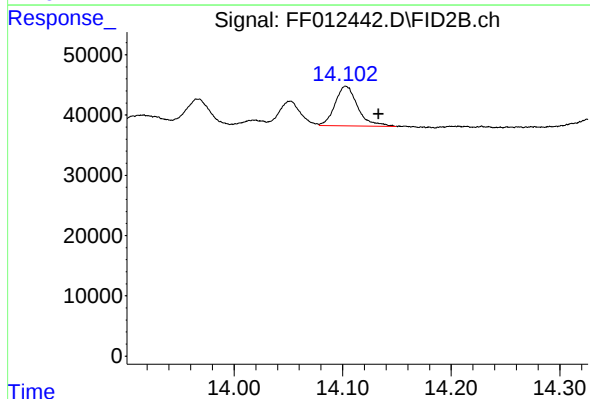


#8 N-DOCOSANE

R.T.: 14.103 min
Delta R.T.: -0.030 min
Response: 94818
Conc: 0.75 ug/ml

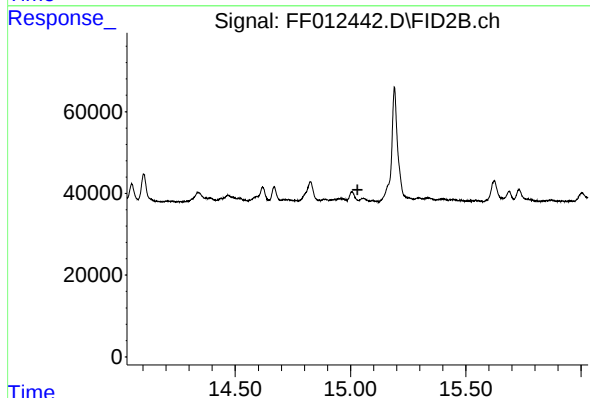


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.030 min
Response: 0
Conc: N.D.

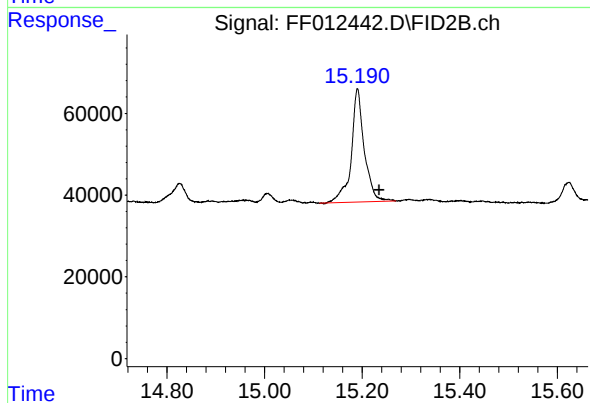

#10 N-TETRACOSANE


R.T.: 15.190 min
Delta R.T.: -0.045 min
Response: 512734
Conc: 4.11 ug/ml

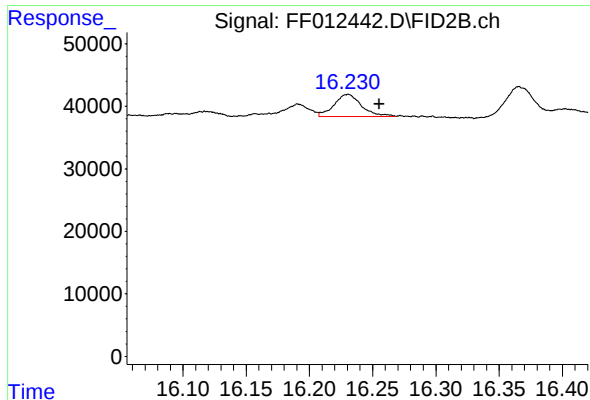

#11 N-HEXACOSANE


R.T.: 16.231 min
Delta R.T.: -0.025 min
Response: 53206
Conc: 0.44 ug/ml

Instrument :
FID_F
ClientSampleId :

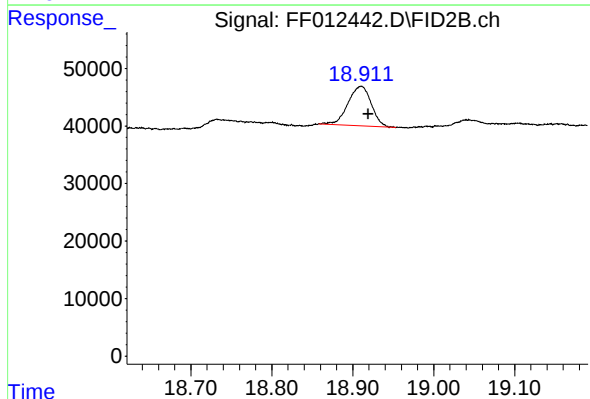


#14 N-DOTRIACONTANE

R.T.: 18.910 min
Delta R.T.: -0.009 min
Response: 137290
Conc: 1.32 ug/ml

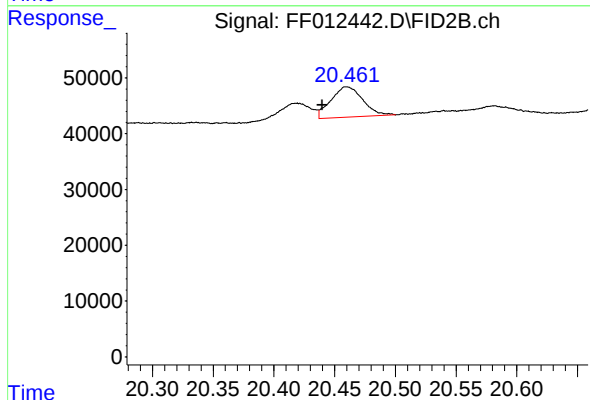


#16 N-HEXATRIACONTANE

R.T.: 20.460 min
Delta R.T.: 0.020 min
Response: 99188
Conc: 1.13 ug/ml

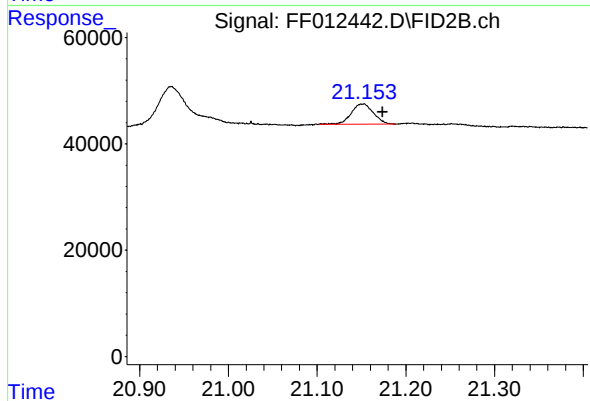

#17 N-OCTATRIACONTANE

R.T.: 21.152 min
Delta R.T.: -0.022 min
Response: 65779
Conc: 0.79 ug/ml

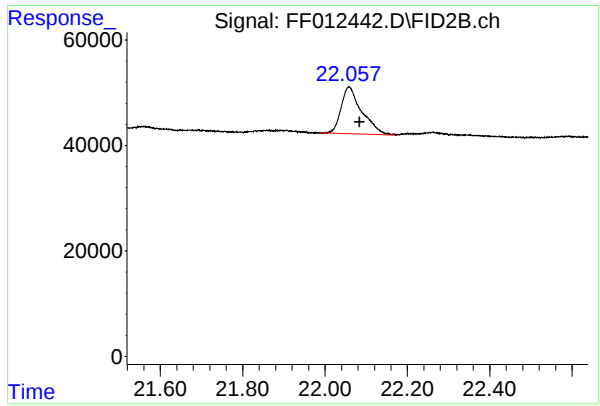

#18 N-TETRACONTANE

R.T.: 22.058 min
Delta R.T.: -0.026 min
Response: 308718
Conc: 3.78 ug/ml

Instrument :
FID_F
ClientSampleId :