

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041123\
 Data File : FF012445.D
 Signal(s) : FID2B.ch
 Acq On : 11 Apr 2023 09:15
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 12 02:23:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.739	1946979	15.705 ug/ml
12) N-OCTACOSANE	17.183	2119677	18.427 ug/ml
13) N-TRIACONTANE	18.071	144647	1.315 ug/ml
14) N-DOTRIACONTANE	18.902	209202	2.016 ug/ml
15) N-TETRATRIACONTANE	19.682	164804	1.742 ug/ml
16) N-HEXATRIACONTANE	20.430	108537	1.239 ug/ml
17) N-OCTATRIACONTANE	21.168	97180	1.174 ug/ml
18) N-TETRACONTANE	22.085	207718	2.543 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041123\
Data File : FF012445.D
Signal(s) : FID2B.ch
Acq On : 11 Apr 2023 09:15
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 02:23:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

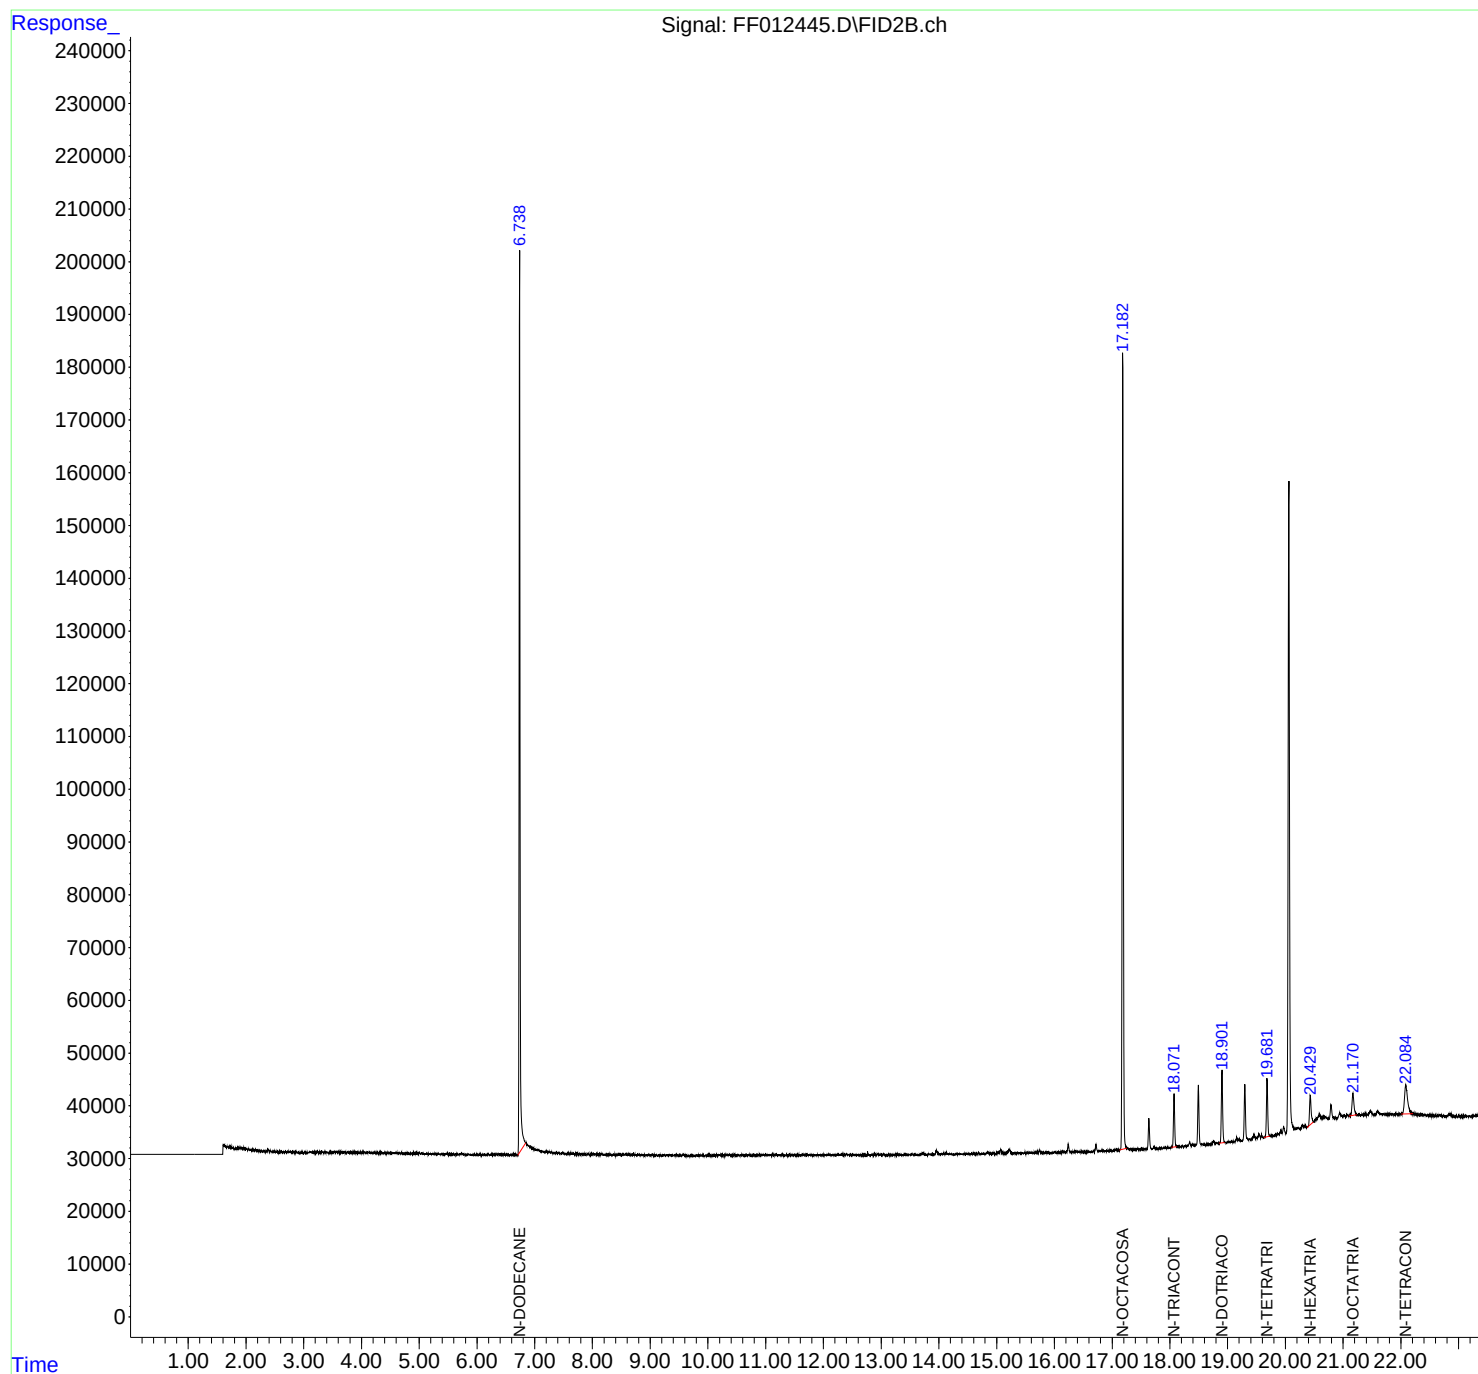


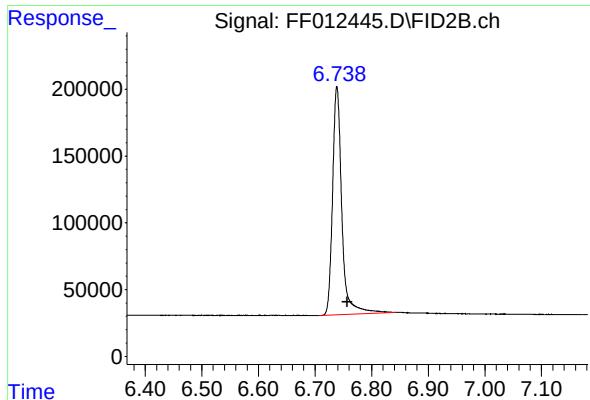

#3 N-DODECANE


R.T.: 6.739 min
Delta R.T.: -0.018 min
Response: 1946979
Conc: 15.71 ug/ml

Instrument :
FID_F
ClientSampleId :

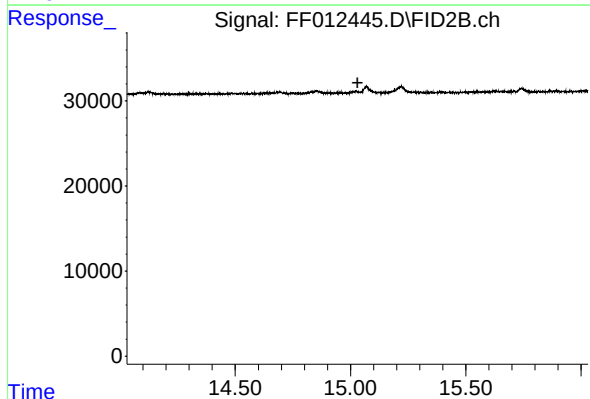


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.030 min
Response: 0
Conc: N.D.

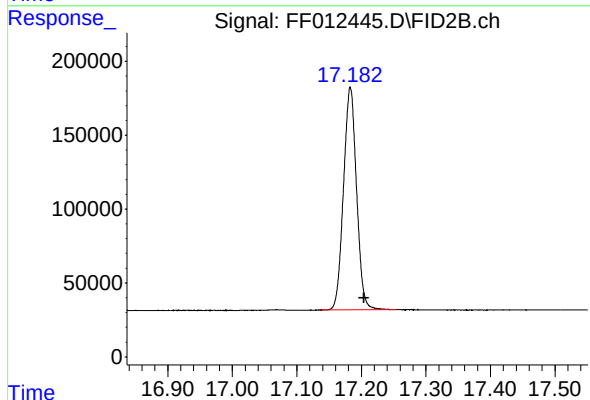


#12 N-OCTACOSANE

R.T.: 17.183 min
Delta R.T.: -0.021 min
Response: 2119677
Conc: 18.43 ug/ml

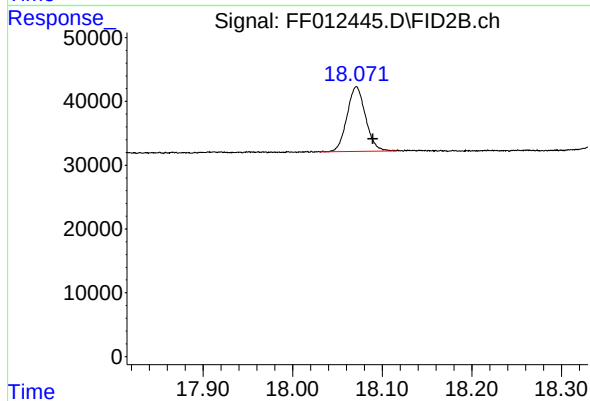

#13 N-TRIACONTANE


R.T.: 18.071 min
Delta R.T.: -0.018 min
Response: 144647
Conc: 1.31 ug/ml

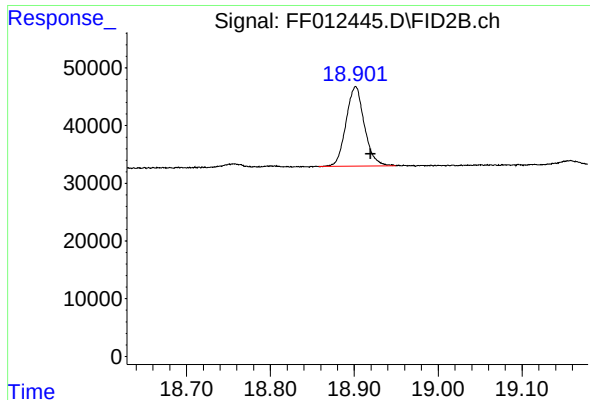

#14 N-DOTRIACONTANE


R.T.: 18.902 min
Delta R.T.: -0.018 min
Response: 209202
Conc: 2.02 ug/ml

Instrument :
FID_F
ClientSampleId :

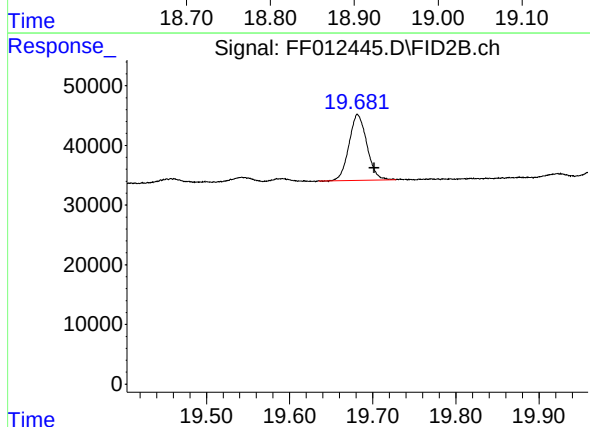


#15 N-TETRATRIACONTANE

R.T.: 19.682 min
Delta R.T.: -0.020 min
Response: 164804
Conc: 1.74 ug/ml

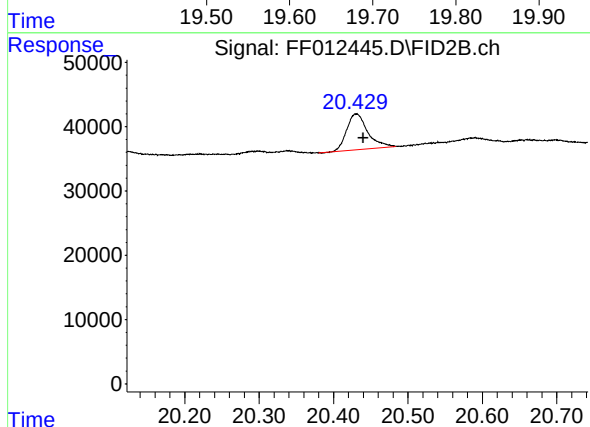


#16 N-HEXATRIACONTANE

R.T.: 20.430 min
Delta R.T.: -0.009 min
Response: 108537
Conc: 1.24 ug/ml

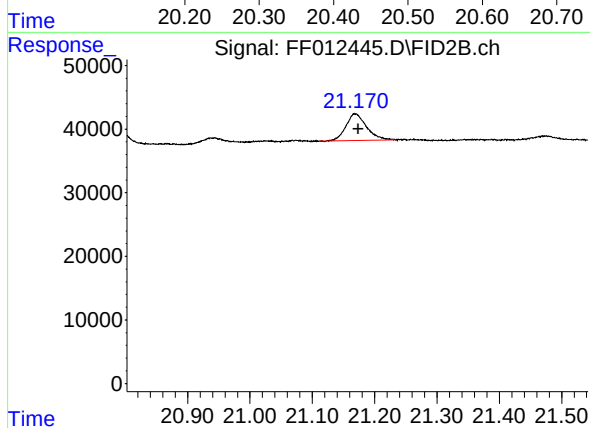

#17 N-OCTATRIACONTANE

R.T.: 21.168 min
Delta R.T.: -0.006 min
Response: 97180
Conc: 1.17 ug/ml

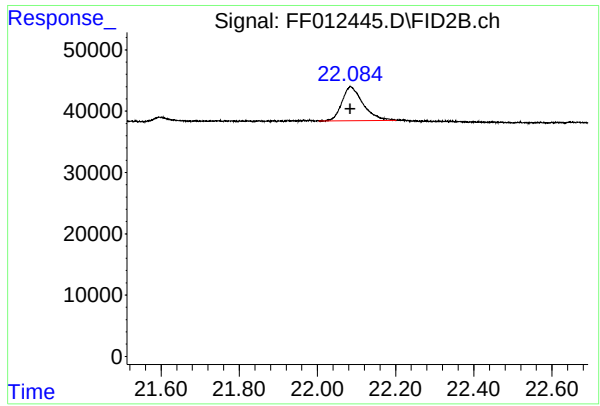

#18 N-TETRACONTANE

R.T.: 22.085 min
Delta R.T.: 0.000 min
Response: 207718
Conc: 2.54 ug/ml

Instrument :
FID_F
ClientSampleId :