

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041123\
 Data File : FF012449.D
 Signal(s) : FID2B.ch
 Acq On : 11 Apr 2023 11:26
 Operator : YP\AJ
 Sample : PB151937BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 12 02:23:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.016	1938222	17.319 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.919	64968	0.626 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041123\
Data File : FF012449.D
Signal(s) : FID2B.ch
Acq On : 11 Apr 2023 11:26
Operator : YP\AJ
Sample : PB151937BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 02:23:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

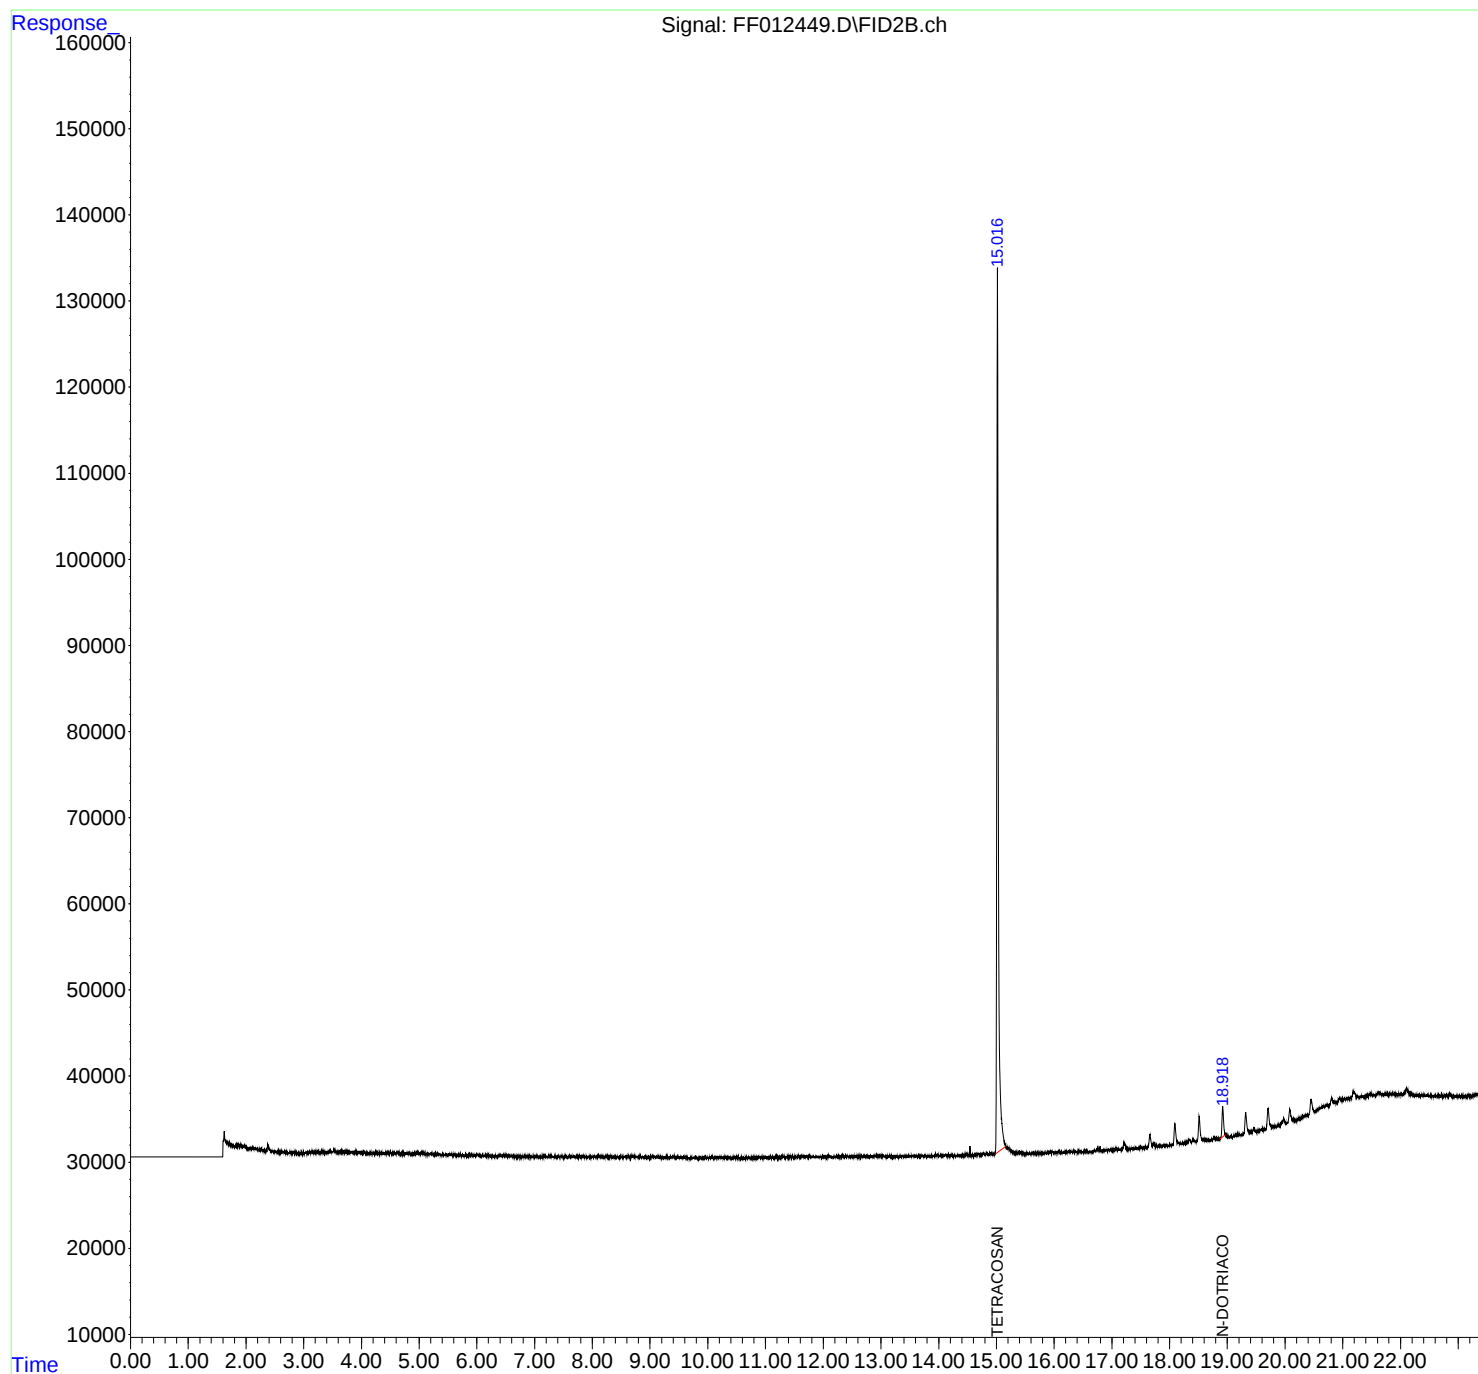


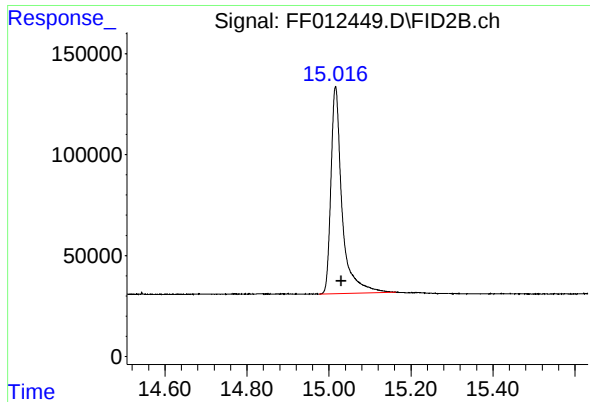

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.016 min
Delta R.T.: -0.014 min
Response: 1938222
Conc: 17.32 ug/ml

Instrument :
FID_F
ClientSampleId :

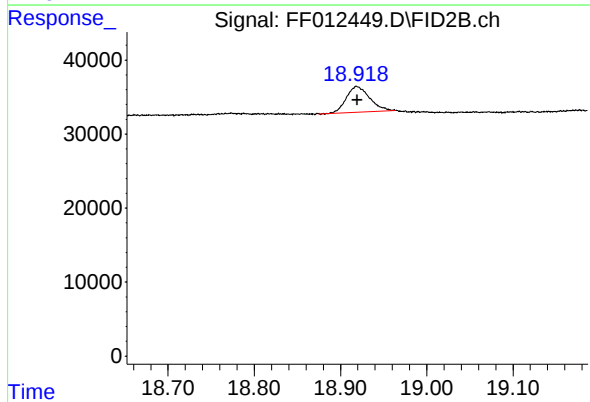

#14 N-DOTRIACONTANE

R.T.: 18.919 min
Delta R.T.: 0.000 min
Response: 64968
Conc: 0.63 ug/ml