

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041123\
 Data File : FF012460.D
 Signal(s) : FID2B.ch
 Acq On : 11 Apr 2023 17:54
 Operator : YP\AJ
 Sample : 02262-07 5X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 12 02:25:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.015	233470	2.086 ug/ml
Target Compounds			
7) N-EICOSANE	12.936	55689	0.419 ug/ml
8) N-DOCOSANE	14.121	73608	0.579 ug/ml
10) N-TETRACOSANE	15.213	1009449	8.094 ug/ml
11) N-HEXACOSANE	16.237	74160	0.619 ug/ml
12) N-OCTACOSANE	17.215	381990	3.321 ug/ml
13) N-TRIACONTANE	18.076	124462	1.131 ug/ml
14) N-DOTRIACONTANE	18.878	365887	3.525 ug/ml
15) N-TETRATRIACONTANE	19.687	67499	0.713 ug/ml
16) N-HEXATRIACONTANE	20.424	113150	1.292 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041123\
Data File : FF012460.D
Signal(s) : FID2B.ch
Acq On : 11 Apr 2023 17:54
Operator : YP\AJ
Sample : 02262-07 5X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 02:25:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

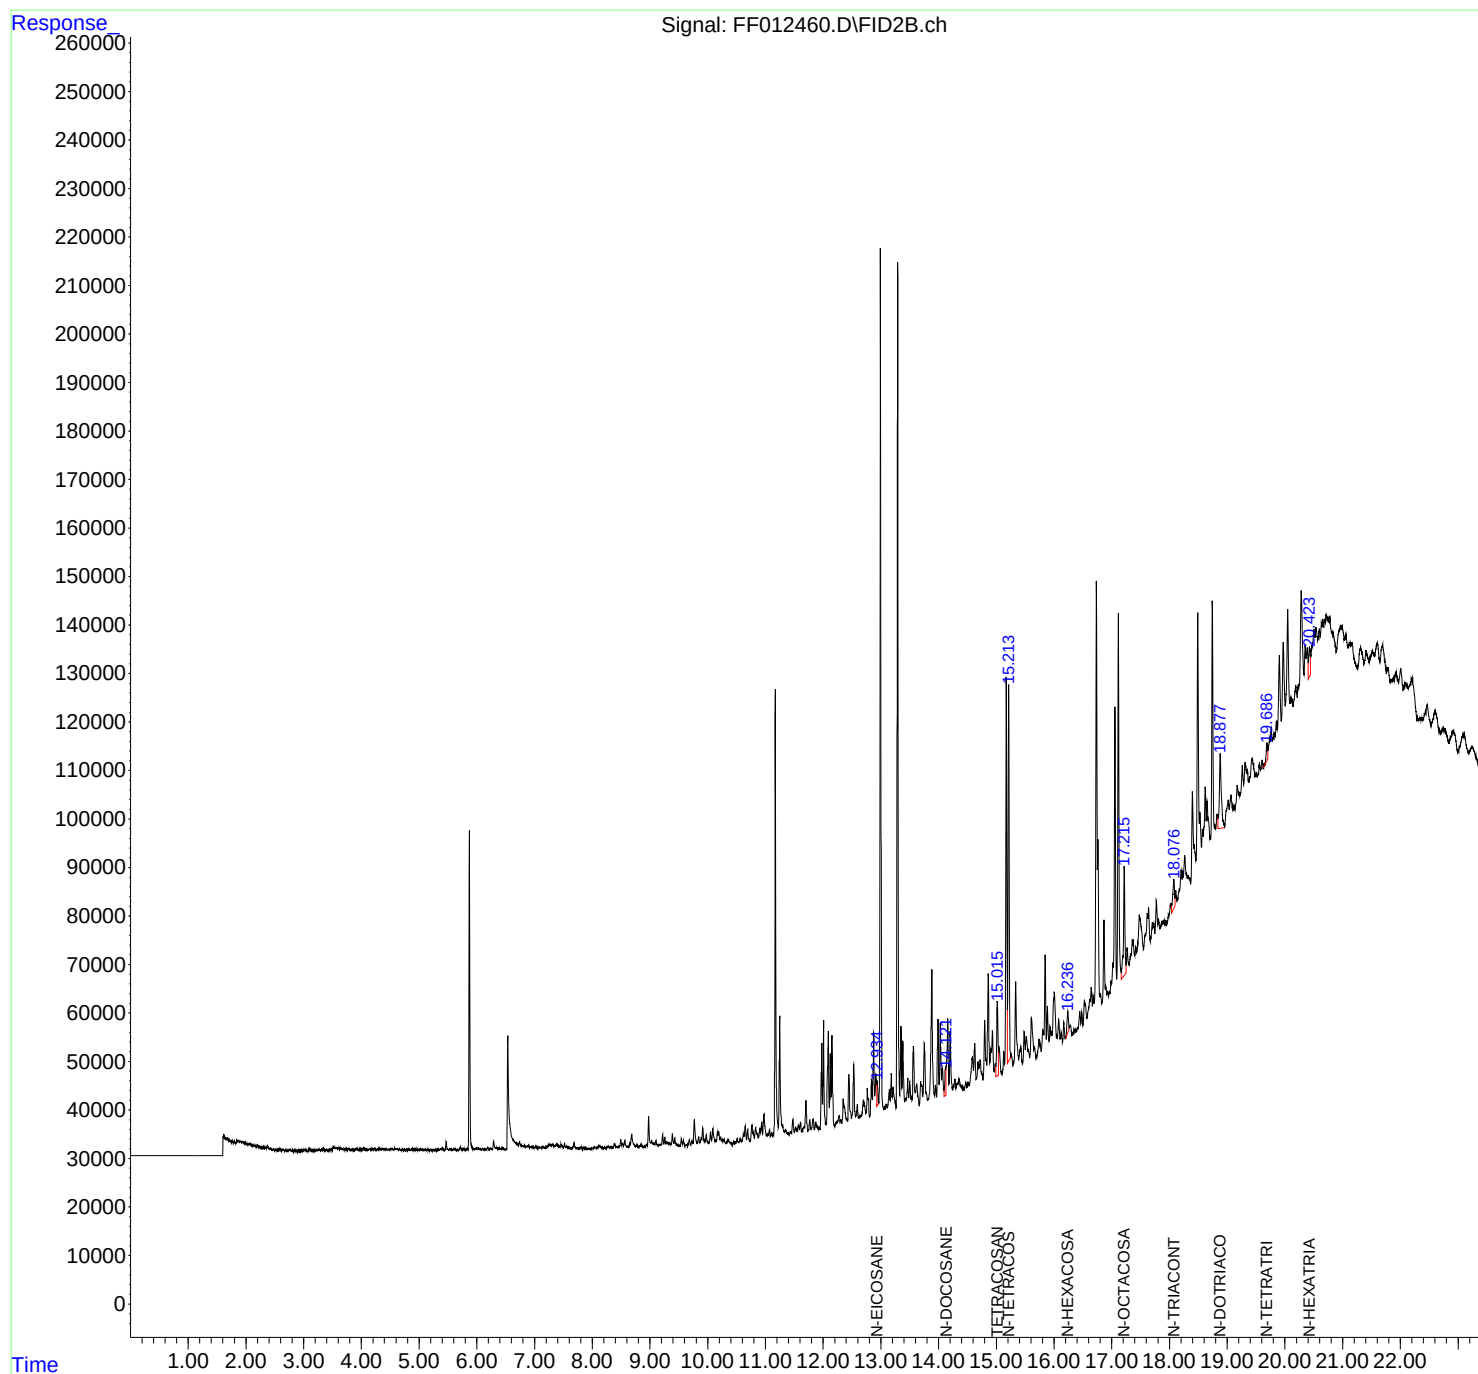


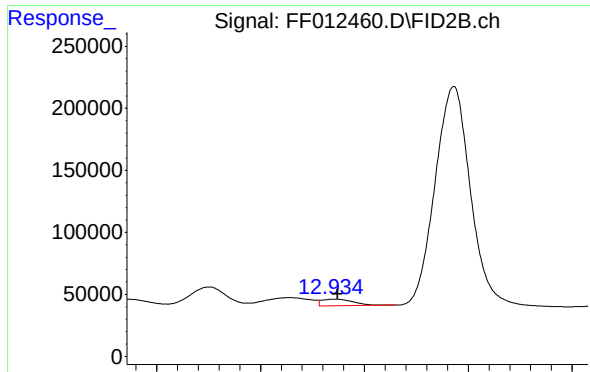

#7 N-EICOSANE


R.T.: 12.936 min
Delta R.T.: -0.001 min
Response: 55689
Conc: 0.42 ug/ml

Instrument :
FID_F
ClientSampleId :

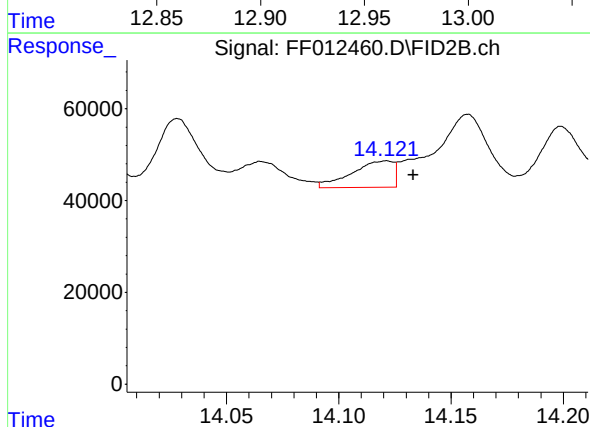


#8 N-DOCOSANE

R.T.: 14.121 min
Delta R.T.: -0.012 min
Response: 73608
Conc: 0.58 ug/ml

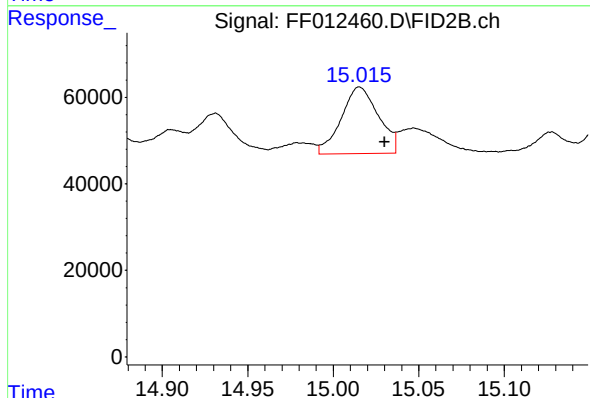


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.015 min
Delta R.T.: -0.015 min
Response: 233470
Conc: 2.09 ug/ml

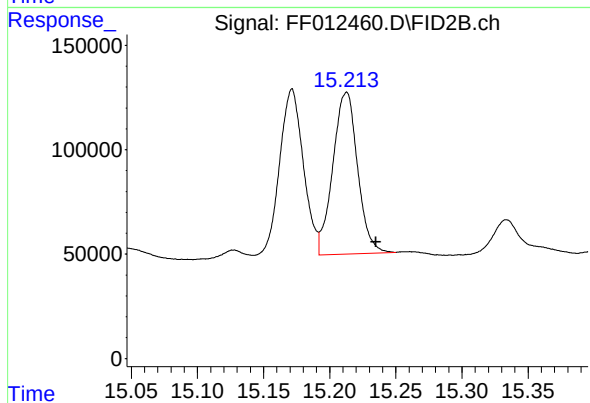

#10 N-TETRACOSANE


R.T.: 15.213 min
Delta R.T.: -0.023 min
Response: 1009449
Conc: 8.09 ug/ml

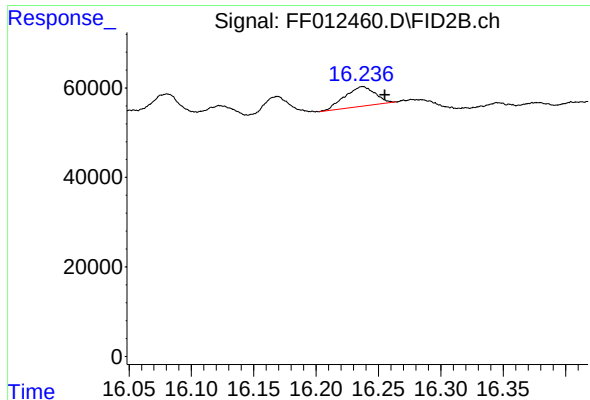

#11 N-HEXACOSANE


R.T.: 16.237 min
Delta R.T.: -0.018 min
Response: 74160
Conc: 0.62 ug/ml

Instrument :
FID_F
ClientSampleId :

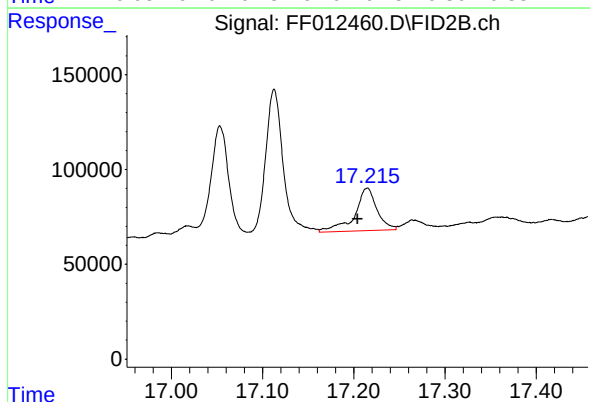


#12 N-OCTACOSANE

R.T.: 17.215 min
Delta R.T.: 0.011 min
Response: 381990
Conc: 3.32 ug/ml

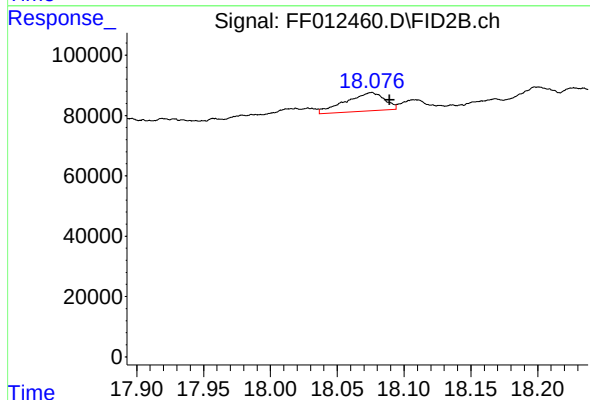


#13 N-TRIACONTANE

R.T.: 18.076 min
Delta R.T.: -0.014 min
Response: 124462
Conc: 1.13 ug/ml

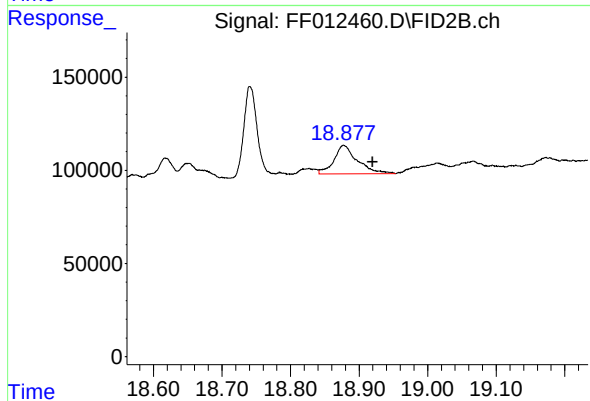

#14 N-DOTRIACONTANE


R.T.: 18.878 min
Delta R.T.: -0.042 min
Response: 365887
Conc: 3.53 ug/ml

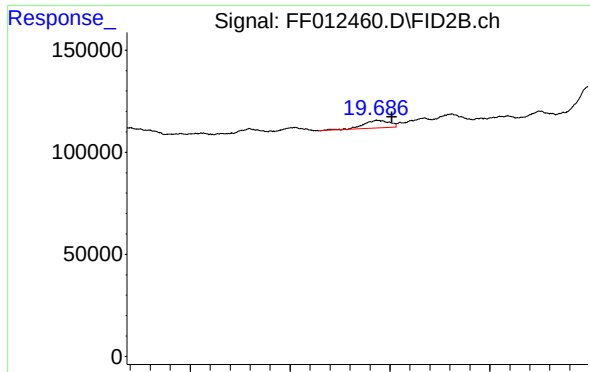

#15 N-TETRATRIACONTANE

R.T.: 19.687 min
Delta R.T.: -0.015 min
Response: 67499
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :

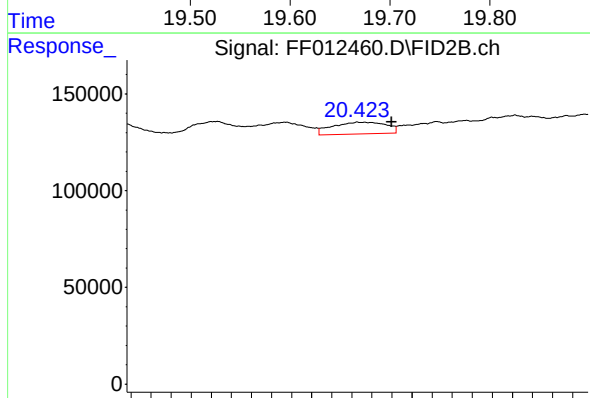

#16 N-HEXATRIACONTANE

R.T.: 20.424 min
Delta R.T.: -0.016 min
Response: 113150
Conc: 1.29 ug/ml