

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041123\
 Data File : FF012462.D
 Signal(s) : FID2B.ch
 Acq On : 11 Apr 2023 18:54
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 12 02:25:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.015	1873328	16.739 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.072	51553	0.469 ug/ml
14) N-DOTRIACONTANE	18.905	77966	0.751 ug/ml
15) N-TETRATRIACONTANE	19.687	74465	0.787 ug/ml
16) N-HEXATRIACONTANE	20.430	32202	0.368 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041123\
Data File : FF012462.D
Signal(s) : FID2B.ch
Acq On : 11 Apr 2023 18:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 12 02:25:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

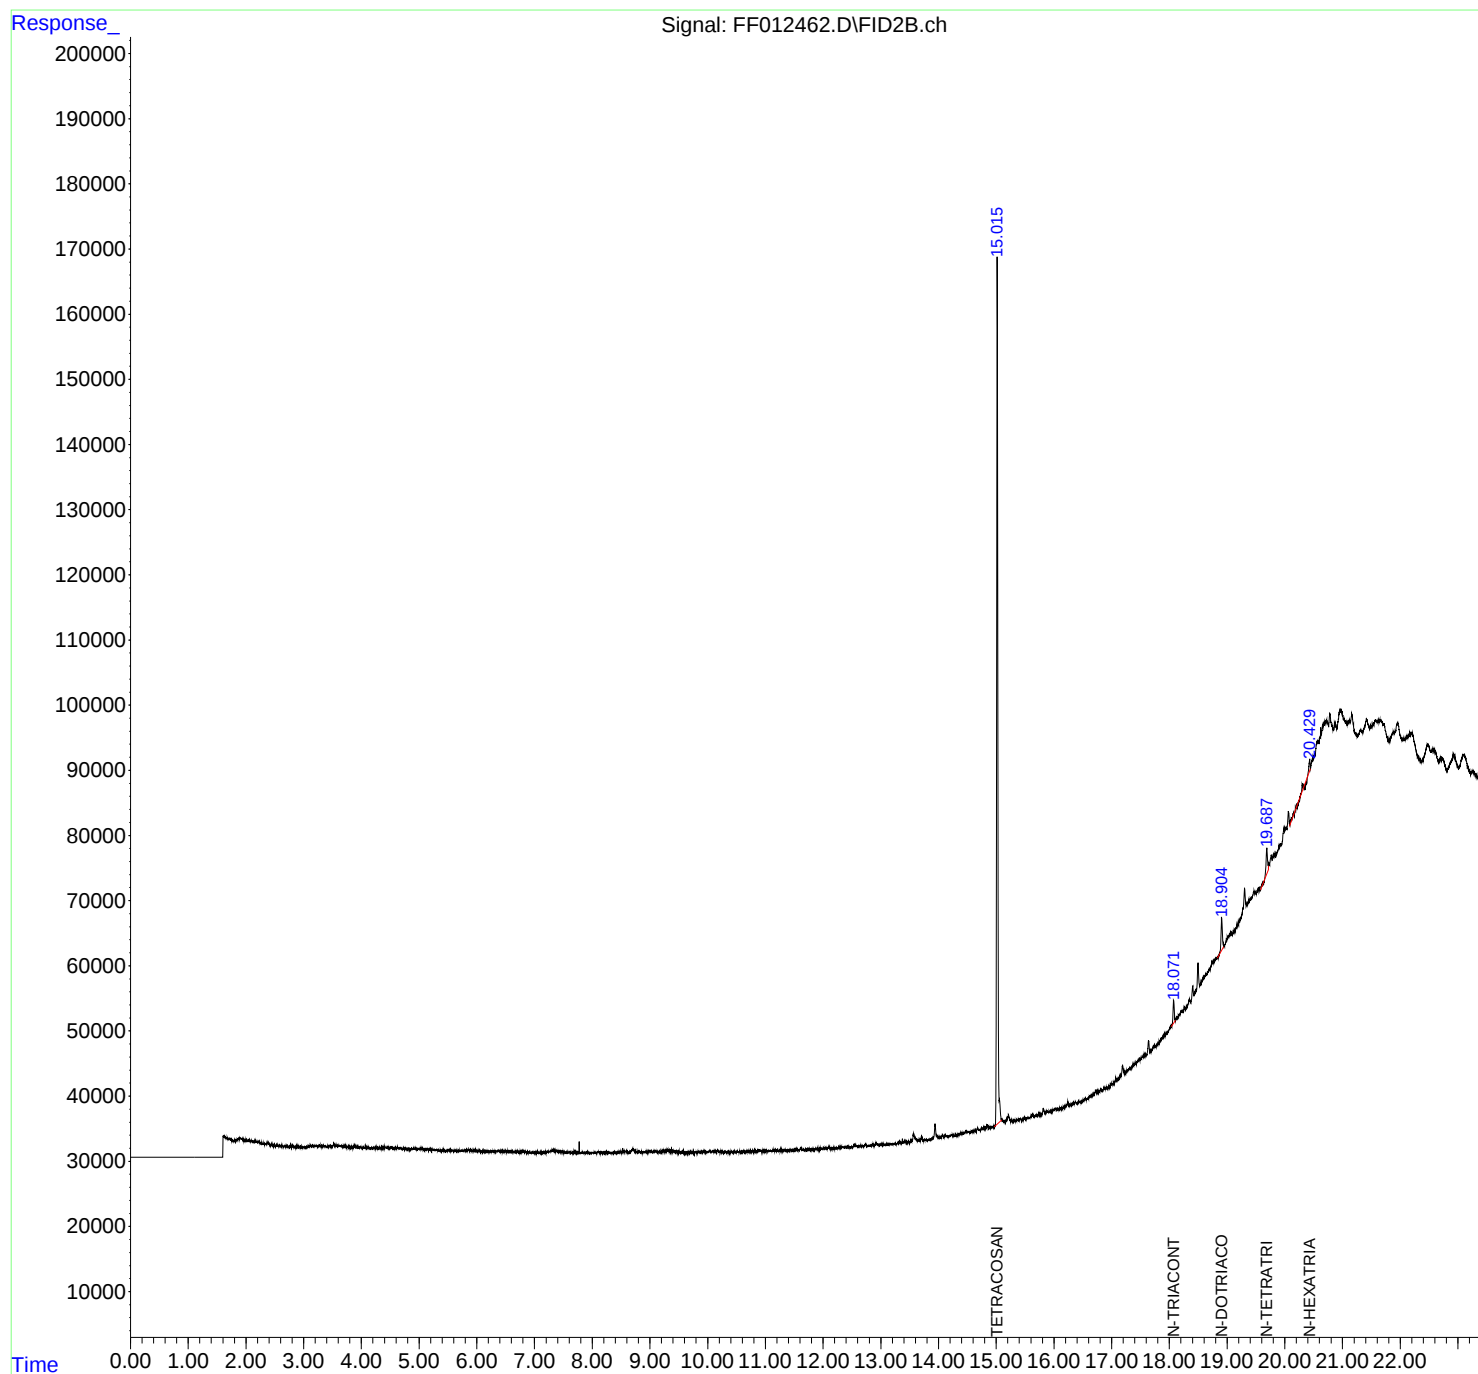


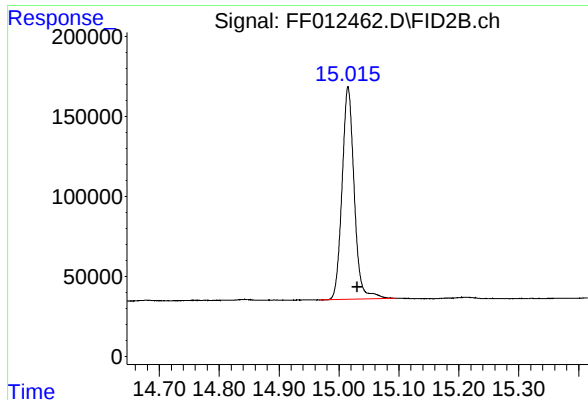

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.015 min
Delta R.T.: -0.015 min
Response: 1873328
Conc: 16.74 ug/ml

Instrument :
FID_F
ClientSampleId :

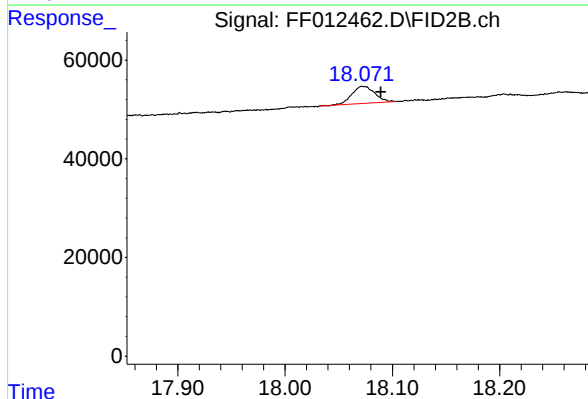


#13 N-TRIACONTANE

R.T.: 18.072 min
Delta R.T.: -0.017 min
Response: 51553
Conc: 0.47 ug/ml

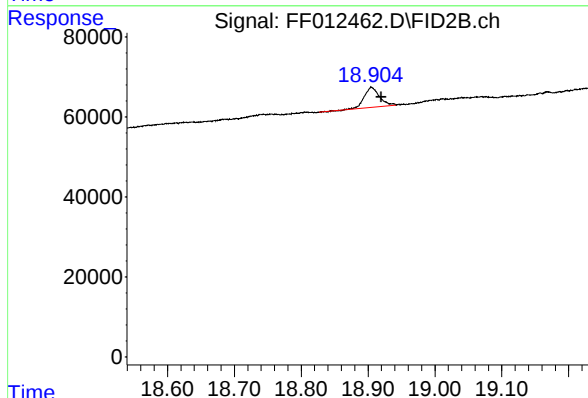


#14 N-DOTRIACONTANE

R.T.: 18.905 min
Delta R.T.: -0.014 min
Response: 77966
Conc: 0.75 ug/ml

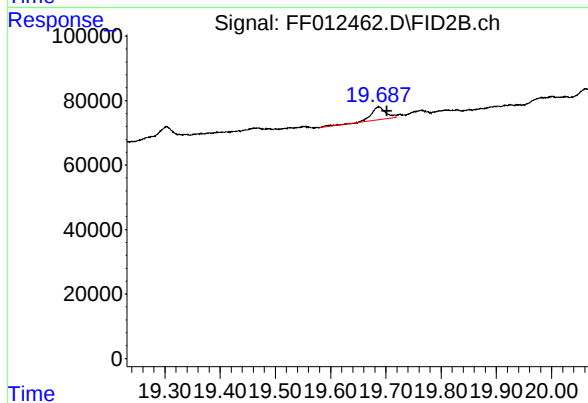

#15 N-TETRATRIACONTANE

R.T.: 19.687 min
Delta R.T.: -0.015 min
Response: 74465
Conc: 0.79 ug/ml

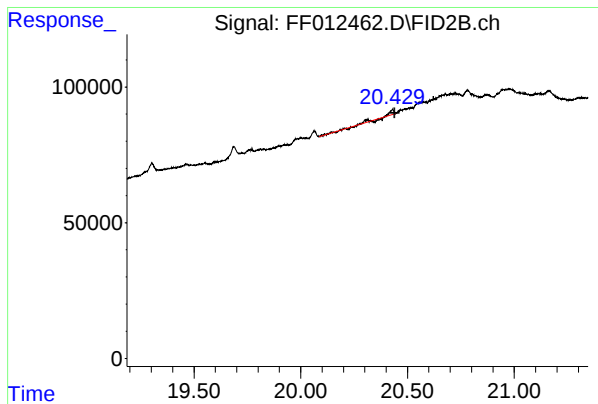

#16 N-HEXATRIACONTANE

R.T.: 20.430 min
Delta R.T.: -0.010 min
Response: 32202
Conc: 0.37 ug/ml

Instrument :
FID_F
ClientSampleId :