

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041323\
 Data File : FF012475.D
 Signal(s) : FID2B.ch
 Acq On : 13 Apr 2023 17:19
 Operator : YP\AJ
 Sample : PB152101BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB152101BL

Integration File: autoint1.e
 Quant Time: Apr 14 02:38:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.009	2304362	19.170 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.913	58184	0.461 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041323\
Data File : FF012475.D
Signal(s) : FID2B.ch
Acq On : 13 Apr 2023 17:19
Operator : YP\AJ
Sample : PB152101BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB152101BL

Integration File: autoint1.e
Quant Time: Apr 14 02:38:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

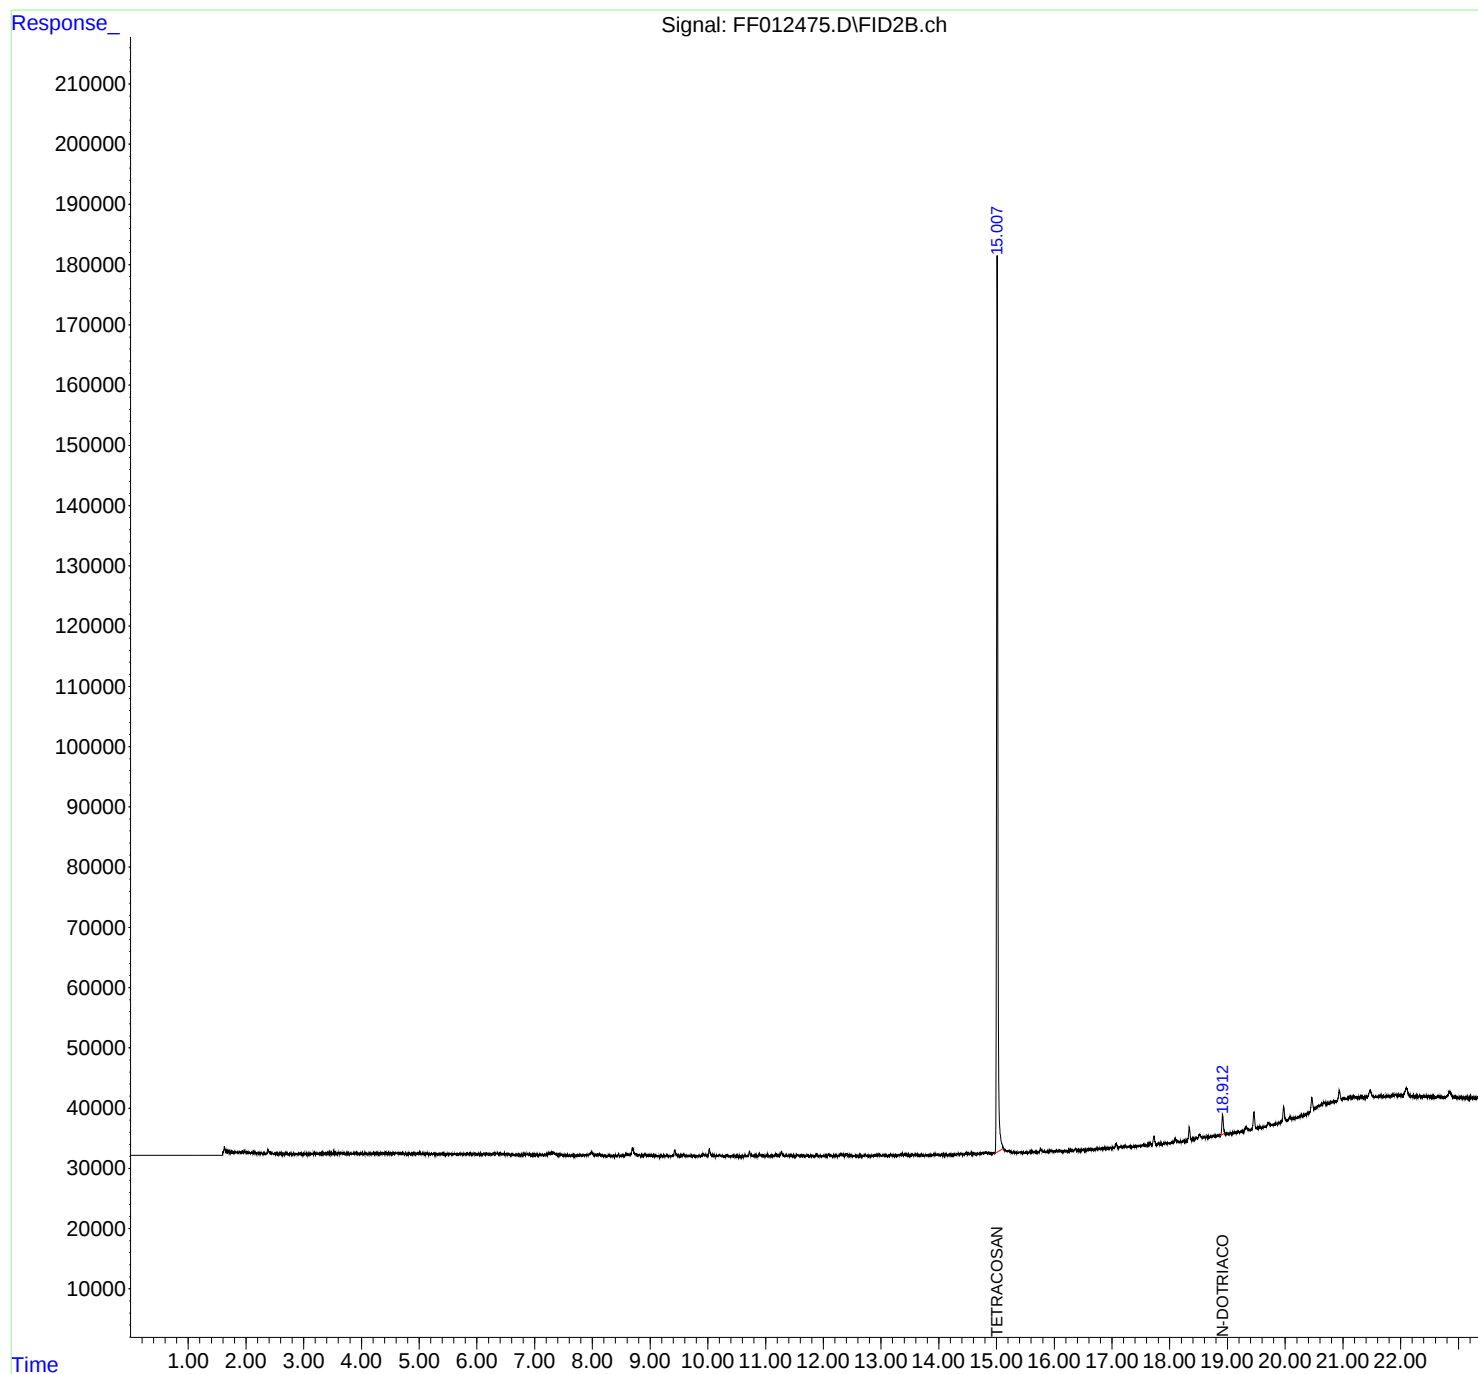


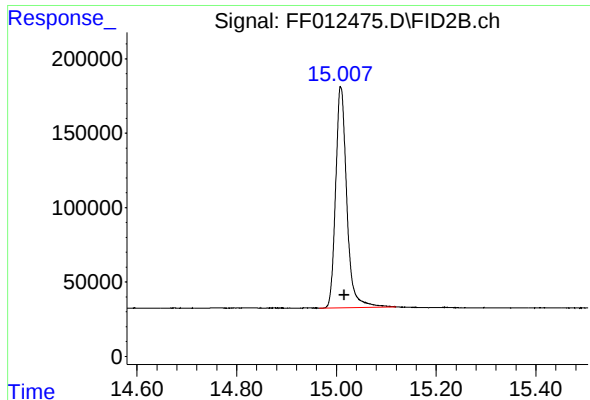

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.009 min
Delta R.T.: -0.007 min
Response: 2304362
Conc: 19.17 ug/ml

Instrument :
FID_F
ClientSampleId :
PB152101BL

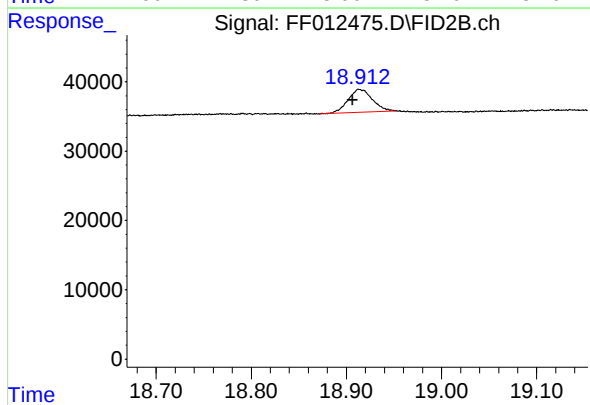

#14 N-DOTRIACONTANE

R.T.: 18.913 min
Delta R.T.: 0.007 min
Response: 58184
Conc: 0.46 ug/ml