

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041323\
Data File : FF012479.D
Signal(s) : FID2B.ch
Acq On : 13 Apr 2023 19:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Apr 14 02:39:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.010	2046388	17.024 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.915	59391	0.471 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041323\
Data File : FF012479.D
Signal(s) : FID2B.ch
Acq On : 13 Apr 2023 19:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Apr 14 02:39:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

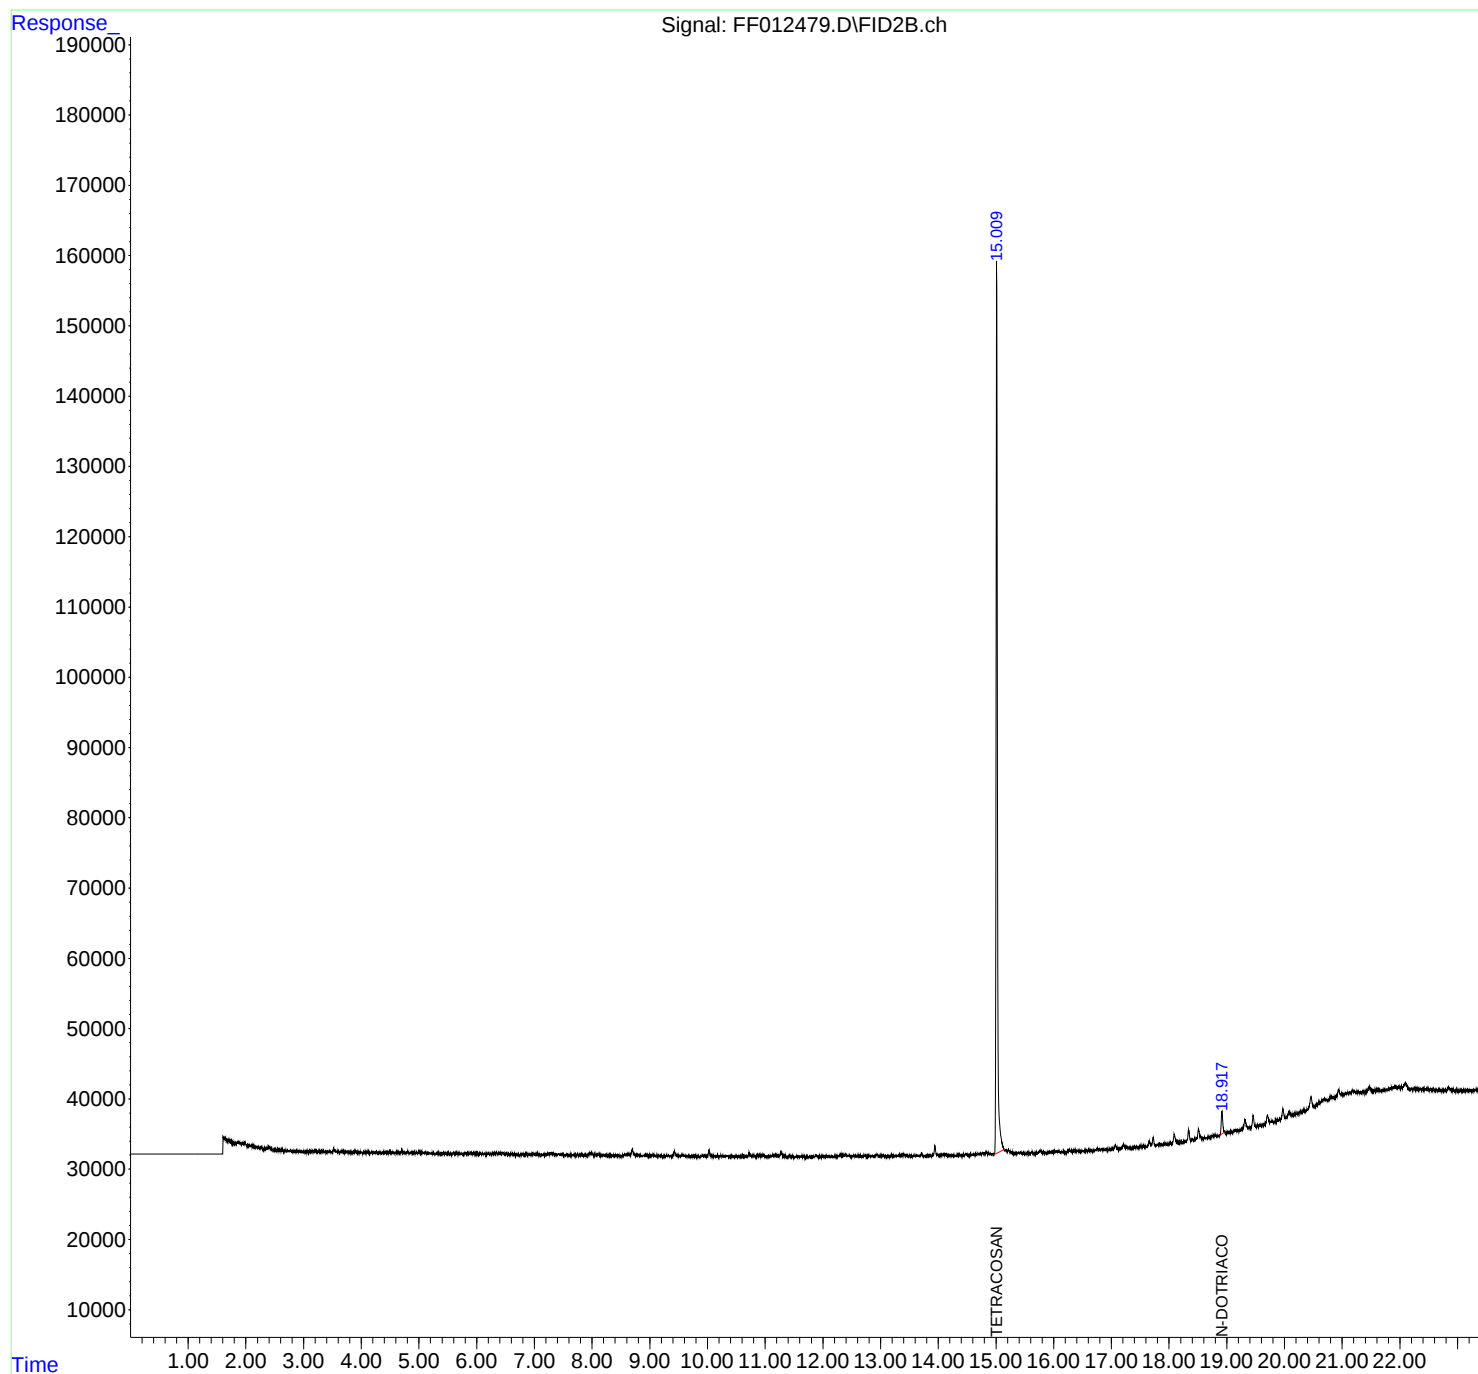


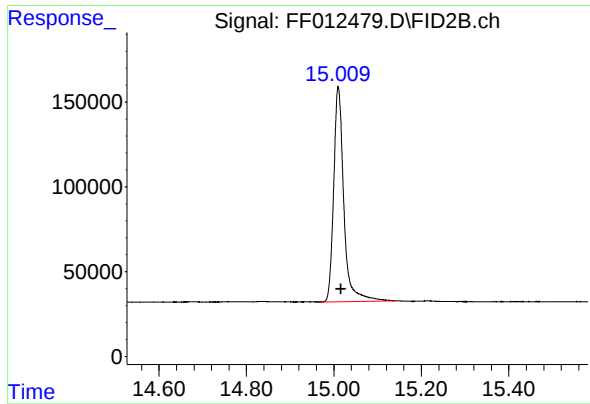

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.010 min
Delta R.T.: -0.006 min
Response: 2046388
Conc: 17.02 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

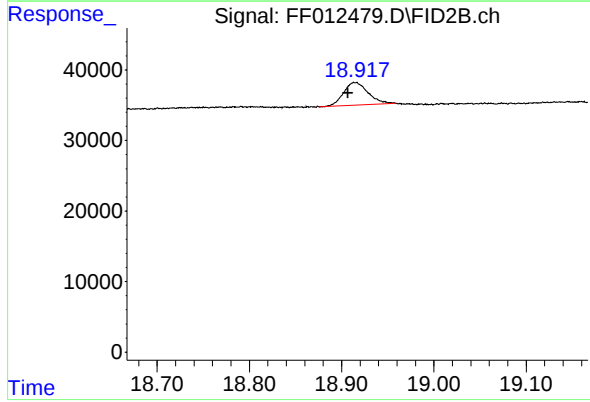

#14 N-DOTRIACONTANE

R.T.: 18.915 min
Delta R.T.: 0.008 min
Response: 59391
Conc: 0.47 ug/ml