

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041522\
 Data File : FF010361.D
 Signal(s) : FID2B.ch
 Acq On : 15 Apr 2022 17:39
 Operator : AJ\MA
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 15 21:25:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
 Quant Title :
 QLast Update : Fri Apr 01 11:58:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.617	5230595	43.760 ug/mlm
Target Compounds			
2) N-DECANE	4.358	6152454	46.277 ug/ml
3) N-DODECANE	6.376	6088486	45.727 ug/ml
4) N-TETRADECANE	8.171	6057567	45.688 ug/ml
5) N-HEXADECANE	9.771	6057198	45.625 ug/ml
6) N-OCTADECANE	11.211	6191056	45.029 ug/ml
7) N-EICOSANE	12.521	5987838	44.568 ug/ml
8) N-DOCOSANE	13.719	5919051	44.238 ug/ml
10) N-TETRACOSANE	14.822	5880589	43.915 ug/ml
11) N-HEXACOSANE	15.842	5799276	43.722 ug/mlm
12) N-OCTACOSANE	16.792	5721792	43.170 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041522\
Data File : FF010361.D
Signal(s) : FID2B.ch
Acq On : 15 Apr 2022 17:39
Operator : AJ\MA
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 15 21:25:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040122.M
Quant Title :
QLast Update : Fri Apr 01 11:58:56 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

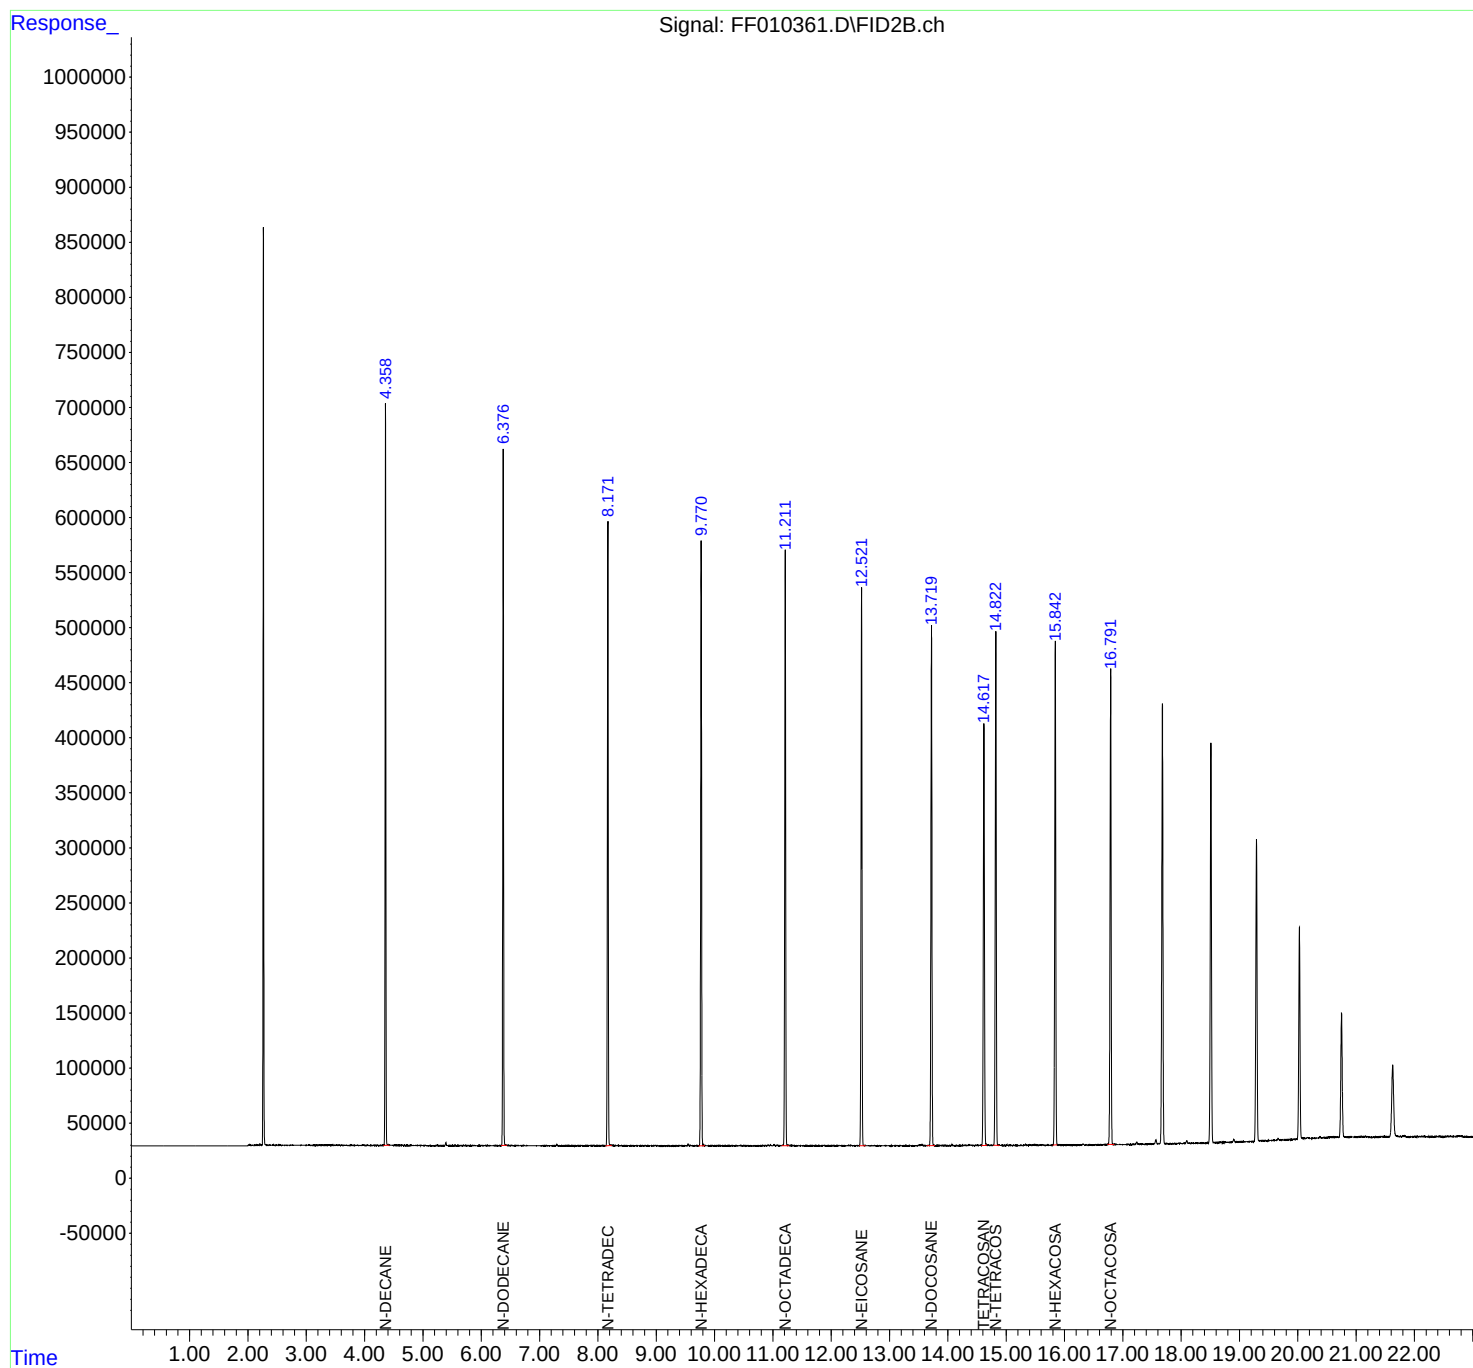

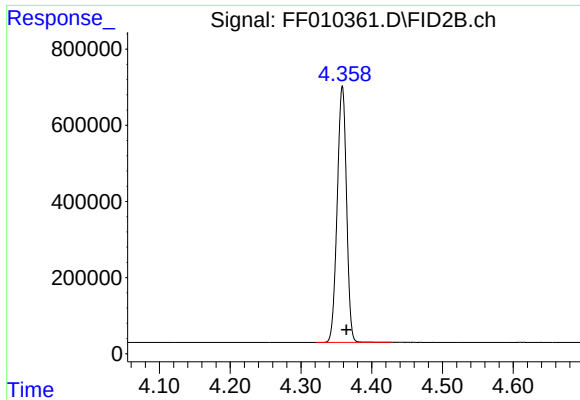


#2 N-DECANE

R.T.: 4.358 min
Delta R.T.: -0.006 min
Response: 6152454
Conc: 46.28 ug/ml

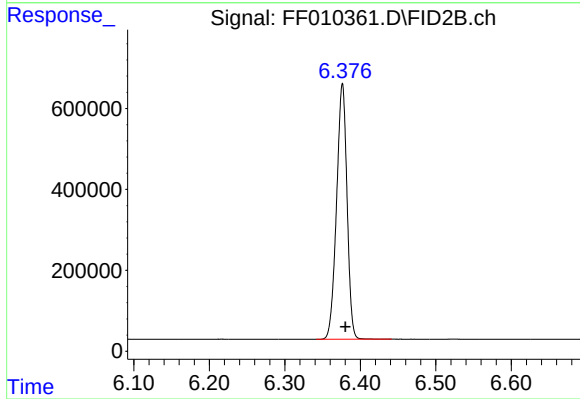


#3 N-DODECANE

R.T.: 6.376 min
Delta R.T.: -0.004 min
Response: 6088486
Conc: 45.73 ug/ml

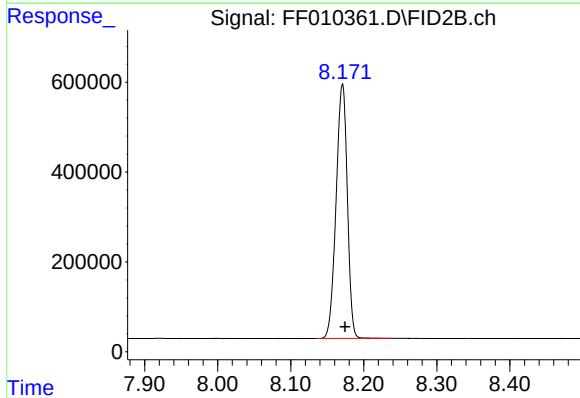


#4 N-TETRADECANE

R.T.: 8.171 min
Delta R.T.: -0.004 min
Response: 6057567
Conc: 45.69 ug/ml

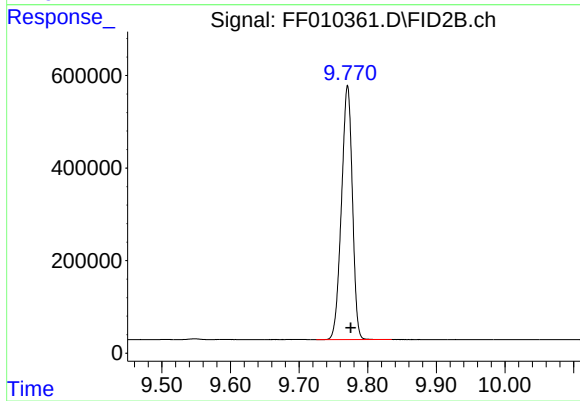


#5 N-HEXADECANE

R.T.: 9.771 min
Delta R.T.: -0.005 min
Response: 6057198
Conc: 45.63 ug/ml

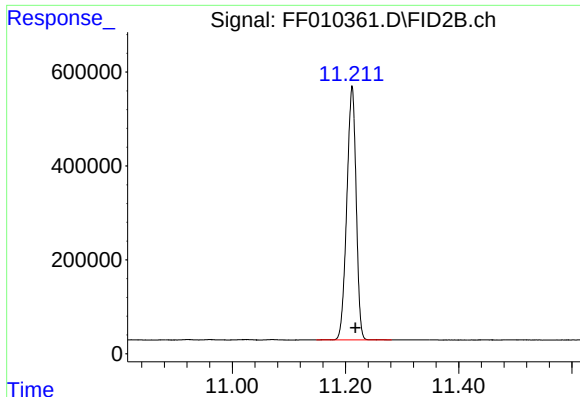


#6 N-OCTADECANE

R.T.: 11.211 min
Delta R.T.: -0.006 min
Response: 6191056
Conc: 45.03 ug/ml

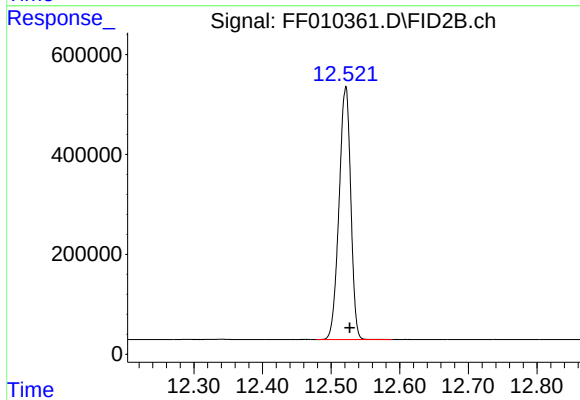


#7 N-EICOSANE

R.T.: 12.521 min
Delta R.T.: -0.006 min
Response: 5987838
Conc: 44.57 ug/ml

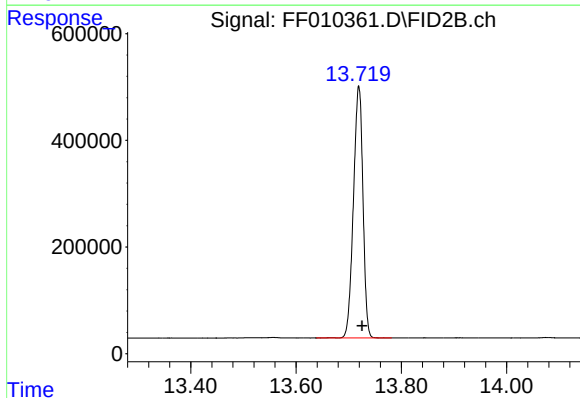


#8 N-DOCOSANE

R.T.: 13.719 min
Delta R.T.: -0.007 min
Response: 5919051
Conc: 44.24 ug/ml

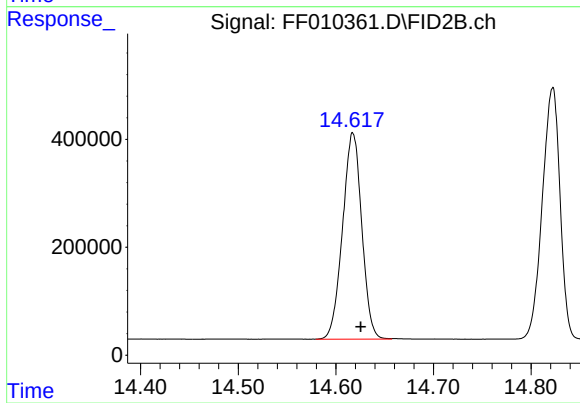


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.617 min
Delta R.T.: -0.009 min
Response: 5230595
Conc: 43.76 ug/ml m

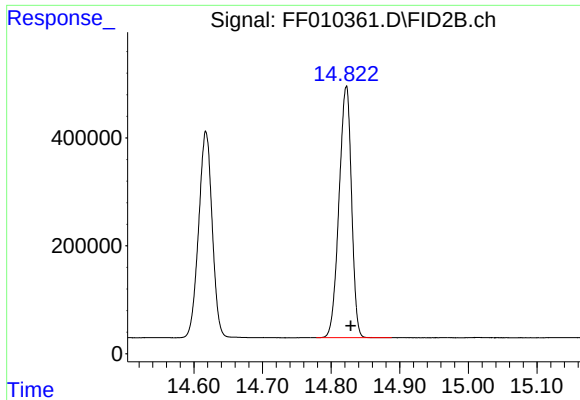


#10 N-TETRACOSANE

R.T.: 14.822 min
Delta R.T.: -0.007 min
Response: 5880589
Conc: 43.92 ug/ml

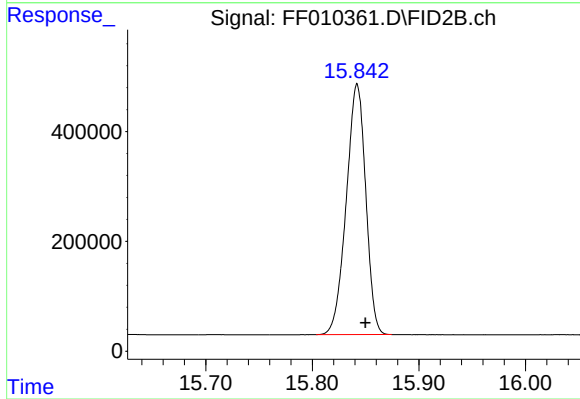

#11 N-HEXACOSANE

R.T.: 15.842 min
Delta R.T.: -0.008 min
Response: 5799276
Conc: 43.72 ug/ml m

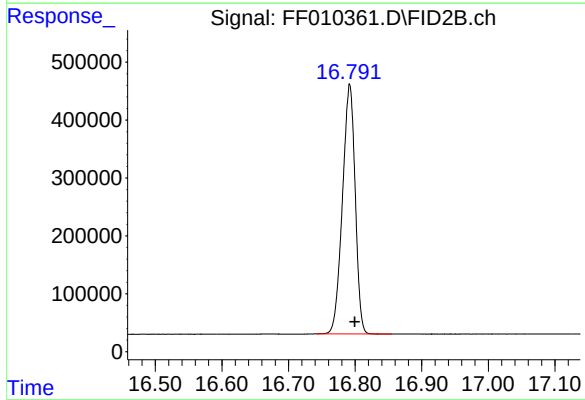

#12 N-OCTACOSANE

R.T.: 16.792 min
Delta R.T.: -0.008 min
Response: 5721792
Conc: 43.17 ug/ml