

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041719\
 Data File : FF004250.D
 Signal(s) : FID2B.ch
 Acq On : 17 Apr 2019 18:17
 Operator : AJ\SJ
 Sample : K2424-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 18 00:49:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.536	2202858	16.945 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.163f	164124	1.154 ug/ml
11)	N-HEXACOSANE	15.760	154080	1.061 ug/ml
12)	N-OCTACOSANE	16.710	437488	3.043 ug/ml
13)	N-TRIACONTANE	17.598	579396	4.057 ug/ml
14)	N-DOTRIACONTANE	18.430	378085	2.678 ug/ml
16)	N-HEXATRIACONTANE	19.957	31392	0.247 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041719\
Data File : FF004250.D
Signal(s) : FID2B.ch
Acq On : 17 Apr 2019 18:17
Operator : AJ\SJ
Sample : K2424-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 18 00:49:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

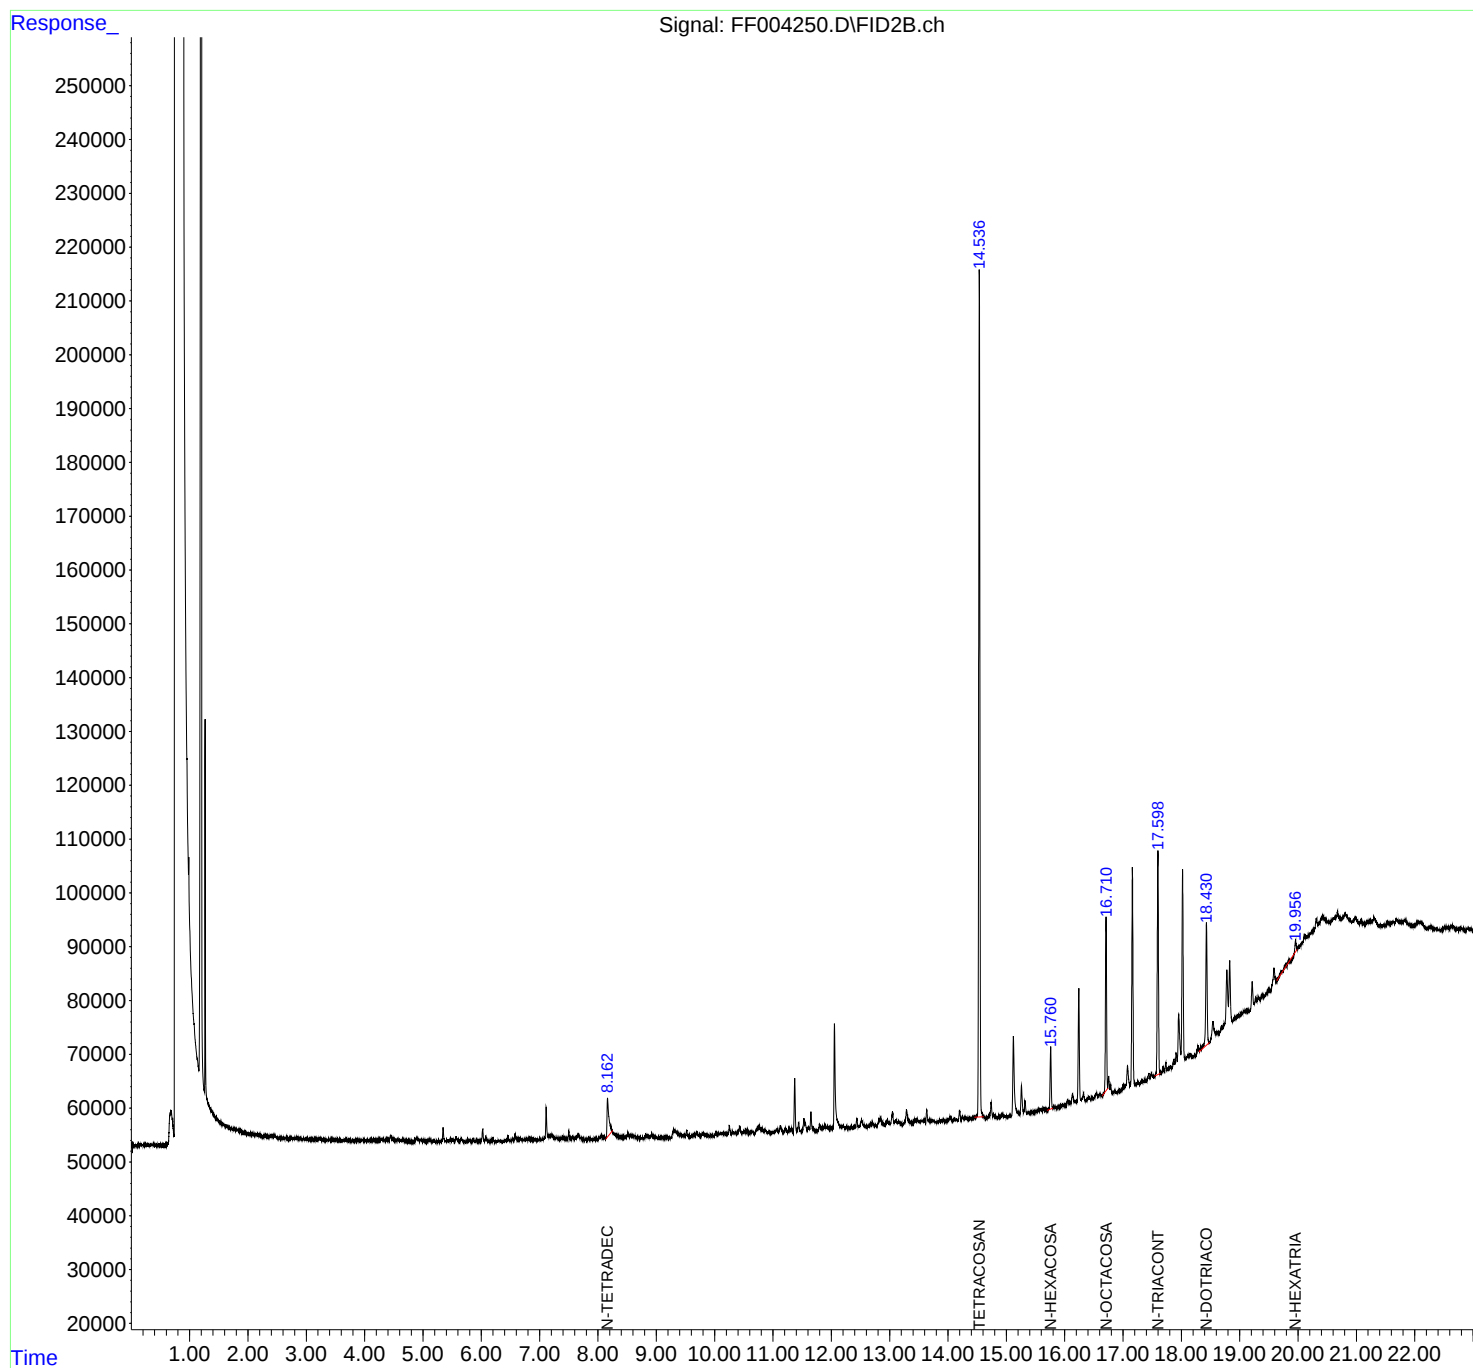

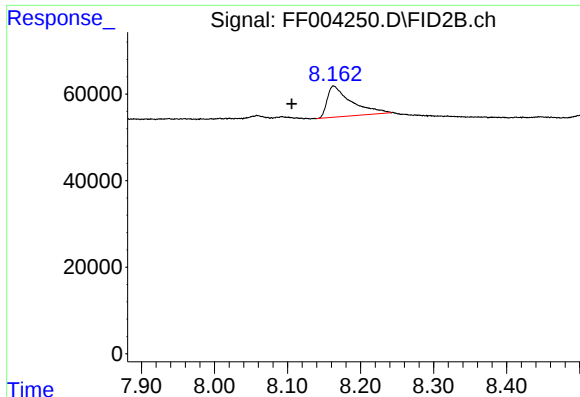


#4 N-TETRADECANE

R.T.: 8.163 min
Delta R.T.: 0.058 min
Response: 164124
Conc: 1.15 ug/ml

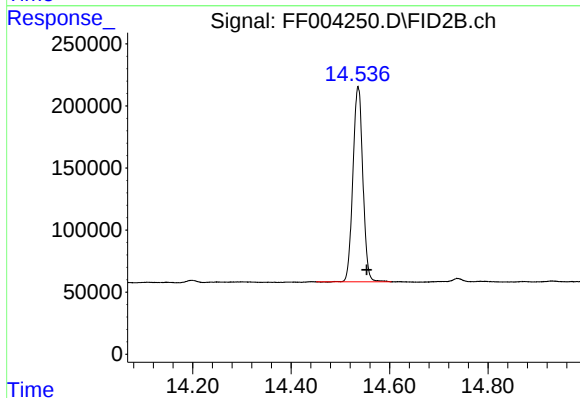


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.536 min
Delta R.T.: -0.017 min
Response: 2202858
Conc: 16.95 ug/ml

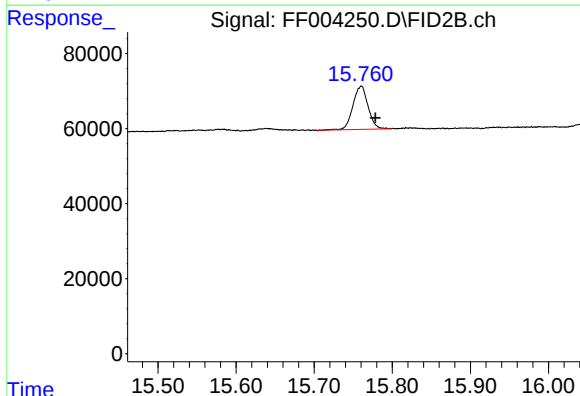


#11 N-HEXACOSANE

R.T.: 15.760 min
Delta R.T.: -0.018 min
Response: 154080
Conc: 1.06 ug/ml

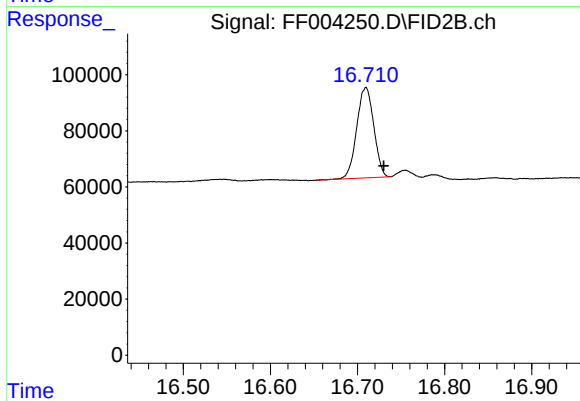


#12 N-OCTACOSANE

R.T.: 16.710 min
Delta R.T.: -0.021 min
Response: 437488
Conc: 3.04 ug/ml

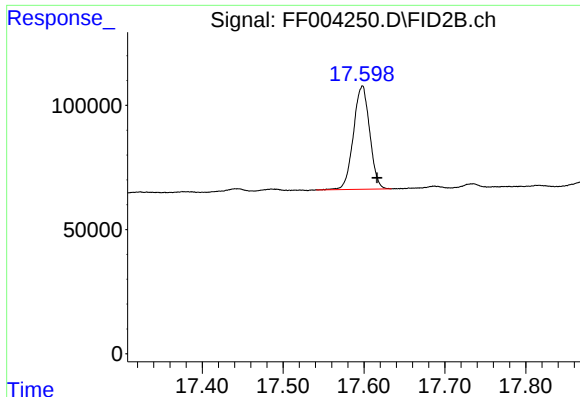


#13 N-TRIACONTANE

R.T.: 17.598 min
Delta R.T.: -0.019 min
Response: 579396
Conc: 4.06 ug/ml

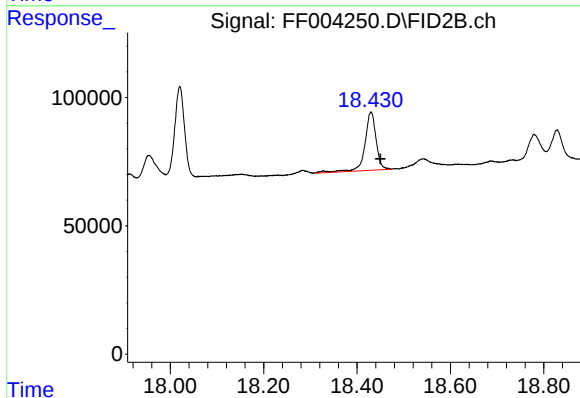

#14 N-DOTRIACONTANE

R.T.: 18.430 min
Delta R.T.: -0.020 min
Response: 378085
Conc: 2.68 ug/ml

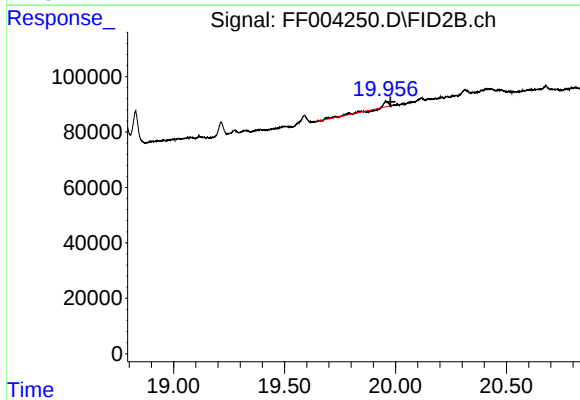

#16 N-HEXATRIACONTANE

R.T.: 19.957 min
Delta R.T.: -0.020 min
Response: 31392
Conc: 0.25 ug/ml