

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041723\
Data File : FF012485.D
Signal(s) : FID2B.ch
Acq On : 17 Apr 2023 08:51
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 18 01:42:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) N-TETRACONTANE	22.082	194976	2.016 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041723\
Data File : FF012485.D
Signal(s) : FID2B.ch
Acq On : 17 Apr 2023 08:51
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 18 01:42:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

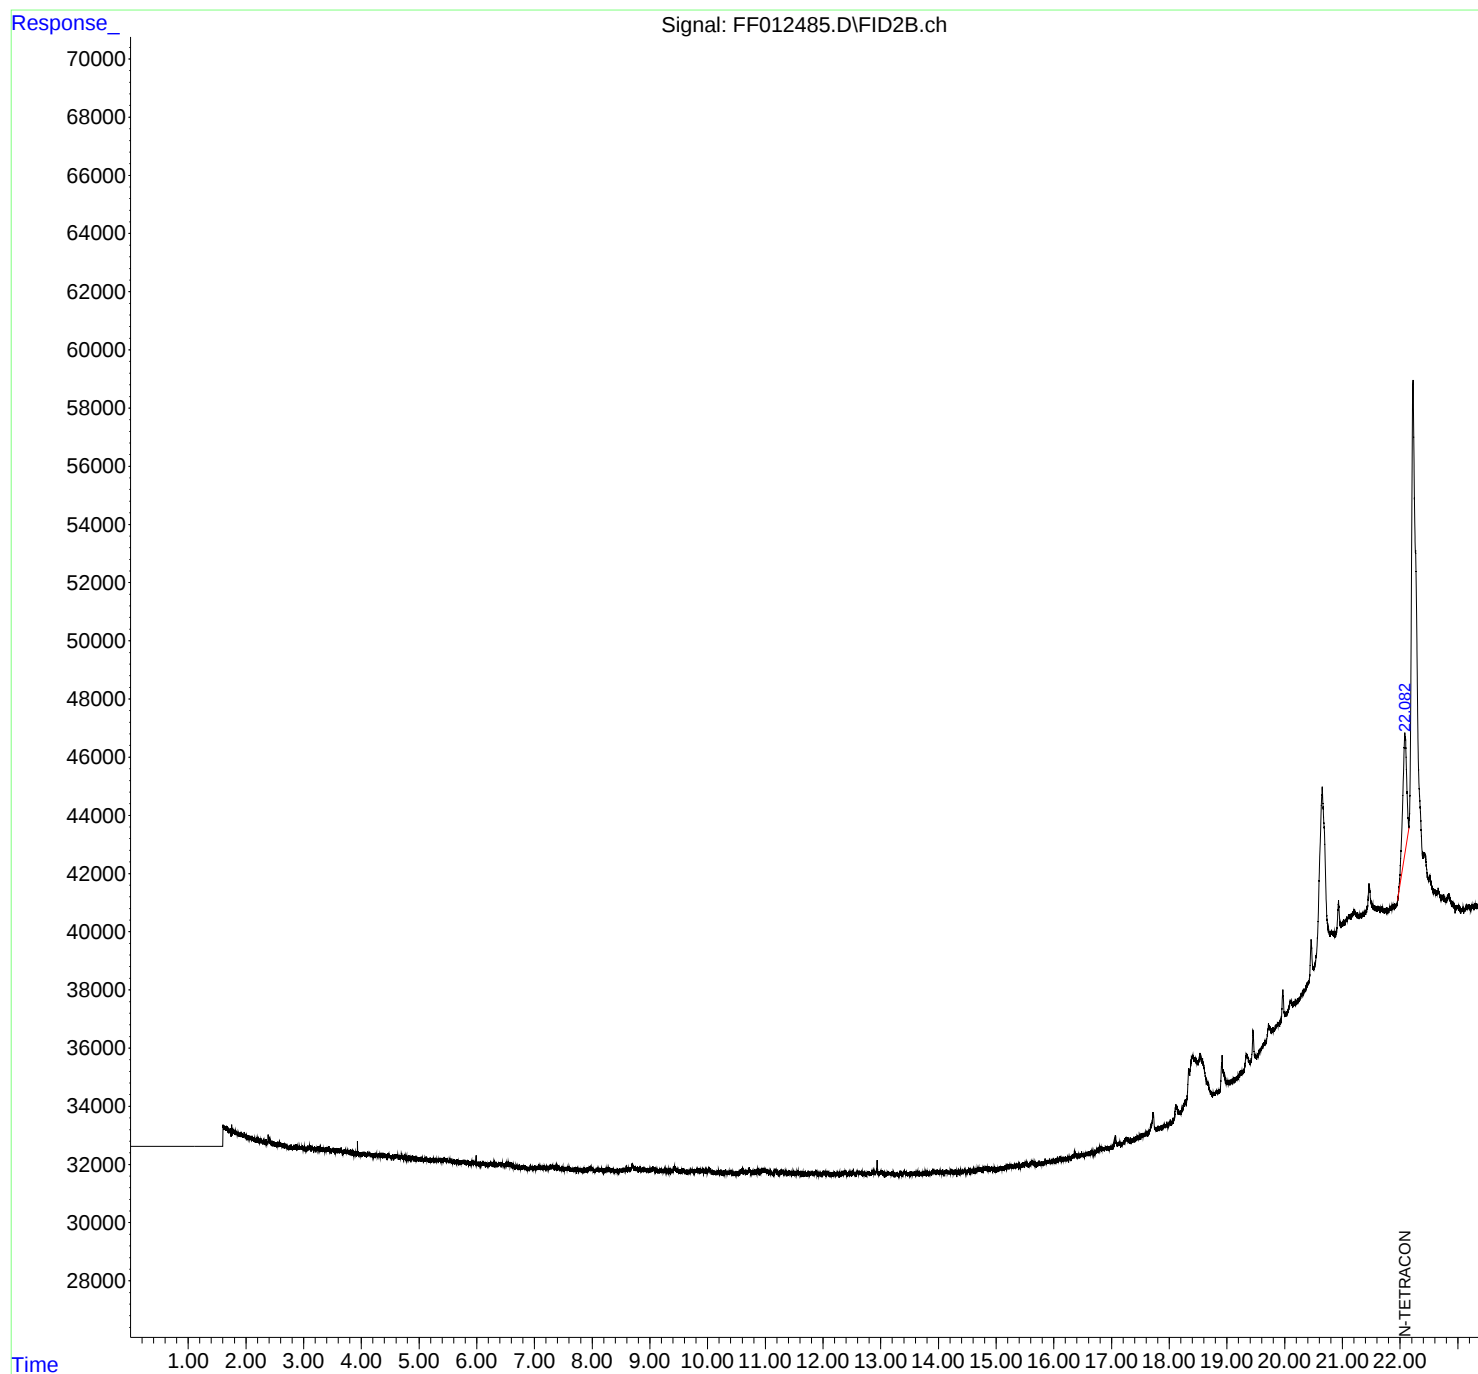


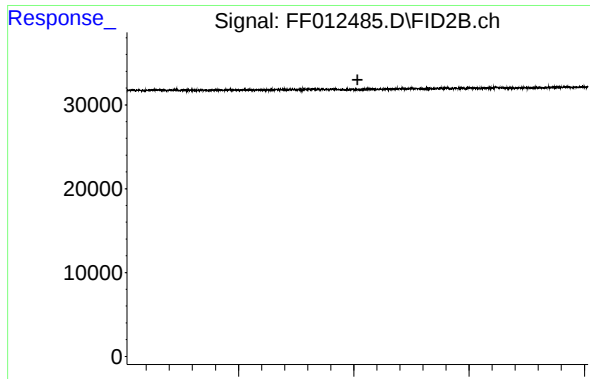

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.016 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

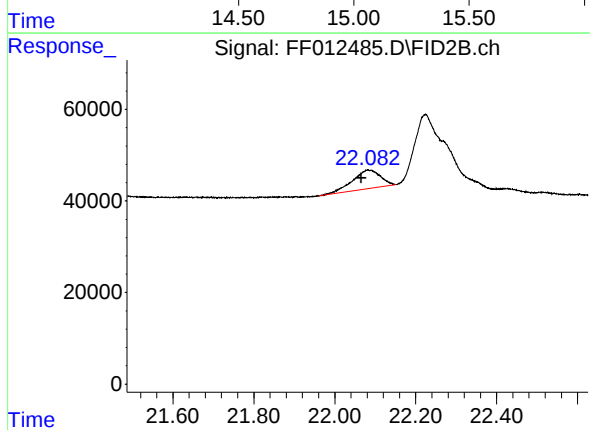

#18 N-TETRACONTANE

R.T.: 22.082 min
Delta R.T.: 0.016 min
Response: 194976
Conc: 2.02 ug/ml