

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041723\
 Data File : FF012496.D
 Signal(s) : FID2B.ch
 Acq On : 17 Apr 2023 18:54
 Operator : YP\AJ
 Sample : 02371-06 10X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 18 01:44:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.006	210007	1.747 ug/ml
Target Compounds			
7) N-EICOSANE	12.928	68989	0.501 ug/ml
8) N-DOCOSANE	14.149	232111	1.724 ug/ml
10) N-TETRACOSANE	15.201	911881	6.741 ug/ml
12) N-OCTACOSANE	17.203	130729	0.991 ug/ml
13) N-TRIACONTANE	18.065	58624	0.449 ug/ml
14) N-DOTRIACONTANE	18.867	175666	1.393 ug/ml
15) N-TETRATRIACONTANE	19.677	24612	0.217 ug/ml
16) N-HEXATRIACONTANE	20.413	64945	0.636 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041723\
Data File : FF012496.D
Signal(s) : FID2B.ch
Acq On : 17 Apr 2023 18:54
Operator : YP\AJ
Sample : 02371-06 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 18 01:44:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

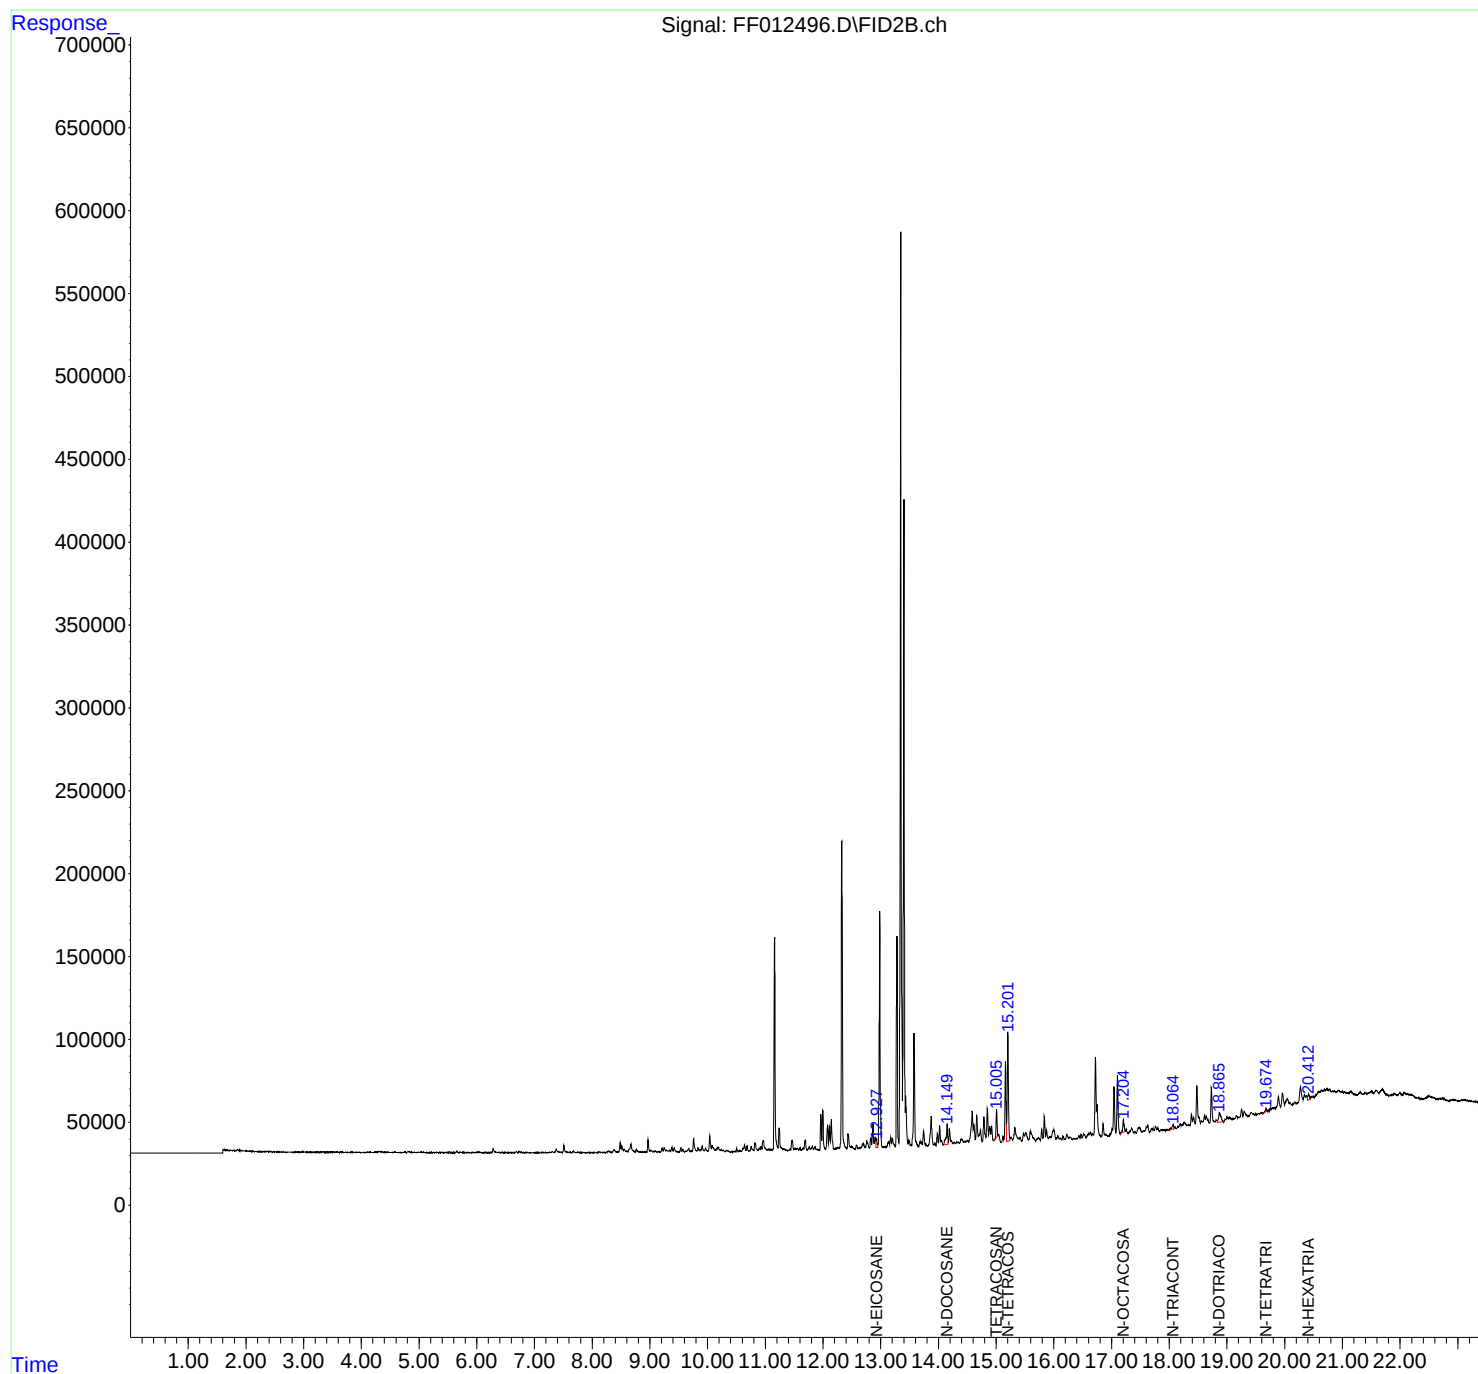


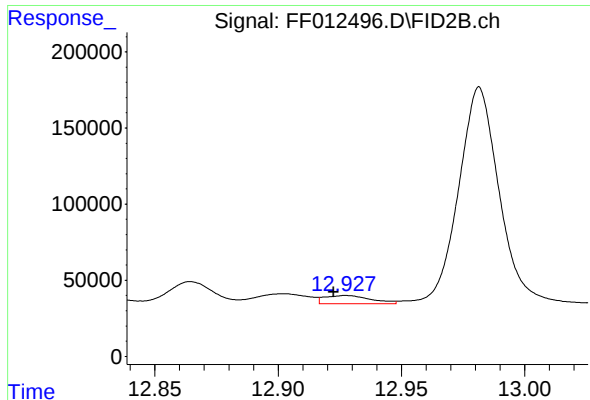

#7 N-EICOSANE


R.T.: 12.928 min
Delta R.T.: 0.005 min
Response: 68989
Conc: 0.50 ug/ml

Instrument :
FID_F
ClientSampleId :

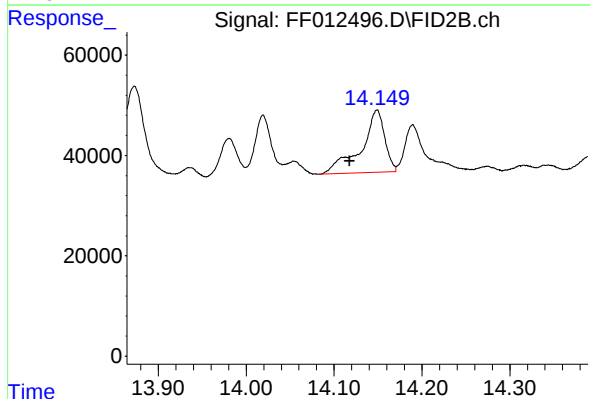


#8 N-DOCOSANE

R.T.: 14.149 min
Delta R.T.: 0.031 min
Response: 232111
Conc: 1.72 ug/ml

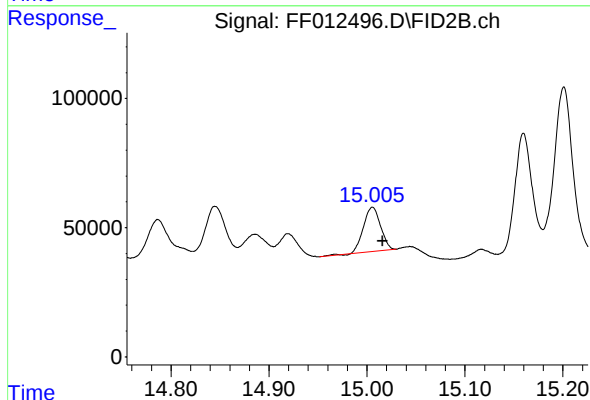


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.006 min
Delta R.T.: -0.010 min
Response: 210007
Conc: 1.75 ug/ml

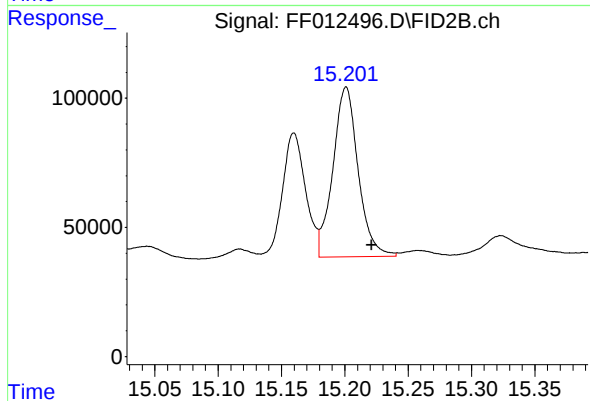

#10 N-TETRACOSANE


R.T.: 15.201 min
Delta R.T.: -0.020 min
Response: 911881
Conc: 6.74 ug/ml

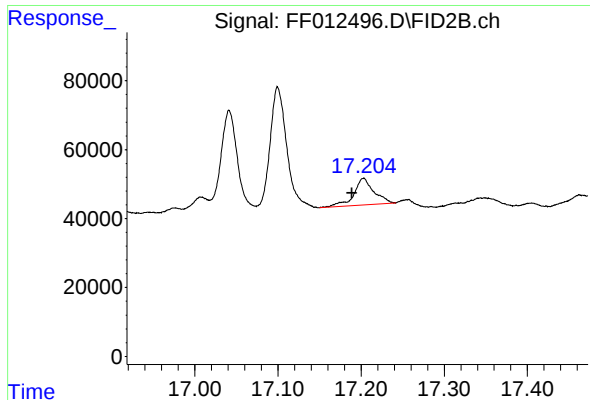

#12 N-OCTACOSANE


R.T.: 17.203 min
Delta R.T.: 0.014 min
Response: 130729
Conc: 0.99 ug/ml

Instrument :
FID_F
ClientSampleId :

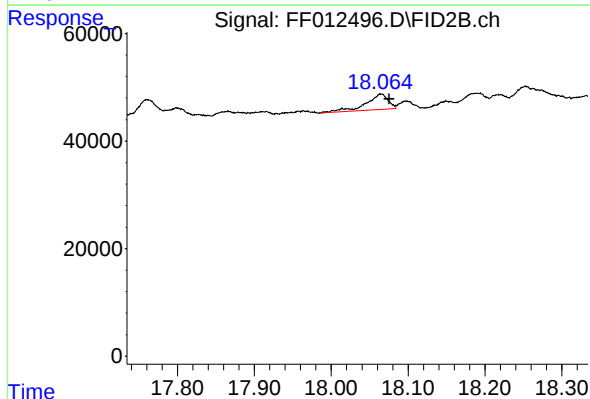


#13 N-TRIACONTANE

R.T.: 18.065 min
Delta R.T.: -0.010 min
Response: 58624
Conc: 0.45 ug/ml

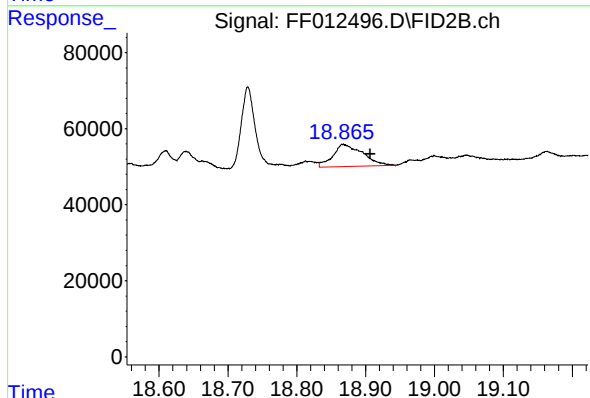


#14 N-DOTRIACONTANE

R.T.: 18.867 min
Delta R.T.: -0.040 min
Response: 175666
Conc: 1.39 ug/ml

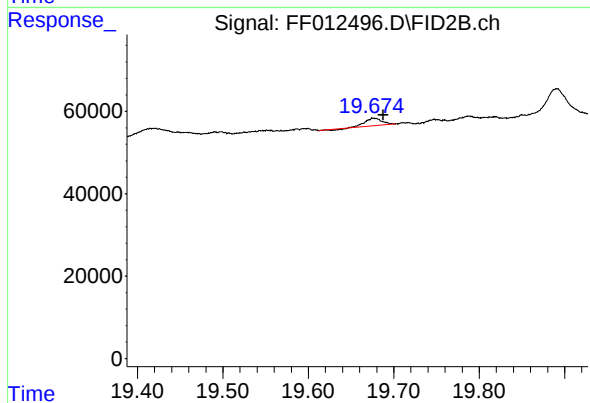

#15 N-TETRATRIACONTANE

R.T.: 19.677 min
Delta R.T.: -0.011 min
Response: 24612
Conc: 0.22 ug/ml

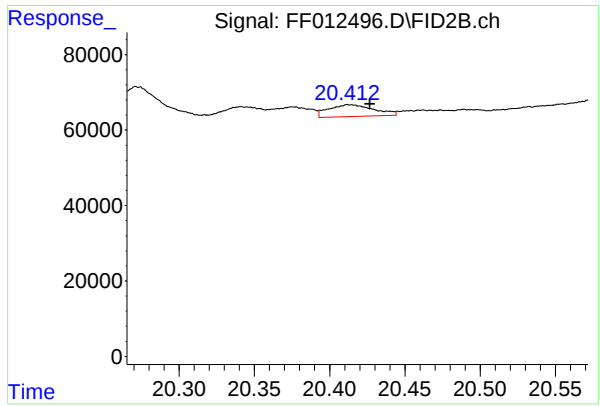

#16 N-HEXATRIACONTANE

R.T.: 20.413 min
Delta R.T.: -0.014 min
Response: 64945
Conc: 0.64 ug/ml

Instrument :

FID_F

ClientSampleId :