

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041823\
Data File : FF012502.D
Signal(s) : FID2B.ch
Acq On : 18 Apr 2023 11:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 18 23:10:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.734	2848949	23.067 ug/ml
12) N-OCTACOSANE	17.175	3066814	23.253 ug/ml
13) N-TRIACONTANE	18.058	128979	0.988 ug/ml
14) N-DOTRIACONTANE	18.890	170891	1.355 ug/ml
15) N-TETRATRIACONTANE	19.673	135811	1.198 ug/ml
16) N-HEXATRIACONTANE	20.415	58459	0.572 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041823\
Data File : FF012502.D
Signal(s) : FID2B.ch
Acq On : 18 Apr 2023 11:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 18 23:10:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

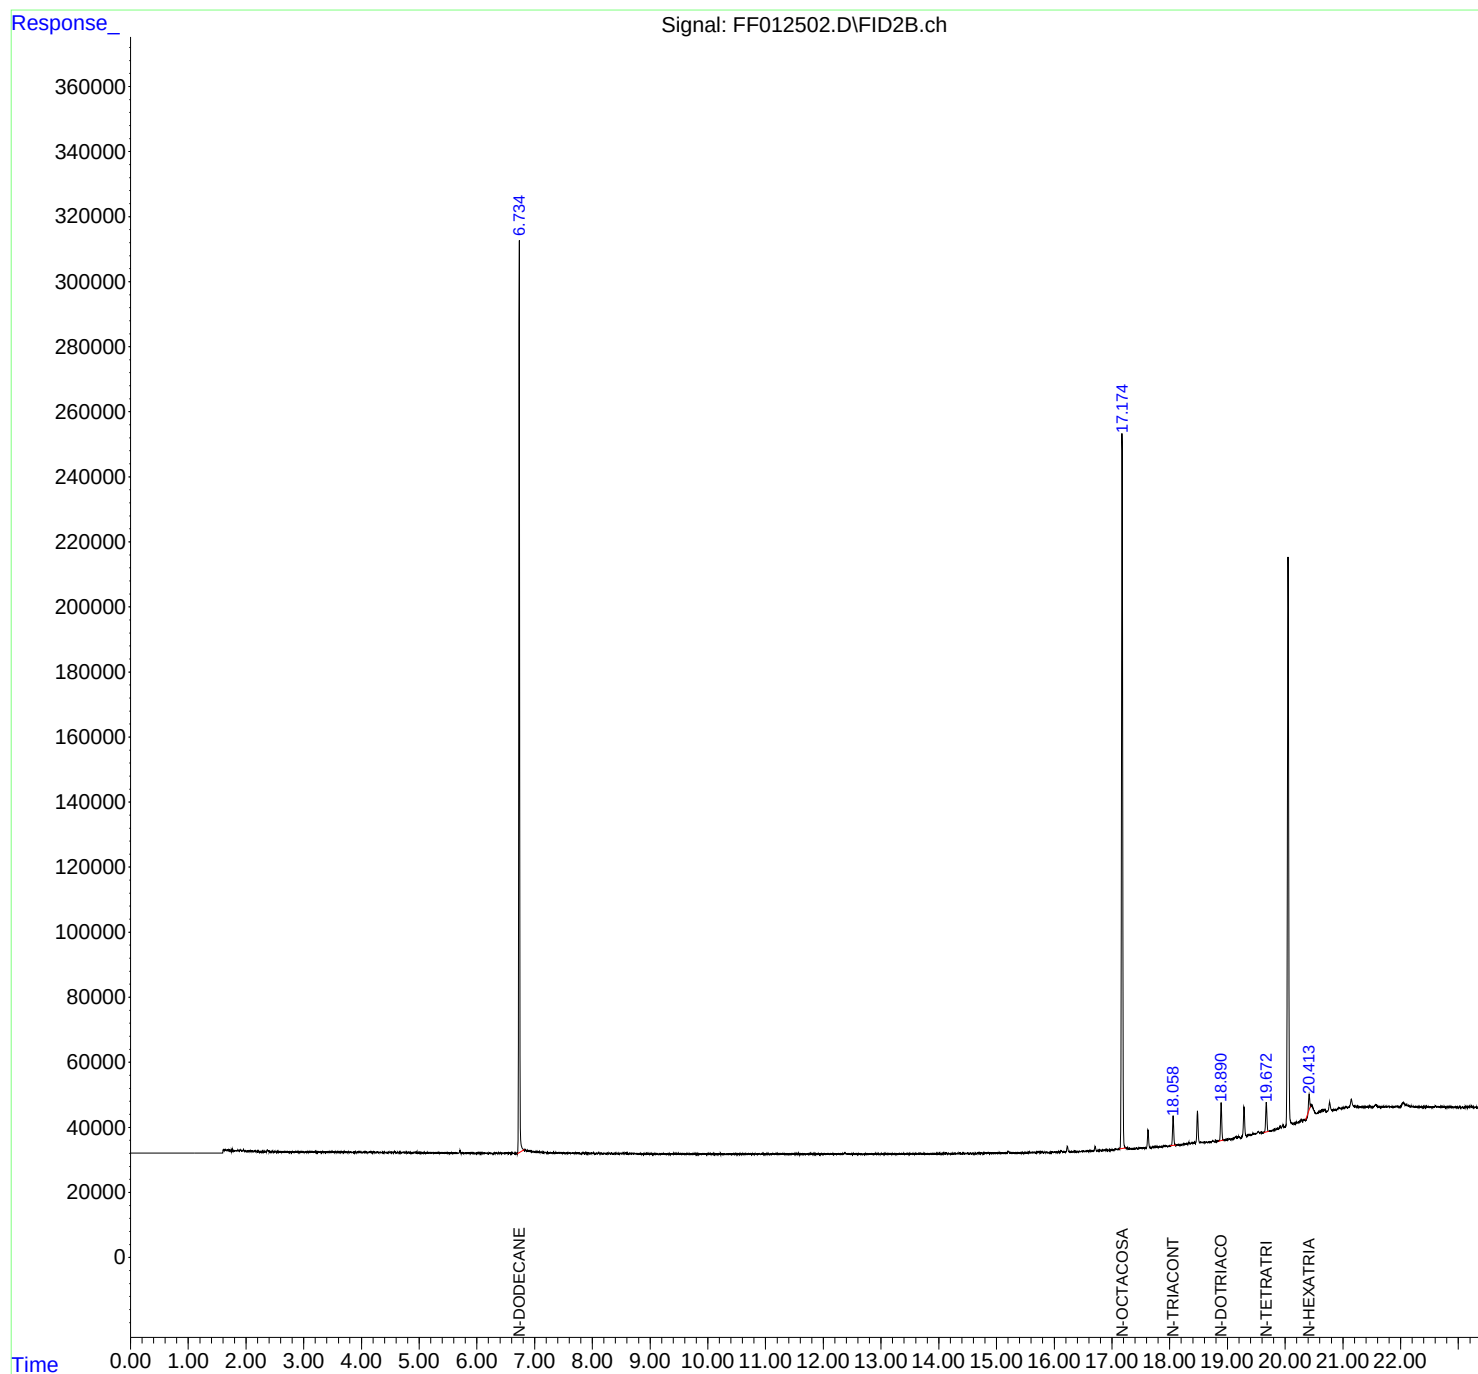


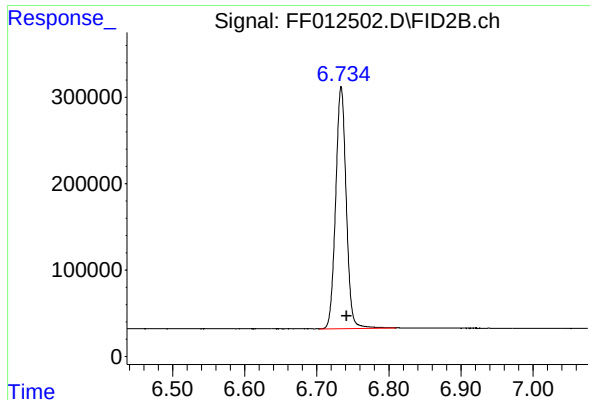

#3 N-DODECANE


R.T.: 6.734 min
Delta R.T.: -0.007 min
Response: 2848949
Conc: 23.07 ug/ml

Instrument :
FID_F
ClientSampleId :

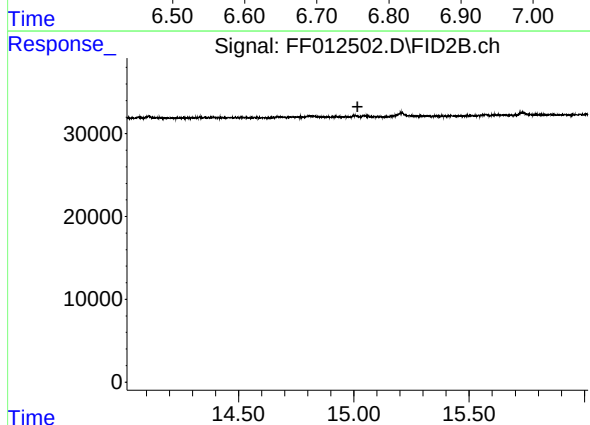


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.016 min
Response: 0
Conc: N.D.

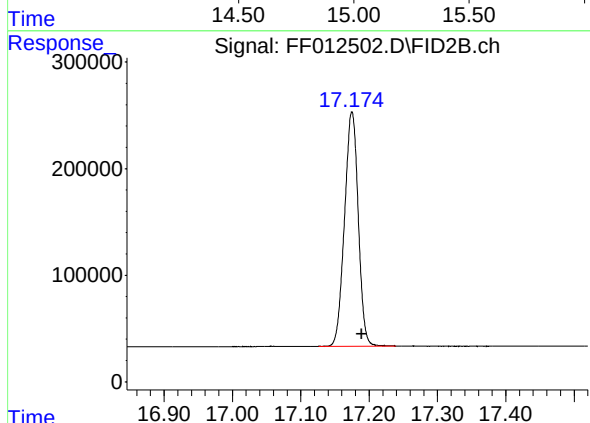


#12 N-OCTACOSANE

R.T.: 17.175 min
Delta R.T.: -0.014 min
Response: 3066814
Conc: 23.25 ug/ml

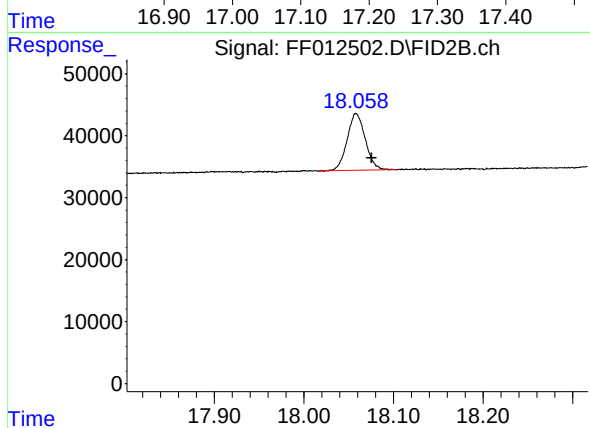

#13 N-TRIACONTANE


R.T.: 18.058 min
Delta R.T.: -0.017 min
Response: 128979
Conc: 0.99 ug/ml

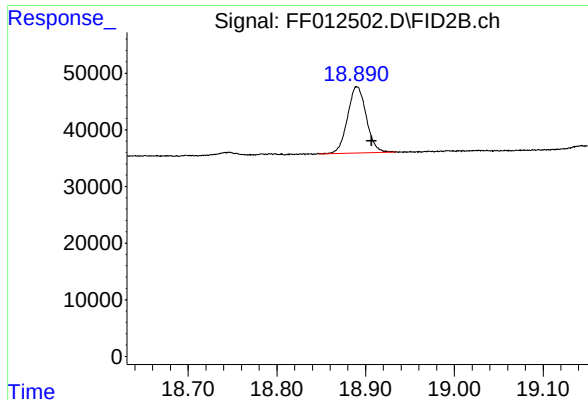

#14 N-DOTRIACONTANE


R.T.: 18.890 min
Delta R.T.: -0.017 min
Response: 170891
Conc: 1.35 ug/ml

Instrument :
FID_F
ClientSampleId :

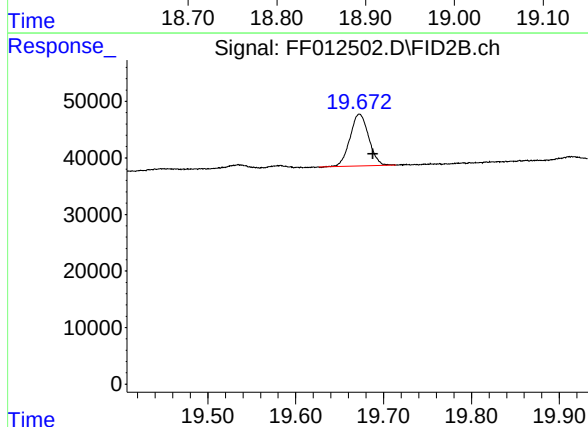

#15 N-TETRATRIACONTANE

R.T.: 19.673 min
Delta R.T.: -0.015 min
Response: 135811
Conc: 1.20 ug/ml

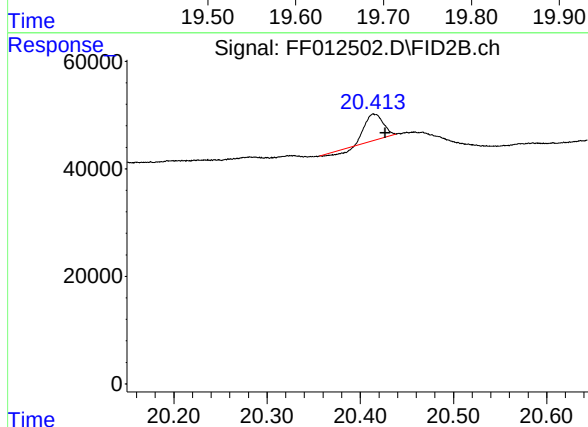

#16 N-HEXATRIACONTANE

R.T.: 20.415 min
Delta R.T.: -0.012 min
Response: 58459
Conc: 0.57 ug/ml