

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041823\
 Data File : FF012505.D
 Signal(s) : FID2B.ch
 Acq On : 18 Apr 2023 12:57
 Operator : YP\AJ
 Sample : 02384-03
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 ROLL-OFF-5PT-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/19/2023
 Supervised By :Ankita Jodhani 04/19/2023

Integration File: autoint1.e
 Quant Time: Apr 18 23:11:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
 Quant Title :
 QLast Update : Thu Apr 13 15:26:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.000	3011729	25.055 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041823\
Data File : FF012505.D
Signal(s) : FID2B.ch
Acq On : 18 Apr 2023 12:57
Operator : YP\AJ
Sample : 02384-03
Misc :
ALS Vial : 63 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
ROLL-OFF-5PT-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023

Integration File: autoint1.e
Quant Time: Apr 18 23:11:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF041323.M
Quant Title :
QLast Update : Thu Apr 13 15:26:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

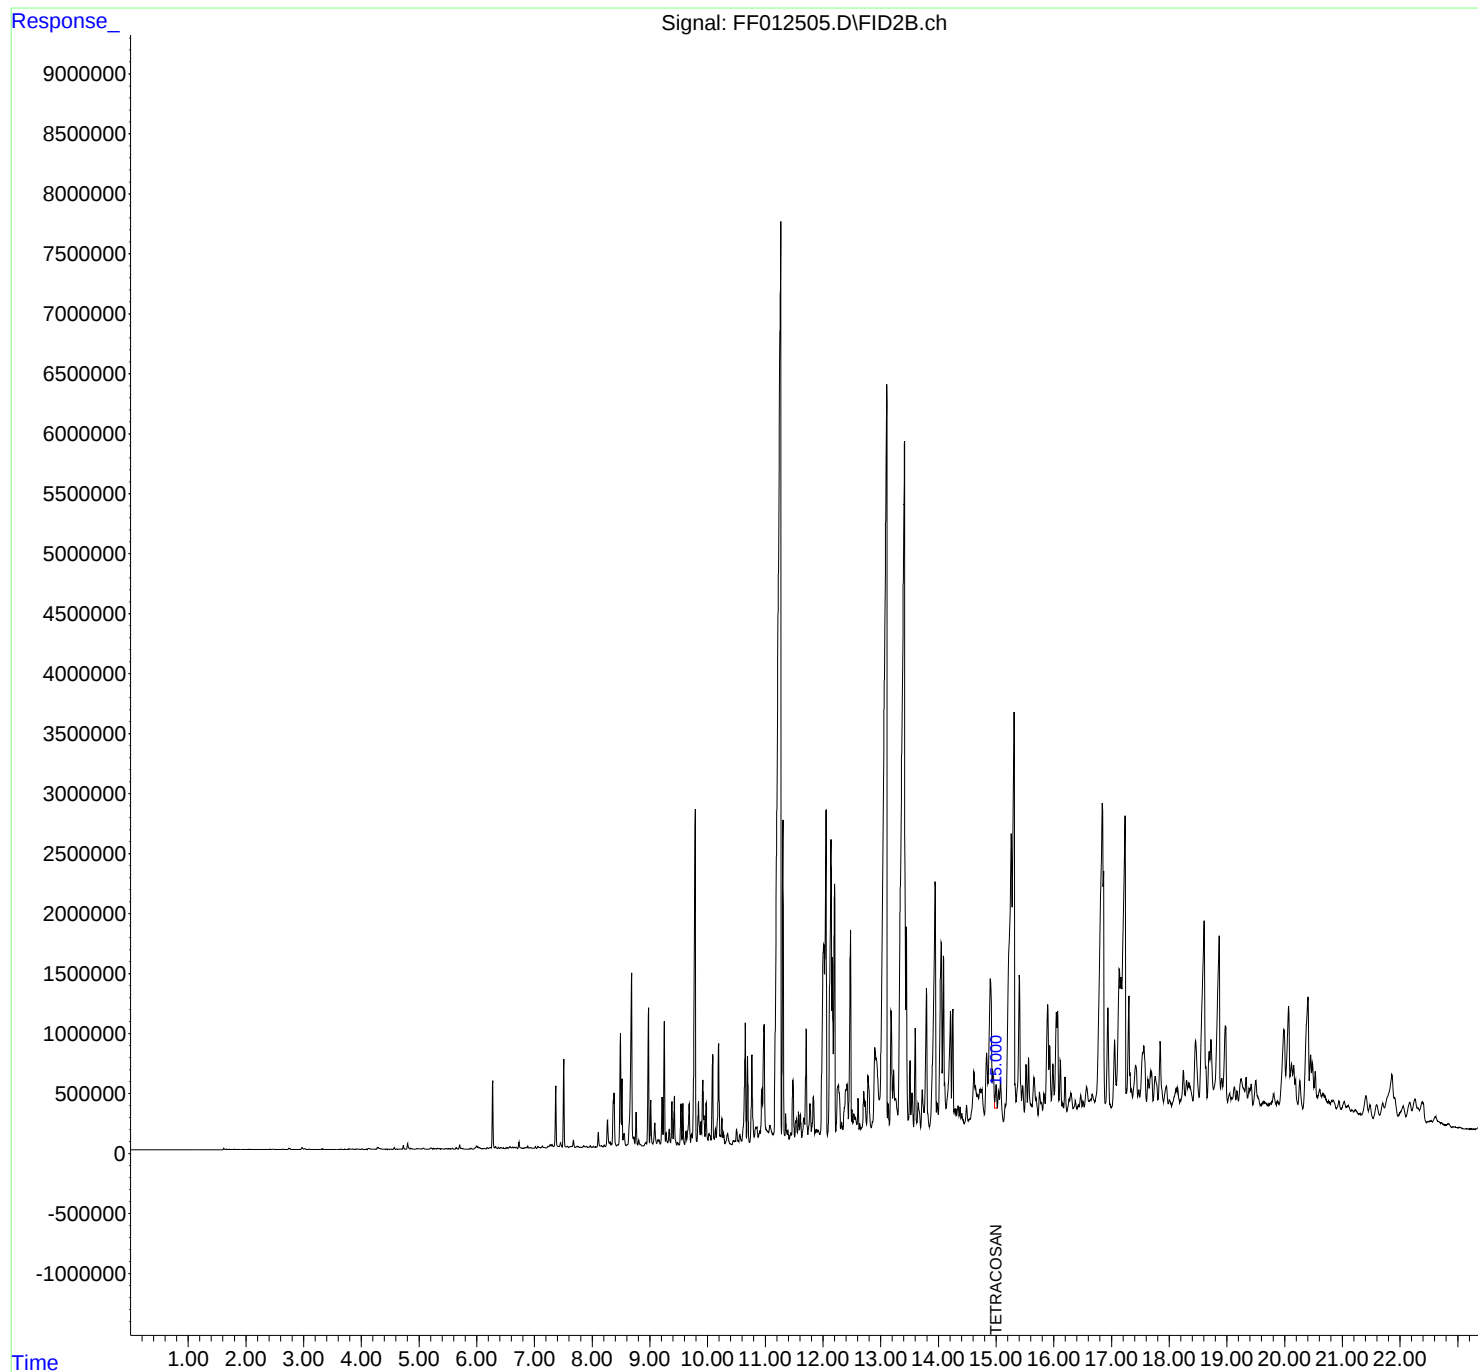

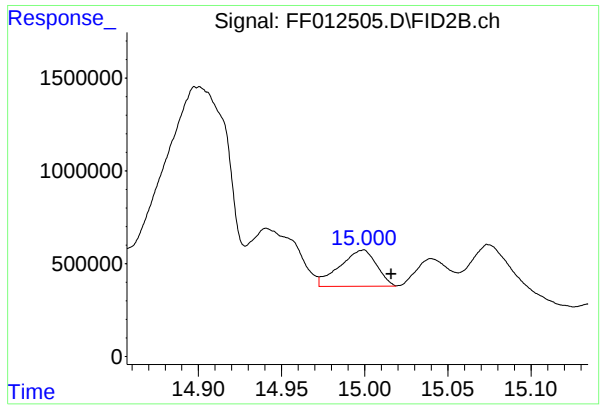

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.000 min
Delta R.T.: -0.016 min
Response: 3011729
Conc: 25.06 ug/ml

Instrument :
FID_F
ClientSampleId :
ROLL-OFF-5PT-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2023
Supervised By :Ankita Jodhani 04/19/2023