

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041919\
 Data File : FF004269.D
 Signal(s) : FID2B.ch
 Acq On : 19 Apr 2019 14:10
 Operator : AJ\SJ
 Sample : K2201-03 10X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 19 23:18:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.561	260030	2.000 ug/ml
Target Compounds			
6) N-OCTADECANE	11.211f	342614	2.275 ug/ml
7) N-EICOSANE	12.442	284246	1.891 ug/ml
8) N-DOCOSANE	13.663	719046	4.804 ug/ml
10) N-TETRACOSANE	14.720	3366605	22.856 ug/ml
11) N-HEXACOSANE	15.785	168970	1.164 ug/ml
12) N-OCTACOSANE	16.732	1089286	7.576 ug/ml
13) N-TRIACONTANE	17.632	88650	0.621 ug/ml
14) N-DOTRIACONTANE	18.414	917344	6.498 ug/ml
15) N-TETRATRIACONTANE	19.226	258888	1.941 ug/ml
16) N-HEXATRIACONTANE	19.962	848345	6.686 ug/ml
17) N-OCTATRIACONTANE	20.689	260986	2.293 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041919\
Data File : FF004269.D
Signal(s) : FID2B.ch
Acq On : 19 Apr 2019 14:10
Operator : AJ\SJ
Sample : K2201-03 10X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 19 23:18:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

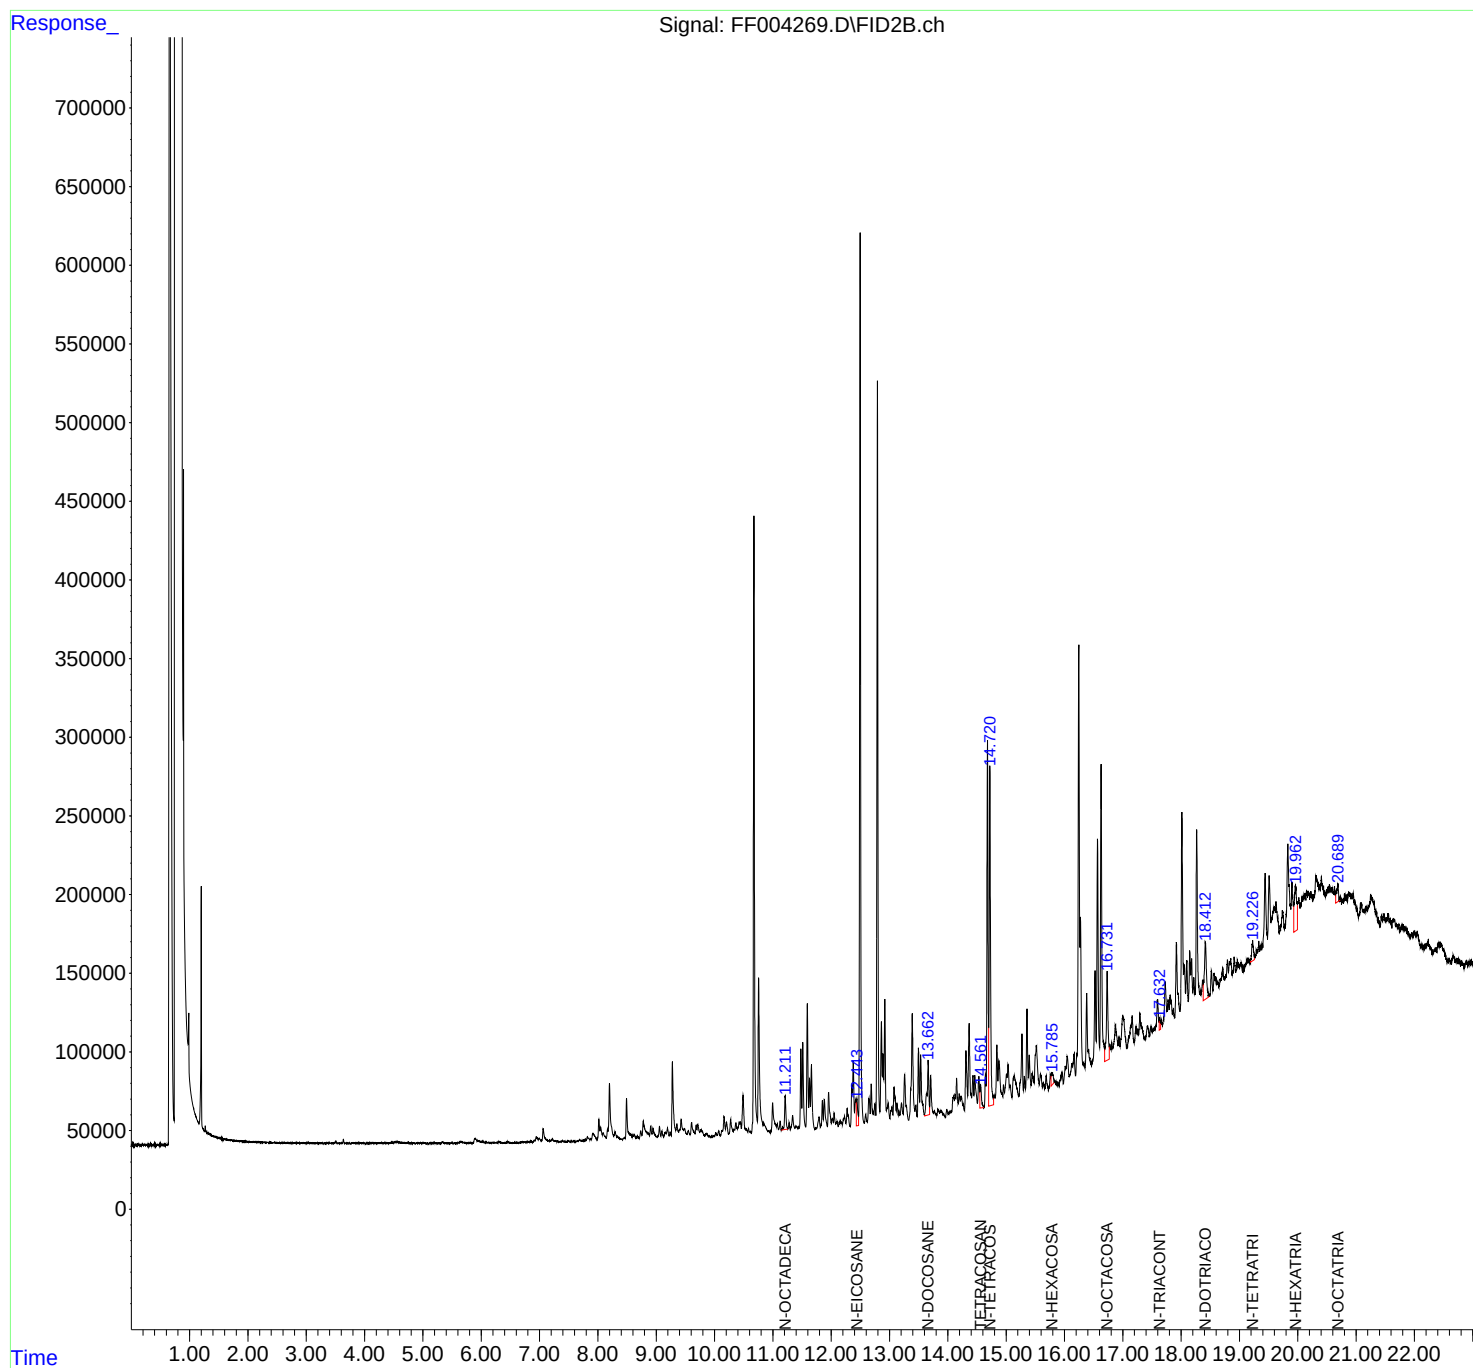

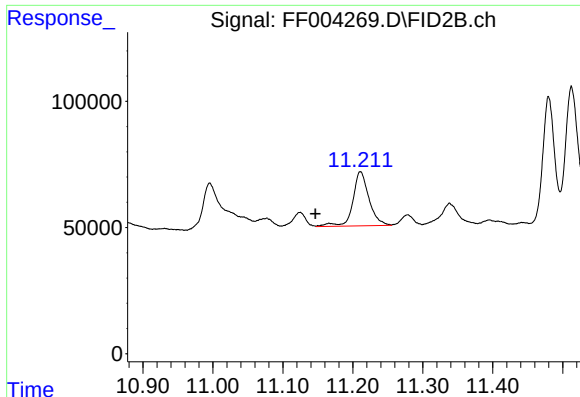


#6 N-OCTADECANE

R.T.: 11.211 min
Delta R.T.: 0.065 min
Response: 342614
Conc: 2.28 ug/ml

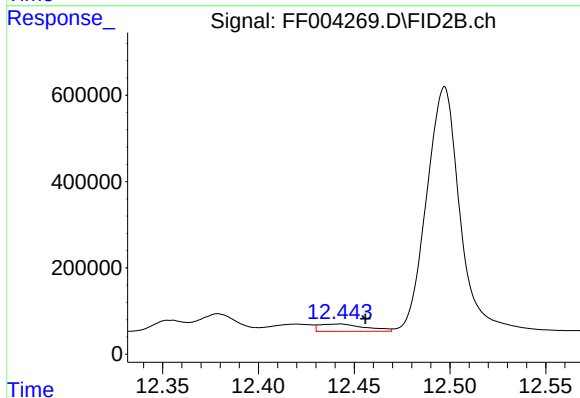


#7 N-EICOSANE

R.T.: 12.442 min
Delta R.T.: -0.014 min
Response: 284246
Conc: 1.89 ug/ml

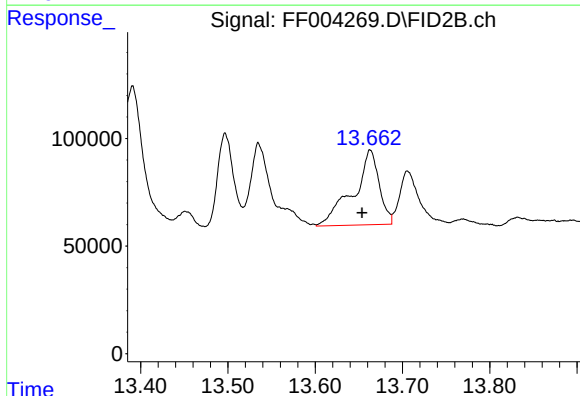


#8 N-DOCOSANE

R.T.: 13.663 min
Delta R.T.: 0.009 min
Response: 719046
Conc: 4.80 ug/ml

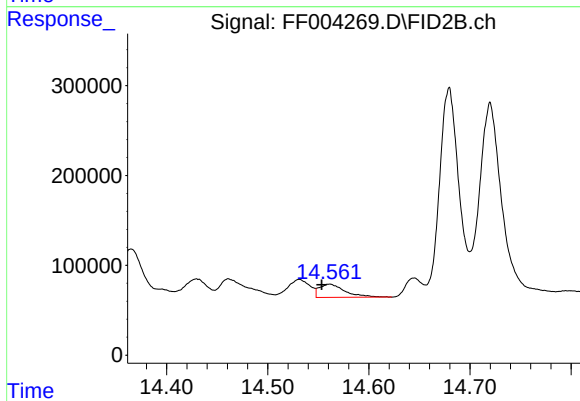


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.561 min
Delta R.T.: 0.008 min
Response: 260030
Conc: 2.00 ug/ml

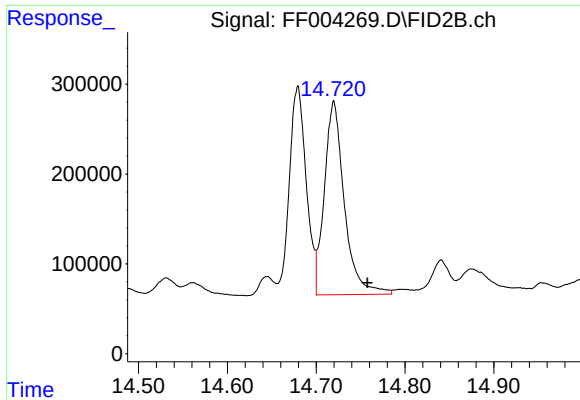


#10 N-TETRACOSANE

R.T.: 14.720 min
Delta R.T.: -0.038 min
Response: 3366605
Conc: 22.86 ug/ml

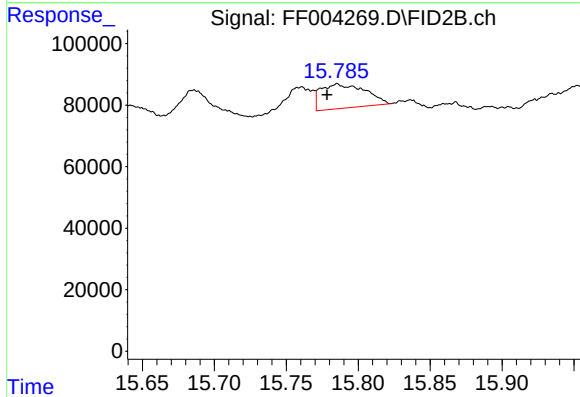


#11 N-HEXACOSANE

R.T.: 15.785 min
Delta R.T.: 0.007 min
Response: 168970
Conc: 1.16 ug/ml

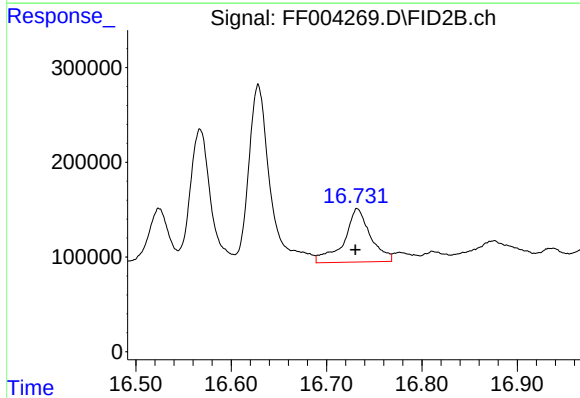


#12 N-OCTACOSANE

R.T.: 16.732 min
Delta R.T.: 0.002 min
Response: 1089286
Conc: 7.58 ug/ml

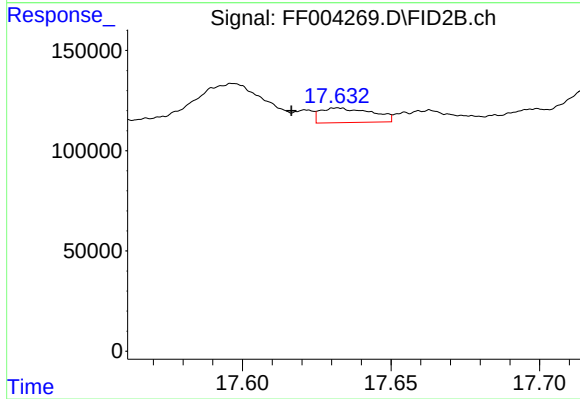


#13 N-TRIACONTANE

R.T.: 17.632 min
Delta R.T.: 0.016 min
Response: 88650
Conc: 0.62 ug/ml

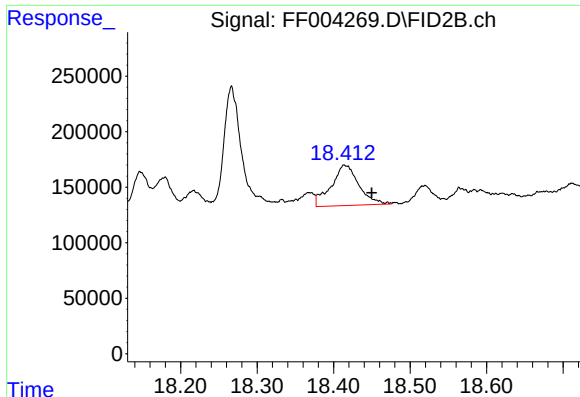


#14 N-DOTRIACONTANE

R.T.: 18.414 min
Delta R.T.: -0.036 min
Response: 917344
Conc: 6.50 ug/ml

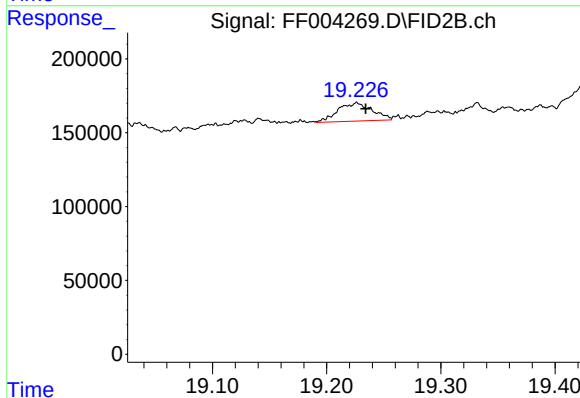


#15 N-TETRATRIACONTANE

R.T.: 19.226 min
Delta R.T.: -0.008 min
Response: 258888
Conc: 1.94 ug/ml

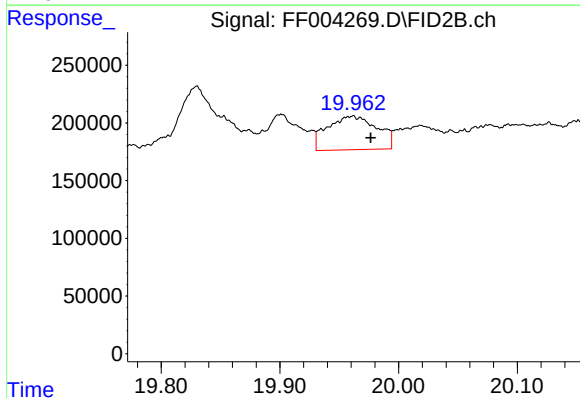

#16 N-HEXATRIACONTANE

R.T.: 19.962 min
Delta R.T.: -0.015 min
Response: 848345
Conc: 6.69 ug/ml

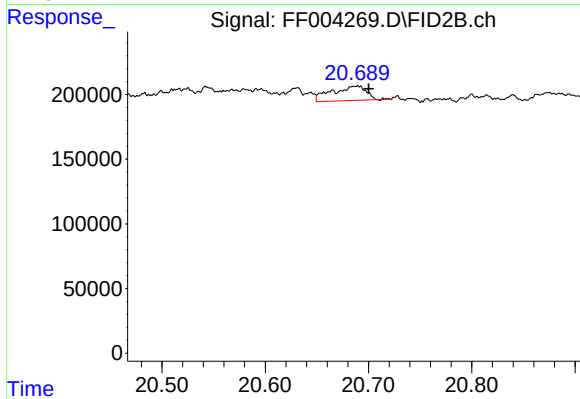

#17 N-OCTATRIACONTANE

R.T.: 20.689 min
Delta R.T.: -0.011 min
Response: 260986
Conc: 2.29 ug/ml