

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041919\
 Data File : FF004279.D
 Signal(s) : FID2B.ch
 Acq On : 19 Apr 2019 19:14
 Operator : AJ\SJ
 Sample : K2201-03 20X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 19 23:21:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.534	68141	0.524 ug/ml
Target Compounds			
6) N-OCTADECANE	11.212f	150377	0.999 ug/ml
7) N-EICOSANE	12.497	3253628	21.650 ug/ml
8) N-DOCOSANE	13.667	234979	1.570 ug/ml
10) N-TETRACOSANE	14.724	1556440	10.567 ug/ml
12) N-OCTACOSANE	16.740	485008	3.373 ug/ml
13) N-TRIACONTANE	17.602	218725	1.532 ug/ml
14) N-DOTRIACONTANE	18.429	525746	3.724 ug/ml
15) N-TETRATRIACONTANE	19.223	167128	1.253 ug/ml
16) N-HEXATRIACONTANE	19.978	481063	3.791 ug/ml
17) N-OCTATRIACONTANE	20.762f	43769	0.384 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041919\
Data File : FF004279.D
Signal(s) : FID2B.ch
Acq On : 19 Apr 2019 19:14
Operator : AJ\SJ
Sample : K2201-03 20X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 19 23:21:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

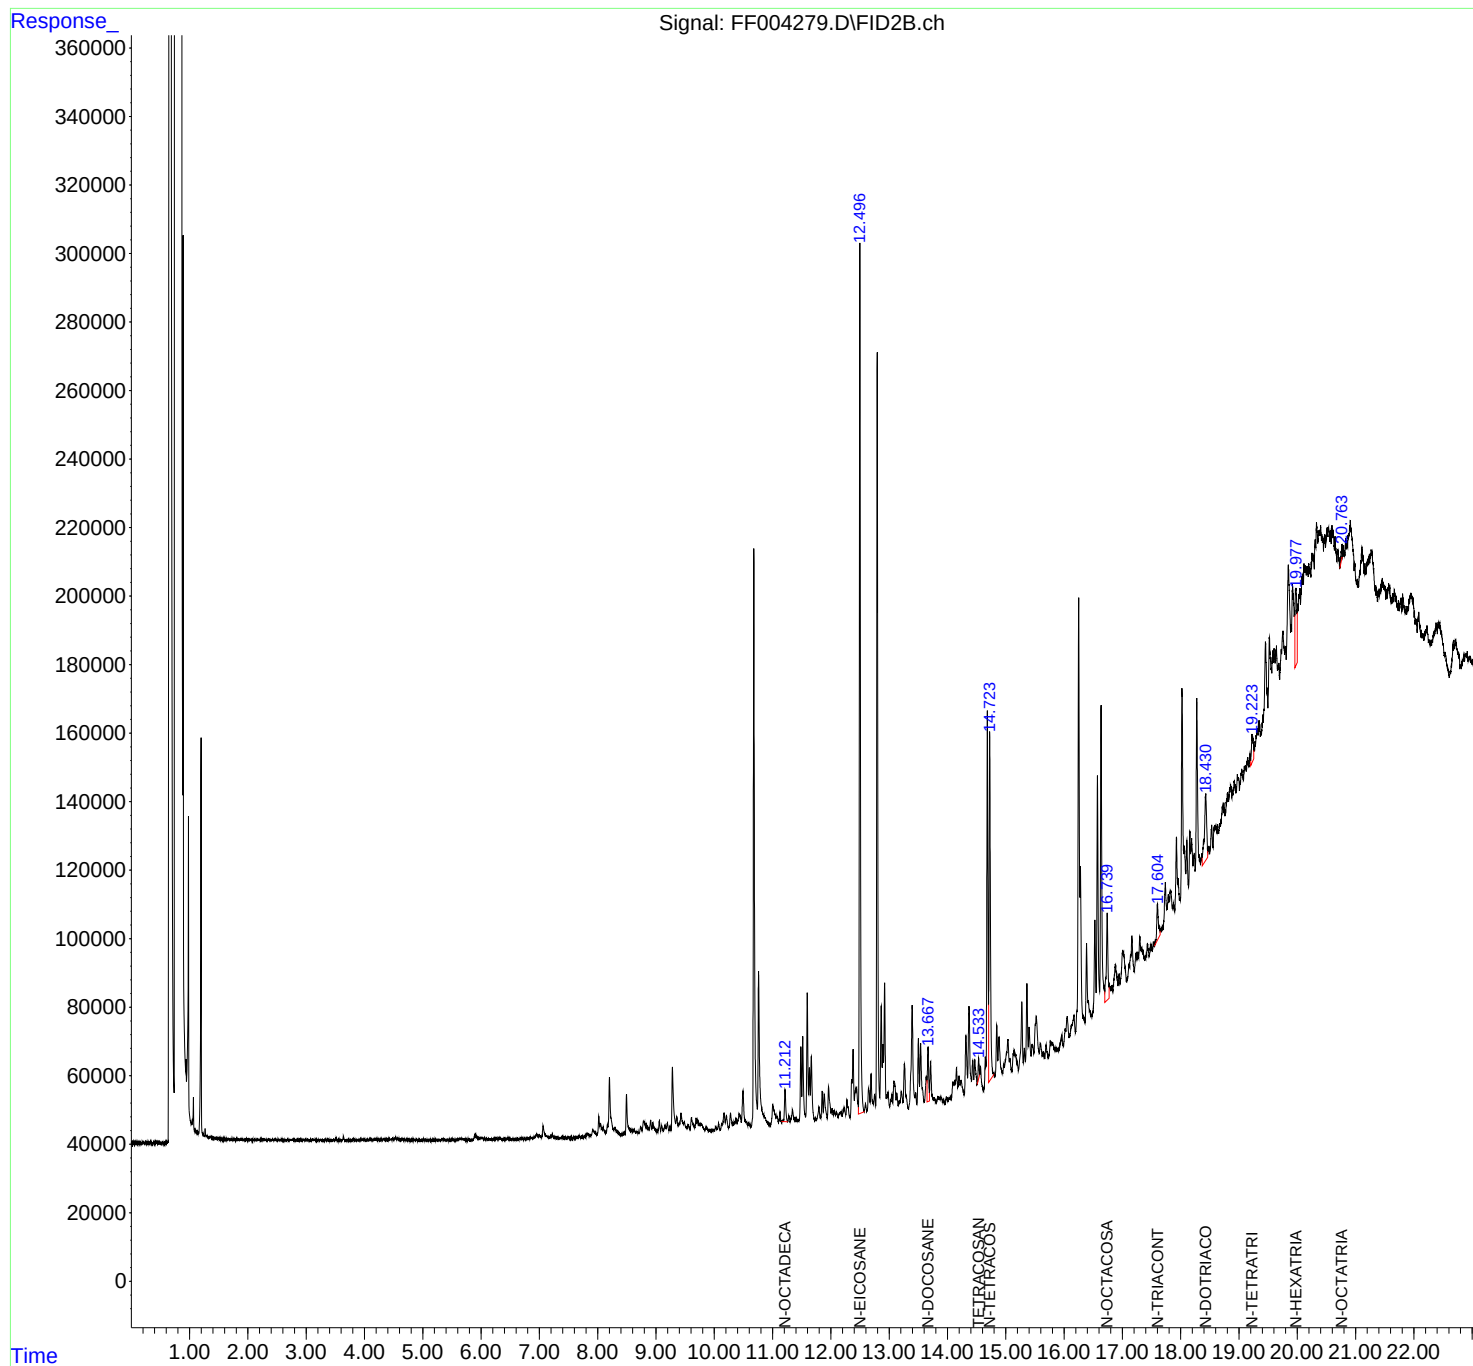

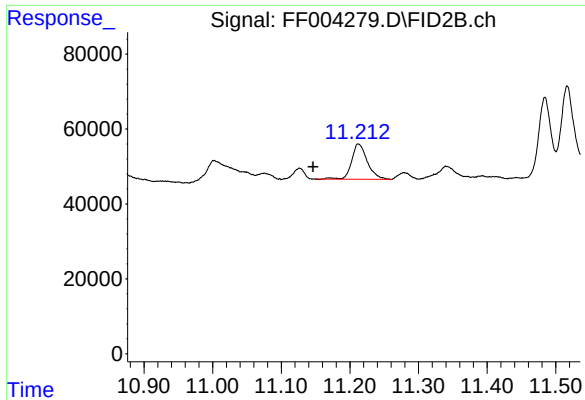


#6 N-OCTADECANE

R.T.: 11.212 min
Delta R.T.: 0.066 min
Response: 150377
Conc: 1.00 ug/ml

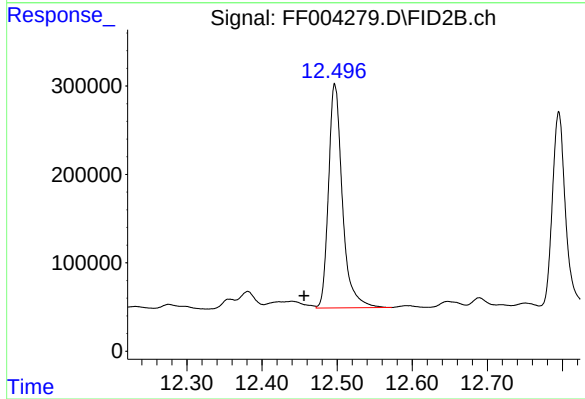


#7 N-EICOSANE

R.T.: 12.497 min
Delta R.T.: 0.041 min
Response: 3253628
Conc: 21.65 ug/ml

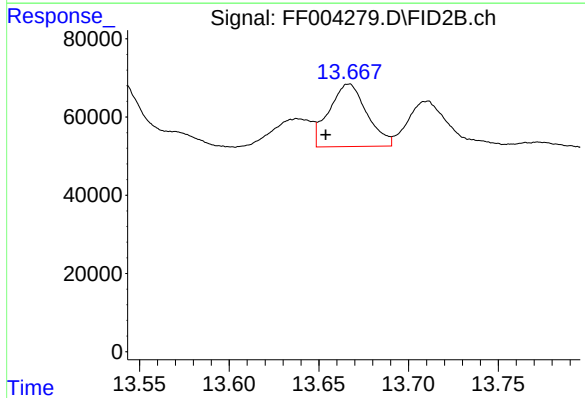


#8 N-DOCOSANE

R.T.: 13.667 min
Delta R.T.: 0.013 min
Response: 234979
Conc: 1.57 ug/ml

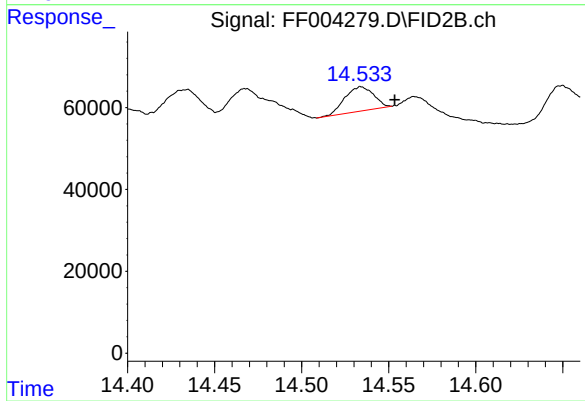


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.534 min
Delta R.T.: -0.019 min
Response: 68141
Conc: 0.52 ug/ml

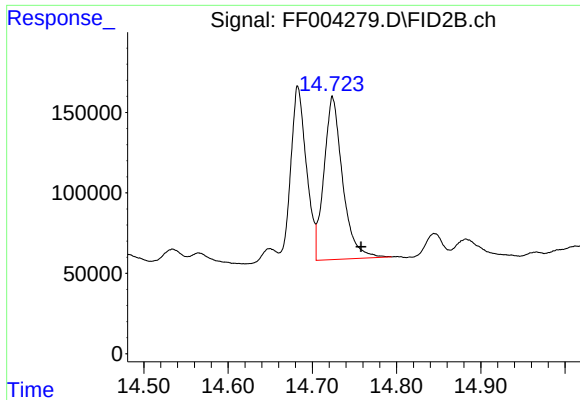


#10 N-TETRACOSANE

R.T.: 14.724 min
Delta R.T.: -0.034 min
Response: 1556440
Conc: 10.57 ug/ml

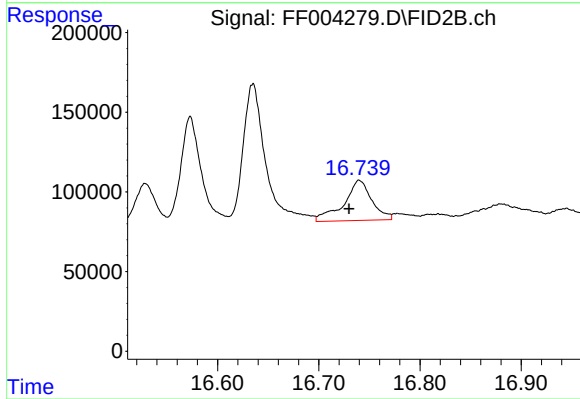


#12 N-OCTACOSANE

R.T.: 16.740 min
Delta R.T.: 0.010 min
Response: 485008
Conc: 3.37 ug/ml

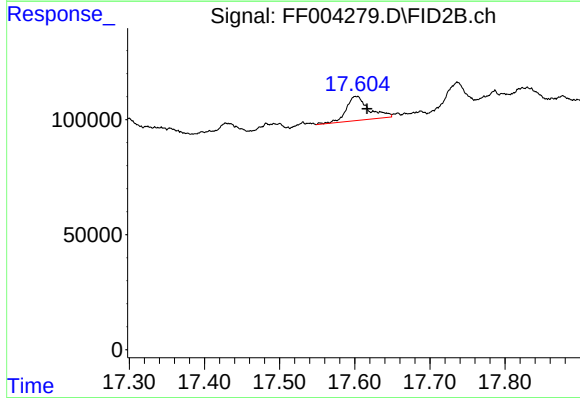


#13 N-TRIACONTANE

R.T.: 17.602 min
Delta R.T.: -0.015 min
Response: 218725
Conc: 1.53 ug/ml

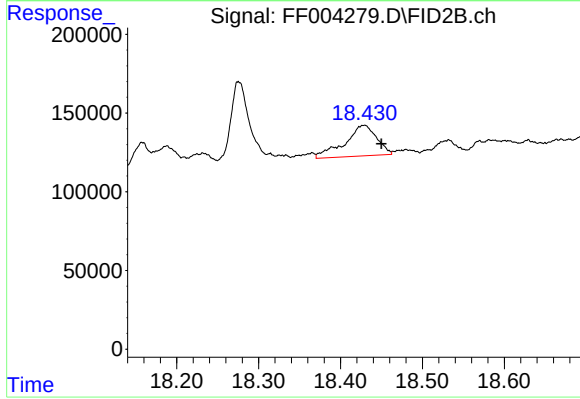


#14 N-DOTRIACONTANE

R.T.: 18.429 min
Delta R.T.: -0.021 min
Response: 525746
Conc: 3.72 ug/ml

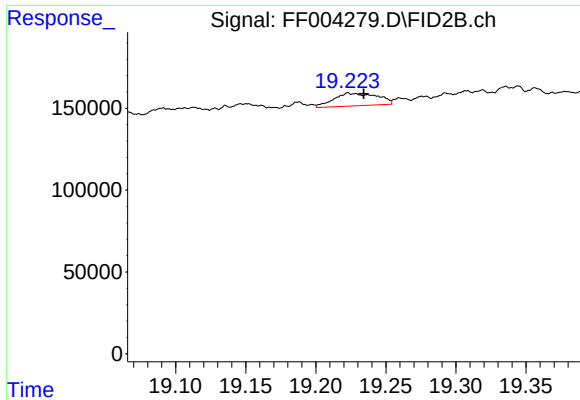


#15 N-TETRATRIACONTANE

R.T.: 19.223 min
Delta R.T.: -0.011 min
Response: 167128
Conc: 1.25 ug/ml

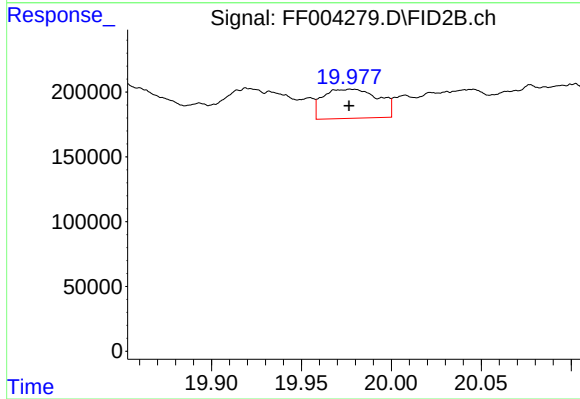

#16 N-HEXATRIACONTANE

R.T.: 19.978 min
Delta R.T.: 0.001 min
Response: 481063
Conc: 3.79 ug/ml

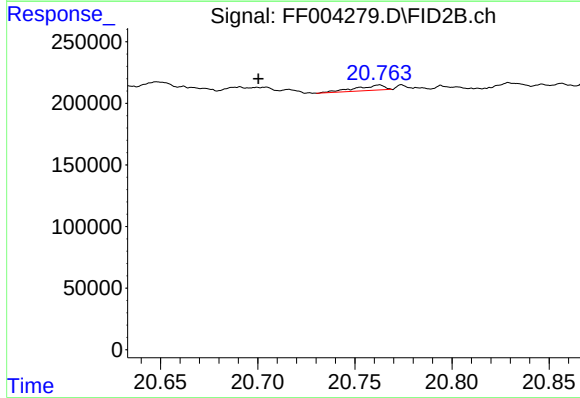

#17 N-OCTATRIACONTANE

R.T.: 20.762 min
Delta R.T.: 0.062 min
Response: 43769
Conc: 0.38 ug/ml