

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041919\
 Data File : FF004281.D
 Signal(s) : FID2B.ch
 Acq On : 19 Apr 2019 20:14
 Operator : AJ\SJ
 Sample : K2202-03 5X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 19 23:22:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
 Quant Title :
 QLast Update : Tue Apr 02 13:45:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.534	330467	2.542 ug/ml
Target Compounds			
5) N-HEXADECANE	9.688	154555	1.044 ug/ml
6) N-OCTADECANE	11.127	138377	0.919 ug/ml
7) N-EICOSANE	12.436	118515	0.789 ug/ml
8) N-DOCOSANE	13.635	76038	0.508 ug/ml
10) N-TETRACOSANE	14.739	183233	1.244 ug/ml
12) N-OCTACOSANE	16.714	165963	1.154 ug/ml
13) N-TRIACONTANE	17.600	209008	1.463 ug/ml
14) N-DOTRIACONTANE	18.436	245742	1.741 ug/ml
15) N-TETRATRIACONTANE	19.228	262535	1.969 ug/ml
16) N-HEXATRIACONTANE	19.973	329267	2.595 ug/ml
17) N-OCTATRIACONTANE	20.641f	117321	1.031 ug/ml
18) N-TETRACONTANE	21.564	70408	0.580 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF041919\
Data File : FF004281.D
Signal(s) : FID2B.ch
Acq On : 19 Apr 2019 20:14
Operator : AJ\SJ
Sample : K2202-03 5X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 19 23:22:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF040219.M
Quant Title :
QLast Update : Tue Apr 02 13:45:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

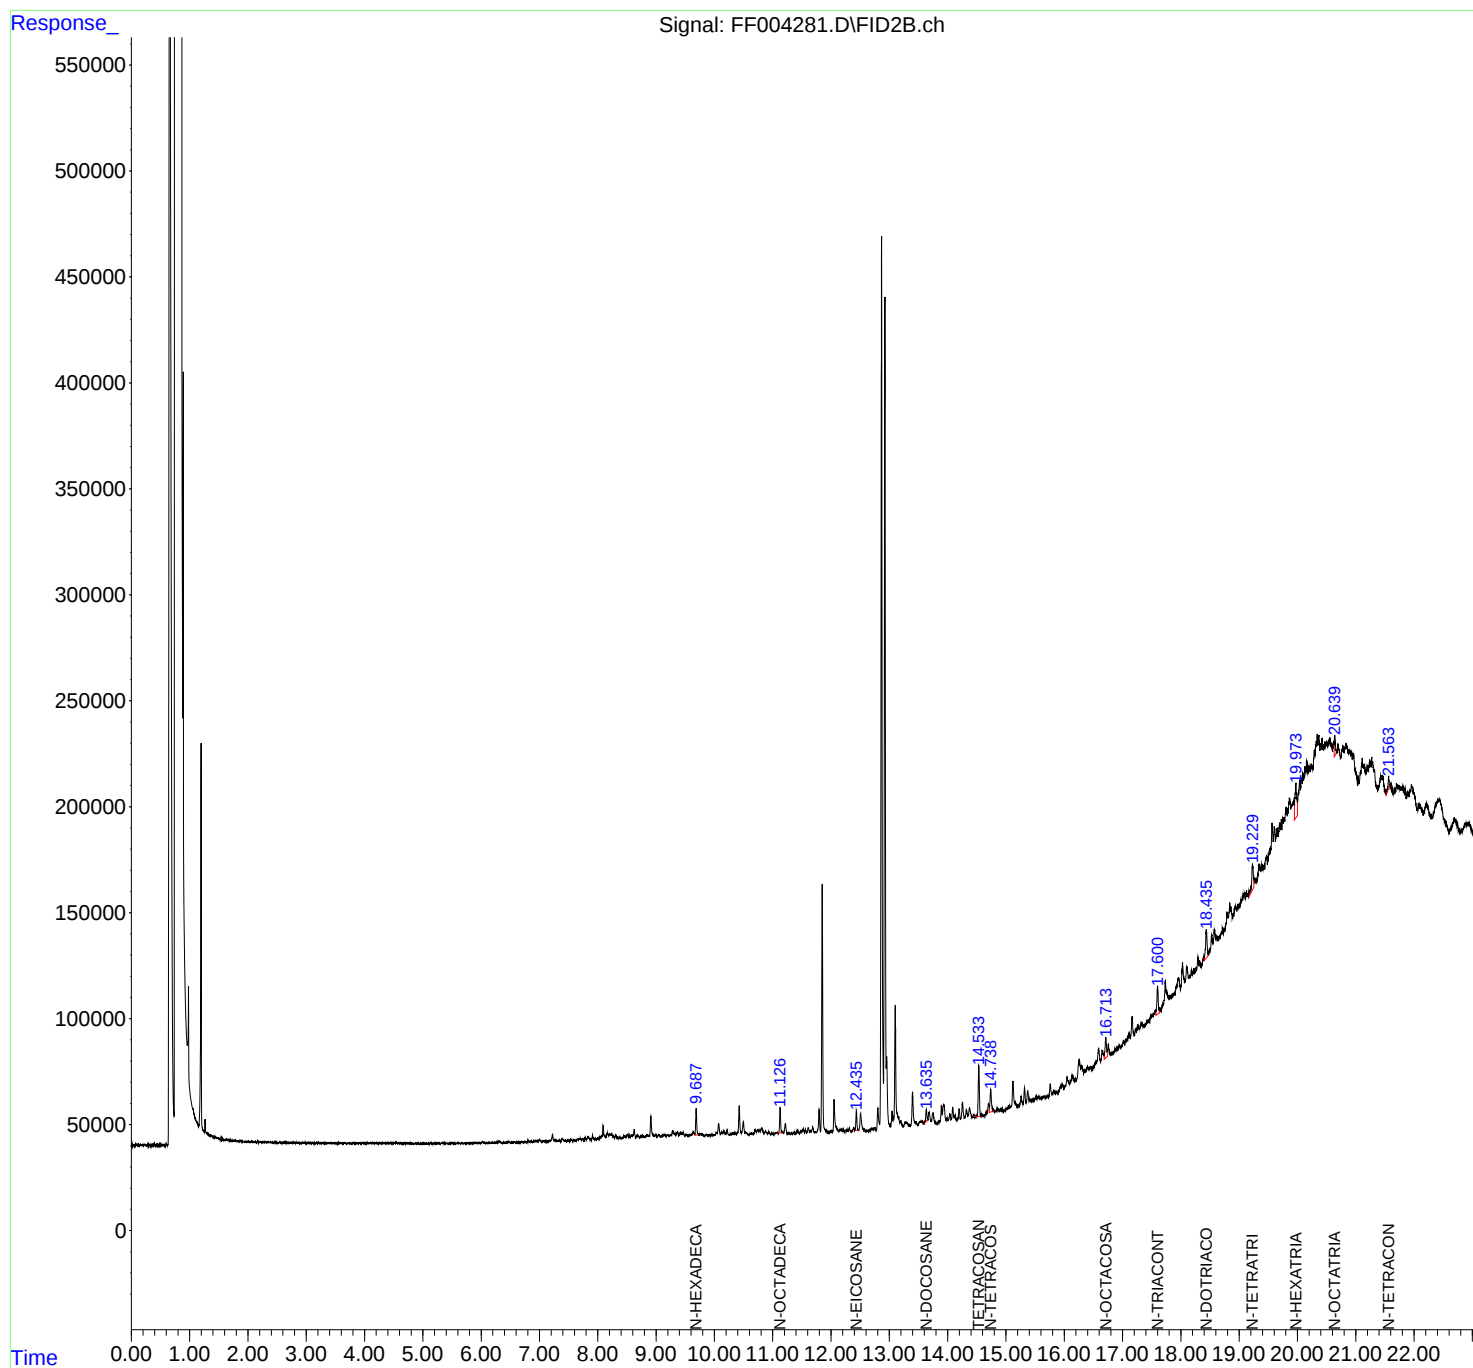

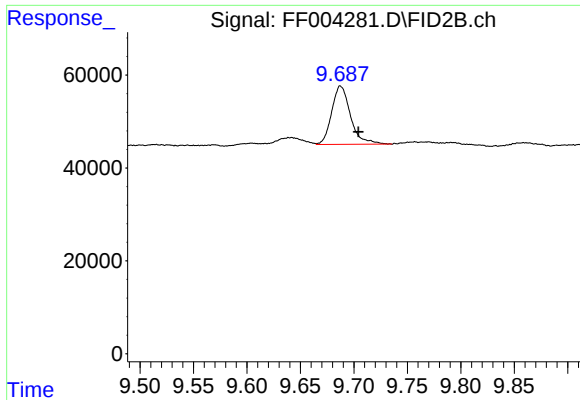


#5 N-HEXADECANE

R.T.: 9.688 min
Delta R.T.: -0.017 min
Response: 154555
Conc: 1.04 ug/ml

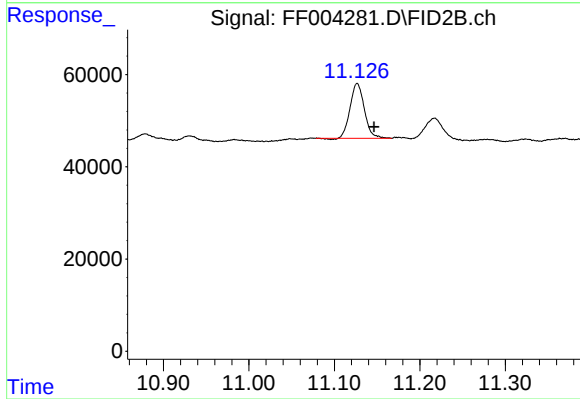


#6 N-OCTADECANE

R.T.: 11.127 min
Delta R.T.: -0.020 min
Response: 138377
Conc: 0.92 ug/ml

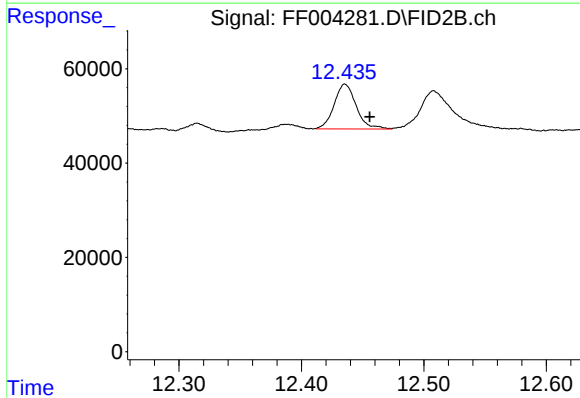


#7 N-EICOSANE

R.T.: 12.436 min
Delta R.T.: -0.020 min
Response: 118515
Conc: 0.79 ug/ml

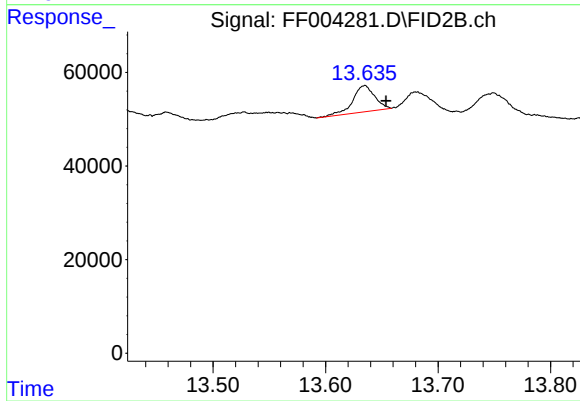


#8 N-DOCOSANE

R.T.: 13.635 min
Delta R.T.: -0.019 min
Response: 76038
Conc: 0.51 ug/ml

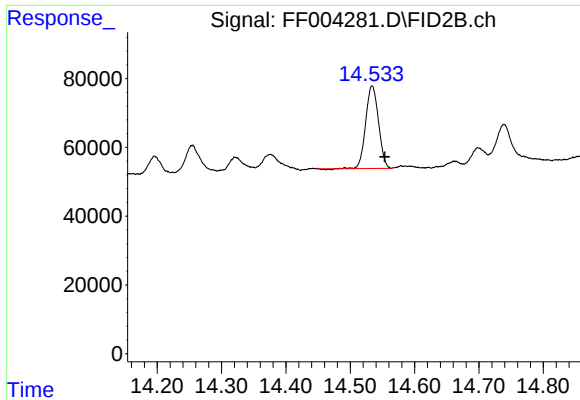


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.534 min
Delta R.T.: -0.019 min
Response: 330467
Conc: 2.54 ug/ml

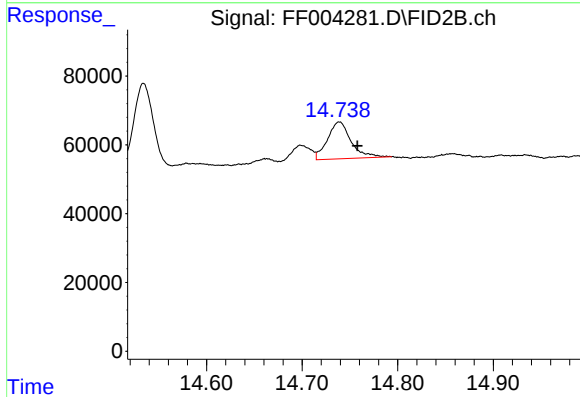


#10 N-TETRACOSANE

R.T.: 14.739 min
Delta R.T.: -0.019 min
Response: 183233
Conc: 1.24 ug/ml

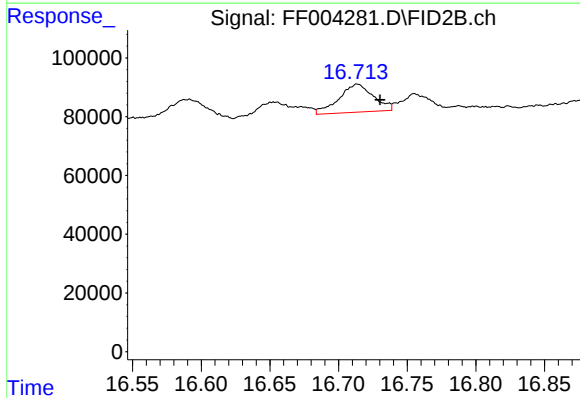


#12 N-OCTACOSANE

R.T.: 16.714 min
Delta R.T.: -0.016 min
Response: 165963
Conc: 1.15 ug/ml

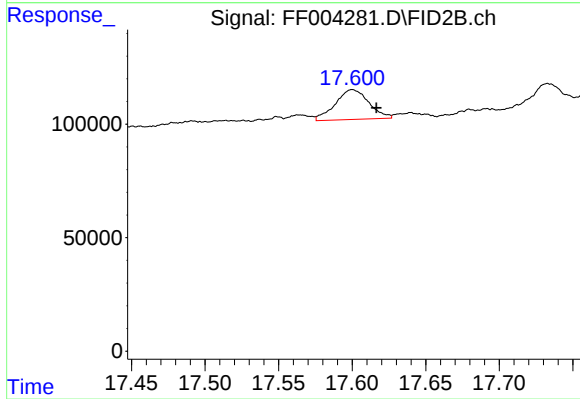


#13 N-TRIACONTANE

R.T.: 17.600 min
Delta R.T.: -0.016 min
Response: 209008
Conc: 1.46 ug/ml

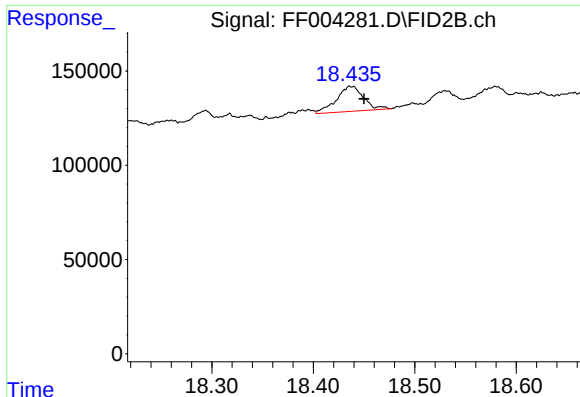


#14 N-DOTRIACONTANE

R.T.: 18.436 min
Delta R.T.: -0.014 min
Response: 245742
Conc: 1.74 ug/ml

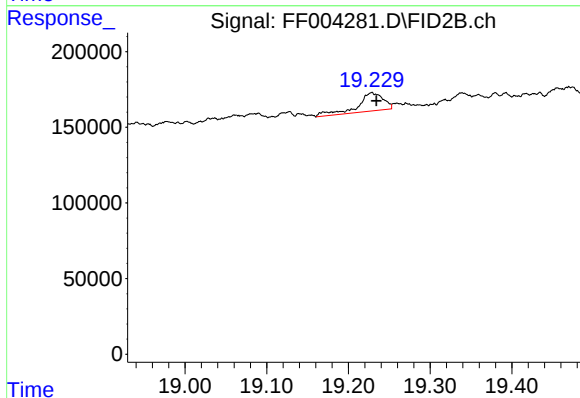


#15 N-TETRATRIACONTANE

R.T.: 19.228 min
Delta R.T.: -0.006 min
Response: 262535
Conc: 1.97 ug/ml

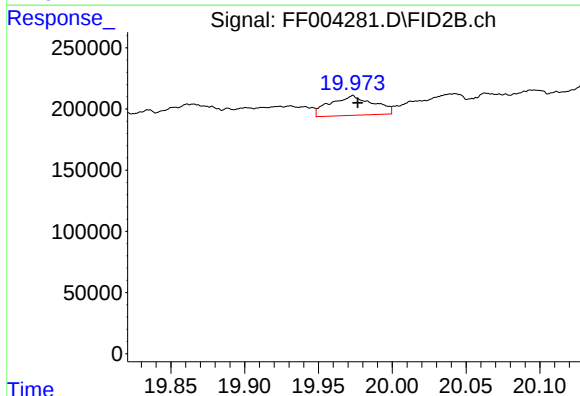


#16 N-HEXATRIACONTANE

R.T.: 19.973 min
Delta R.T.: -0.003 min
Response: 329267
Conc: 2.60 ug/ml

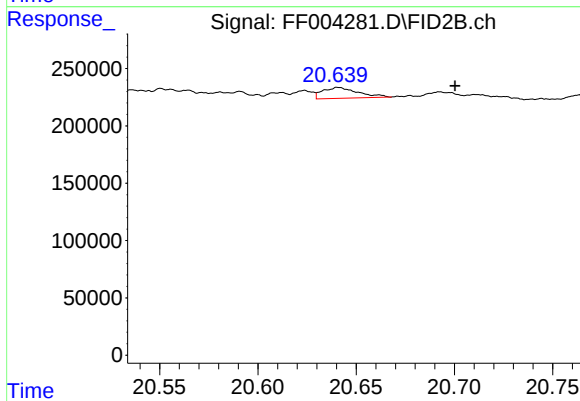

#17 N-OCTATRIACONTANE

R.T.: 20.641 min
Delta R.T.: -0.059 min
Response: 117321
Conc: 1.03 ug/ml

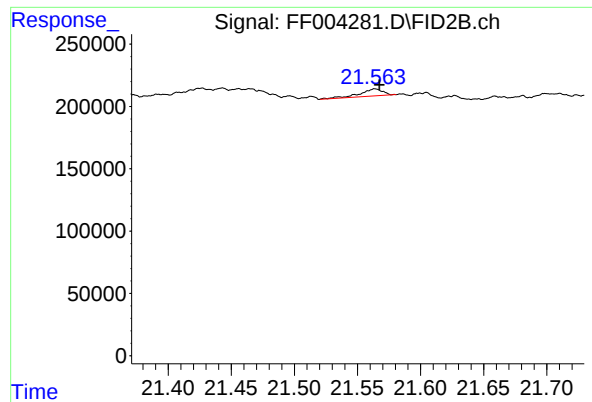

#18 N-TETRACONTANE

R.T.: 21.564 min
Delta R.T.: -0.003 min
Response: 70408
Conc: 0.58 ug/ml